

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042821\
Data File : VW018824.D
Acq On : 28 Apr 2021 16:43
Operator : SY/VA
Sample : M2177-10
Misc : 3.08G/10ML/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG576

Manual Integrations
APPROVED

MMDadoda
4/30/2021 10:48:13 AM

Quant Time: Apr 29 00:16:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 29 00:13:39 2021
Response via : Initial Calibration

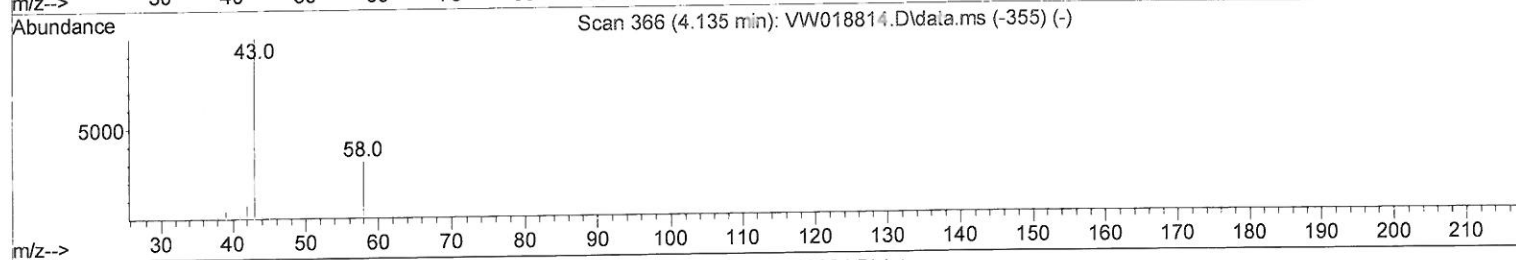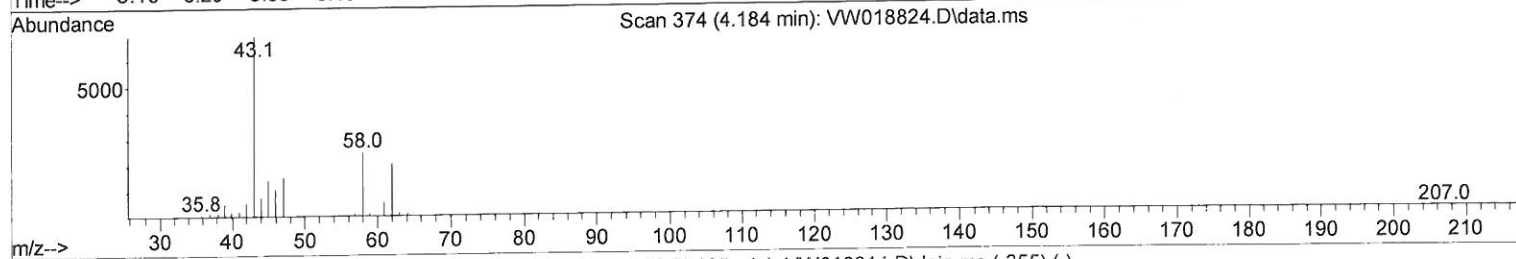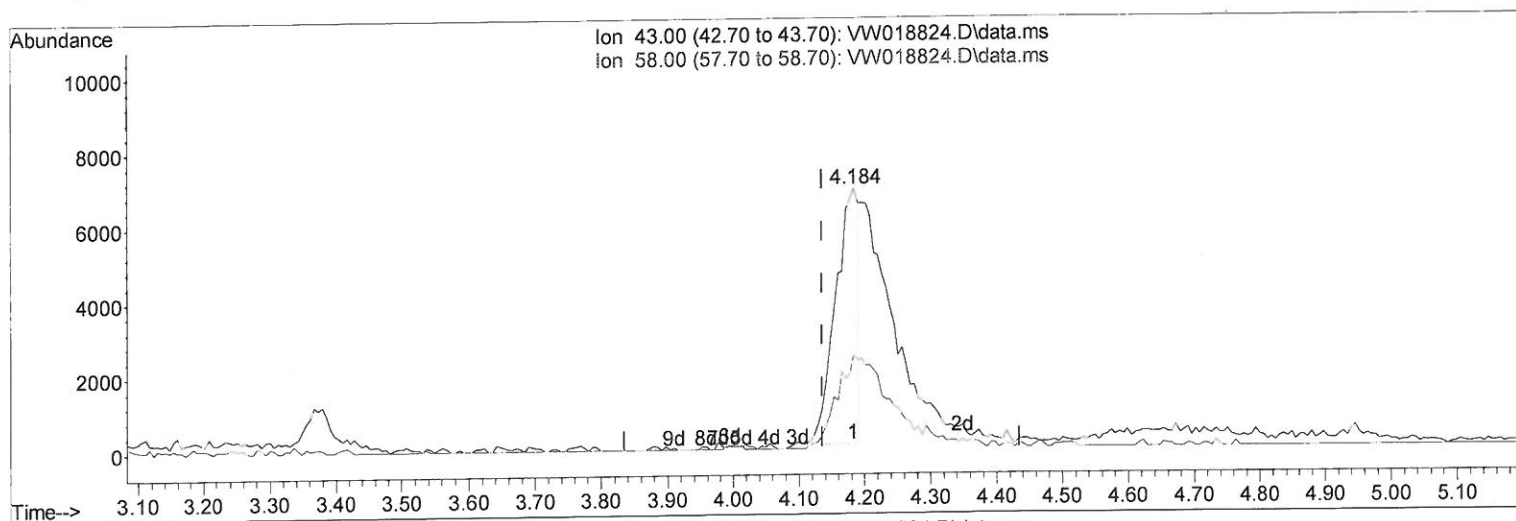

TIC: VW018824.D\data.ms

(13) Acetone (T)

4.184min (+ 0.049) 15.35 ug/L

response 16427

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	23.50
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042821\
 Data File : VW018824.D
 Acq On : 28 Apr 2021 16:43
 Operator : SY/VA
 Sample : M2177-10
 Misc : 3.08G/10ML/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG576

Manual Integrations
 APPROVED

MMDadoda
 4/30/2021 10:48:13 AM

Quant Time: Apr 29 00:16:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 29 00:13:39 2021
 Response via : Initial Calibration

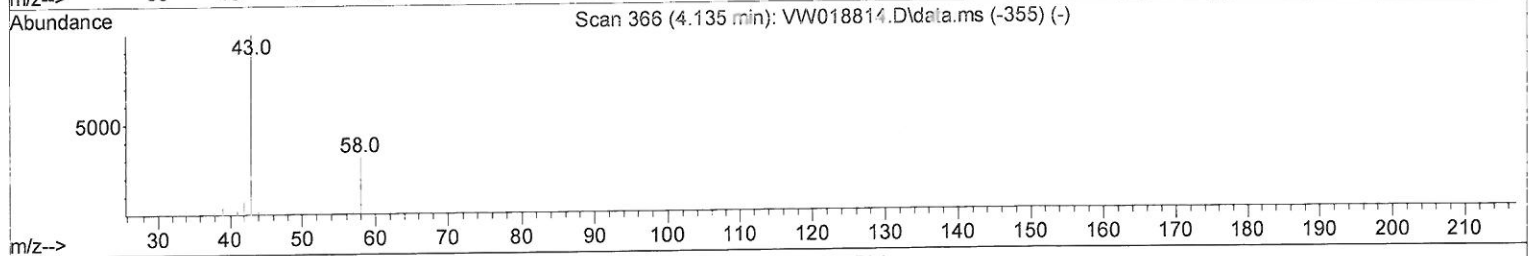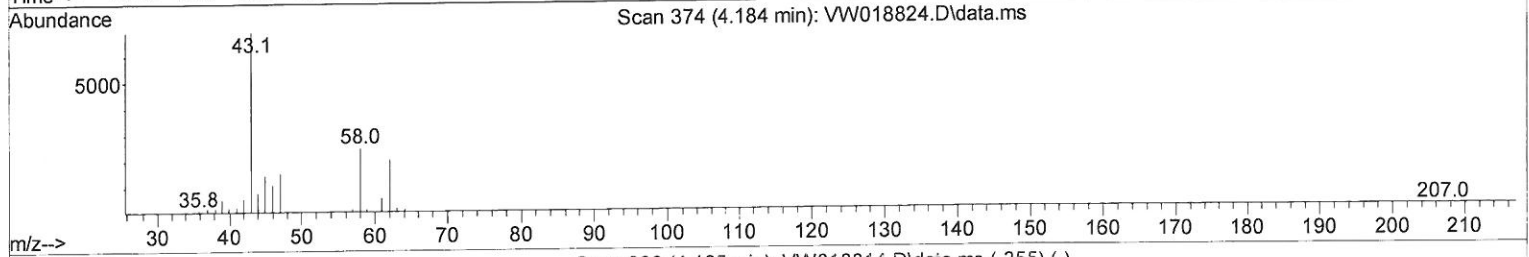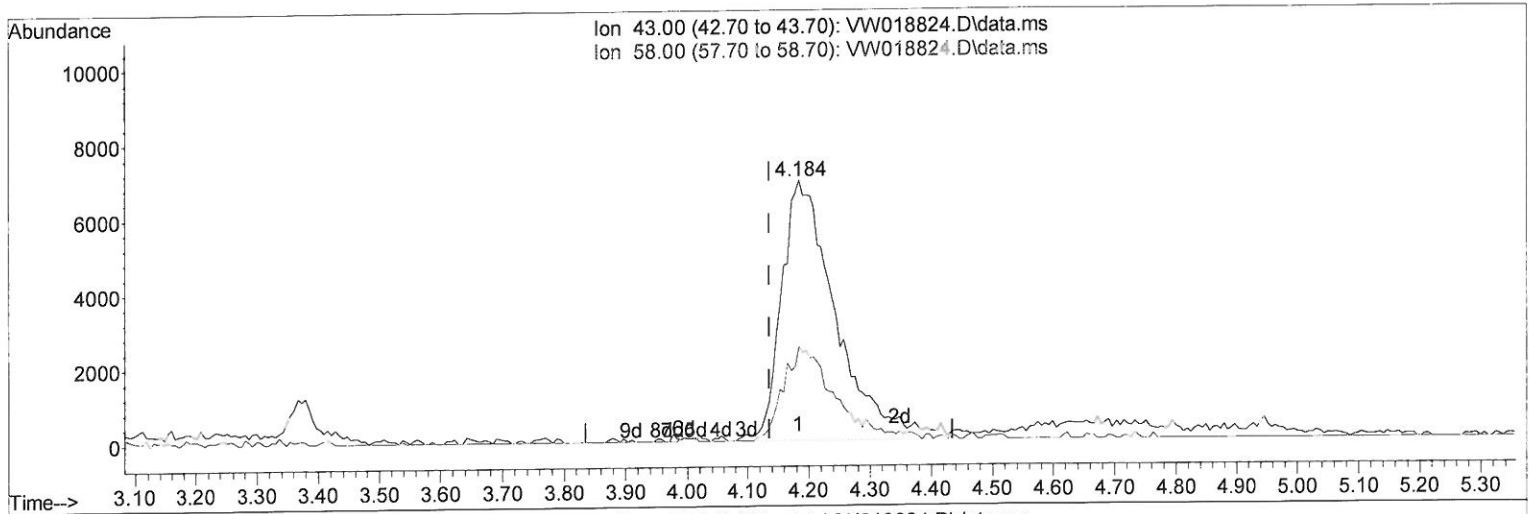

TIC: VW018824.D\data.ms

(13) Acetone (T)

4.184min (+ 0.049) 38.94 ug/L m >04/30/21 by

response 41664

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	9.27
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042821\
Data File : VW018824.D
Acq On : 28 Apr 2021 16:43
Operator : SY/VA
Sample : M2177-10
Misc : 3.08G/10ML/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG576

Manual Integrations
APPROVED

MMDadoda
4/30/2021 10:48:13 AM

Quant Time: Apr 29 00:16:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 29 00:13:39 2021
Response via : Initial Calibration

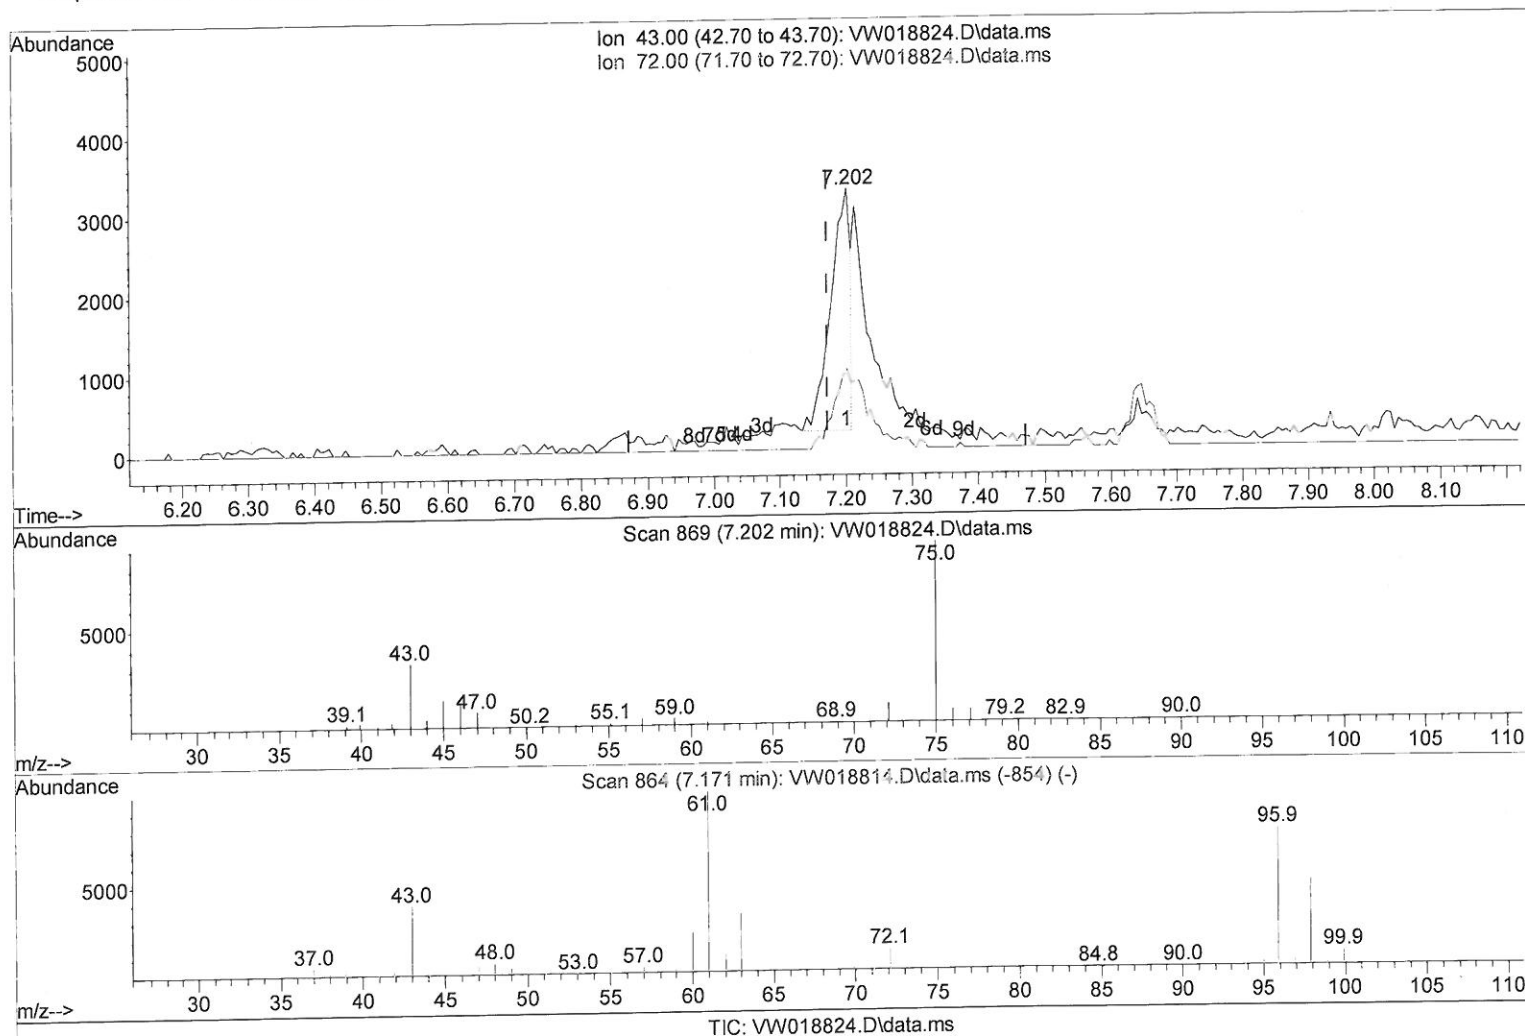

(22) 2-Butanone (T)

7.202min (+ 0.030) 3.83 ug/L

response 6230

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	23.16
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042821\
Data File : VW018824.D
Acq On : 28 Apr 2021 16:43
Operator : SY/VA
Sample : M2177-10
Misc : 3.08G/10ML/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG576

Manual Integrations
APPROVED

MMDadoda
4/30/2021 10:48:13 AM

Quant Time: Apr 29 00:16:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 29 00:13:39 2021
Response via : Initial Calibration

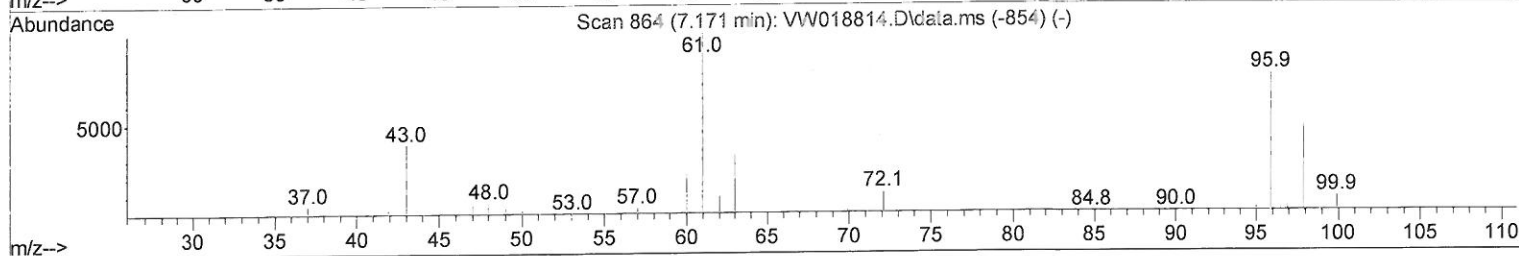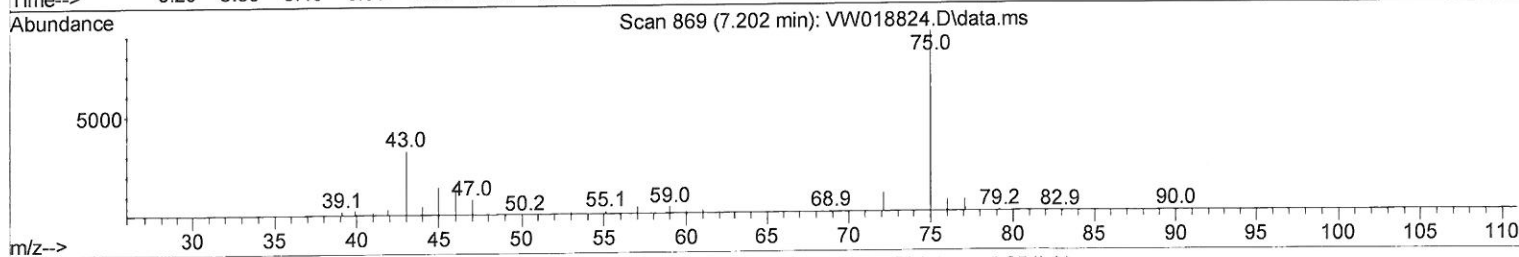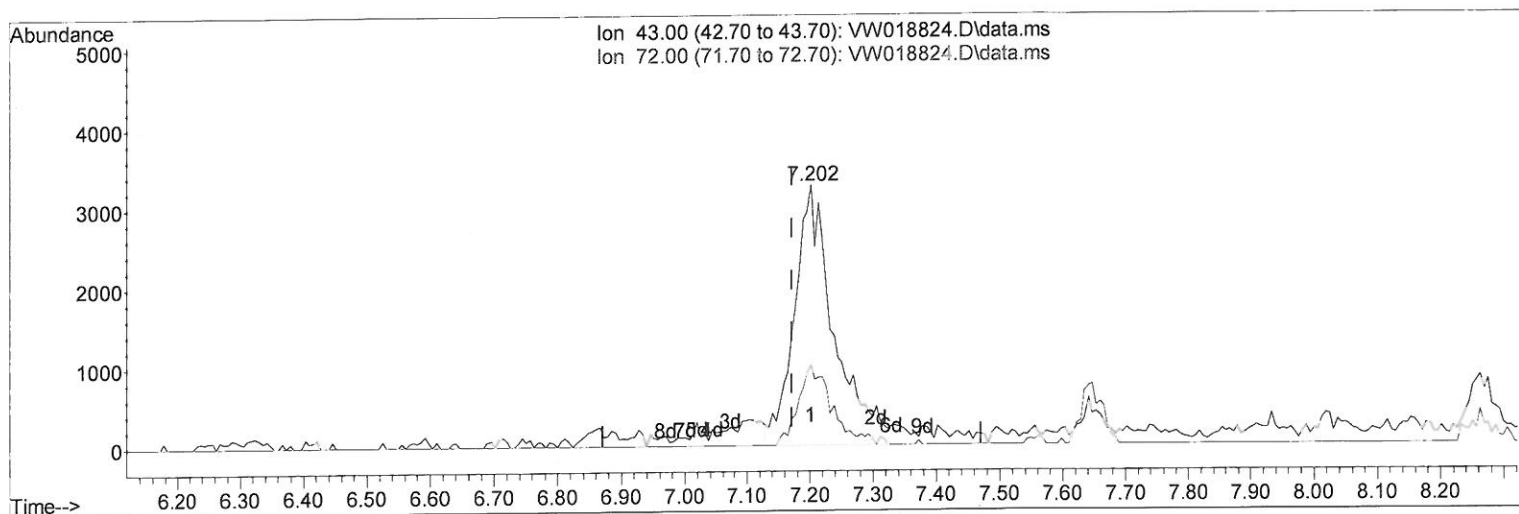

TIC: VW018824.D\data.ms

(22) 2-Butanone (T)

7.202min (+ 0.030) 8.68 ug/L m

response 14120

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	10.22#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042821\
 Data File : VW018824.D
 Acq On : 28 Apr 2021 16:43
 Operator : SY/VA
 Sample : M2177-10
 Misc : 3.08G/10ML/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG576

Manual Integrations
 APPROVED

MMDadoda
 4/30/2021 10:48:13 AM

Quant Time: Apr 29 00:16:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 29 00:13:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	426155	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	321537	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	101912	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	73615	11.37	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	45.48%		
7) Chloroethane-d5	2.885	69	77666	13.53	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	54.12%		
11) 1,1-Dichloroethene-d2	4.007	63	103046	9.16	ug/L	-0.02
Spiked Amount 25.000	Range 45 - 110		Recovery =	36.64%#		
21) 2-Butanone-d5	7.110	46	92098	62.48	ug/L	0.02
Spiked Amount 50.000	Range 20 - 135		Recovery =	124.96%		
24) Chloroform-d	7.647	84	238890	20.43	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	81.72%		
26) 1,2-Dichloroethane-d4	8.305	65	143530	21.83	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.32%		
32) Benzene-d6	8.275	84	392392	20.80	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.20%		
36) 1,2-Dichloropropane-d6	9.274	67	142808	25.12	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	100.48%		
41) Toluene-d8	10.323	98	298935	17.33	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	69.32%		
43) trans-1,3-Dichloroprop...	10.579	79	49920	20.63	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.52%		
47) 2-Hexanone-d5	10.927	63	79656	80.59	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	161.18%#		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	130853	27.56	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	110.24%		
66) 1,2-Dichlorobenzene-d4	13.853	152	79654	22.25	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.00%		
Target Compounds						
13) Acetone	4.184	43	41664m	38.94	ug/L	Qvalue
14) Carbon disulfide	4.373	76	37775	2.27	ug/L	100
16) Methylene chloride	4.909	84	36534	5.23	ug/L	89
22) 2-Butanone	7.202	43	14120m	8.68	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042821\
Data File : VW018824.D
Acq On : 28 Apr 2021 16:43
Operator : SY/VA
Sample : M2177-10
Misc : 3.08G/10ML/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG576

Manual Integrations
APPROVED

MMDadoda
4/30/2021 10:48:13 AM

Quant Time: Apr 29 00:16:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 29 00:13:39 2021
Response via : Initial Calibration

