

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022659.D
 Acq On : 28 Apr 2022 12:37
 Operator : SY/VA
 Sample : N2562-12RE
 Misc : 6.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 29 01:10:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 01:08:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	341591	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	313580	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	136455	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	71505	9.469	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	37.880%
7) Chloroethane-d5	2.885	69	60379	12.758	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	51.040%
11) 1,1-Dichloroethene-d2	4.019	63	84569	8.634	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	34.520%#
21) 2-Butanone-d5	7.080	46	64436	48.874	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.740%
24) Chloroform-d	7.653	84	181642	17.012	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	68.040%
26) 1,2-Dichloroethane-d4	8.396	65	159	0.026	ug/L	0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.274	84	307713	16.061	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	64.240%
36) 1,2-Dichloropropane-d6	9.274	67	103120	18.599	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.400%
41) Toluene-d8	10.323	98	271586	14.474	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	57.880%
43) trans-1,3-Dichloroprop...	10.579	79	38641	14.768	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	59.080%
47) 2-Hexanone-d5	10.920	63	51954	50.366	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.740%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	110018	23.338	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	93808	19.409	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	77.640%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	21117	4.108	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022659.D
Acq On : 28 Apr 2022 12:37
Operator : SY/VA
Sample : N2562-12RE
Misc : 6.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Apr 29 01:10:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 01:08:57 2022
Response via : Initial Calibration

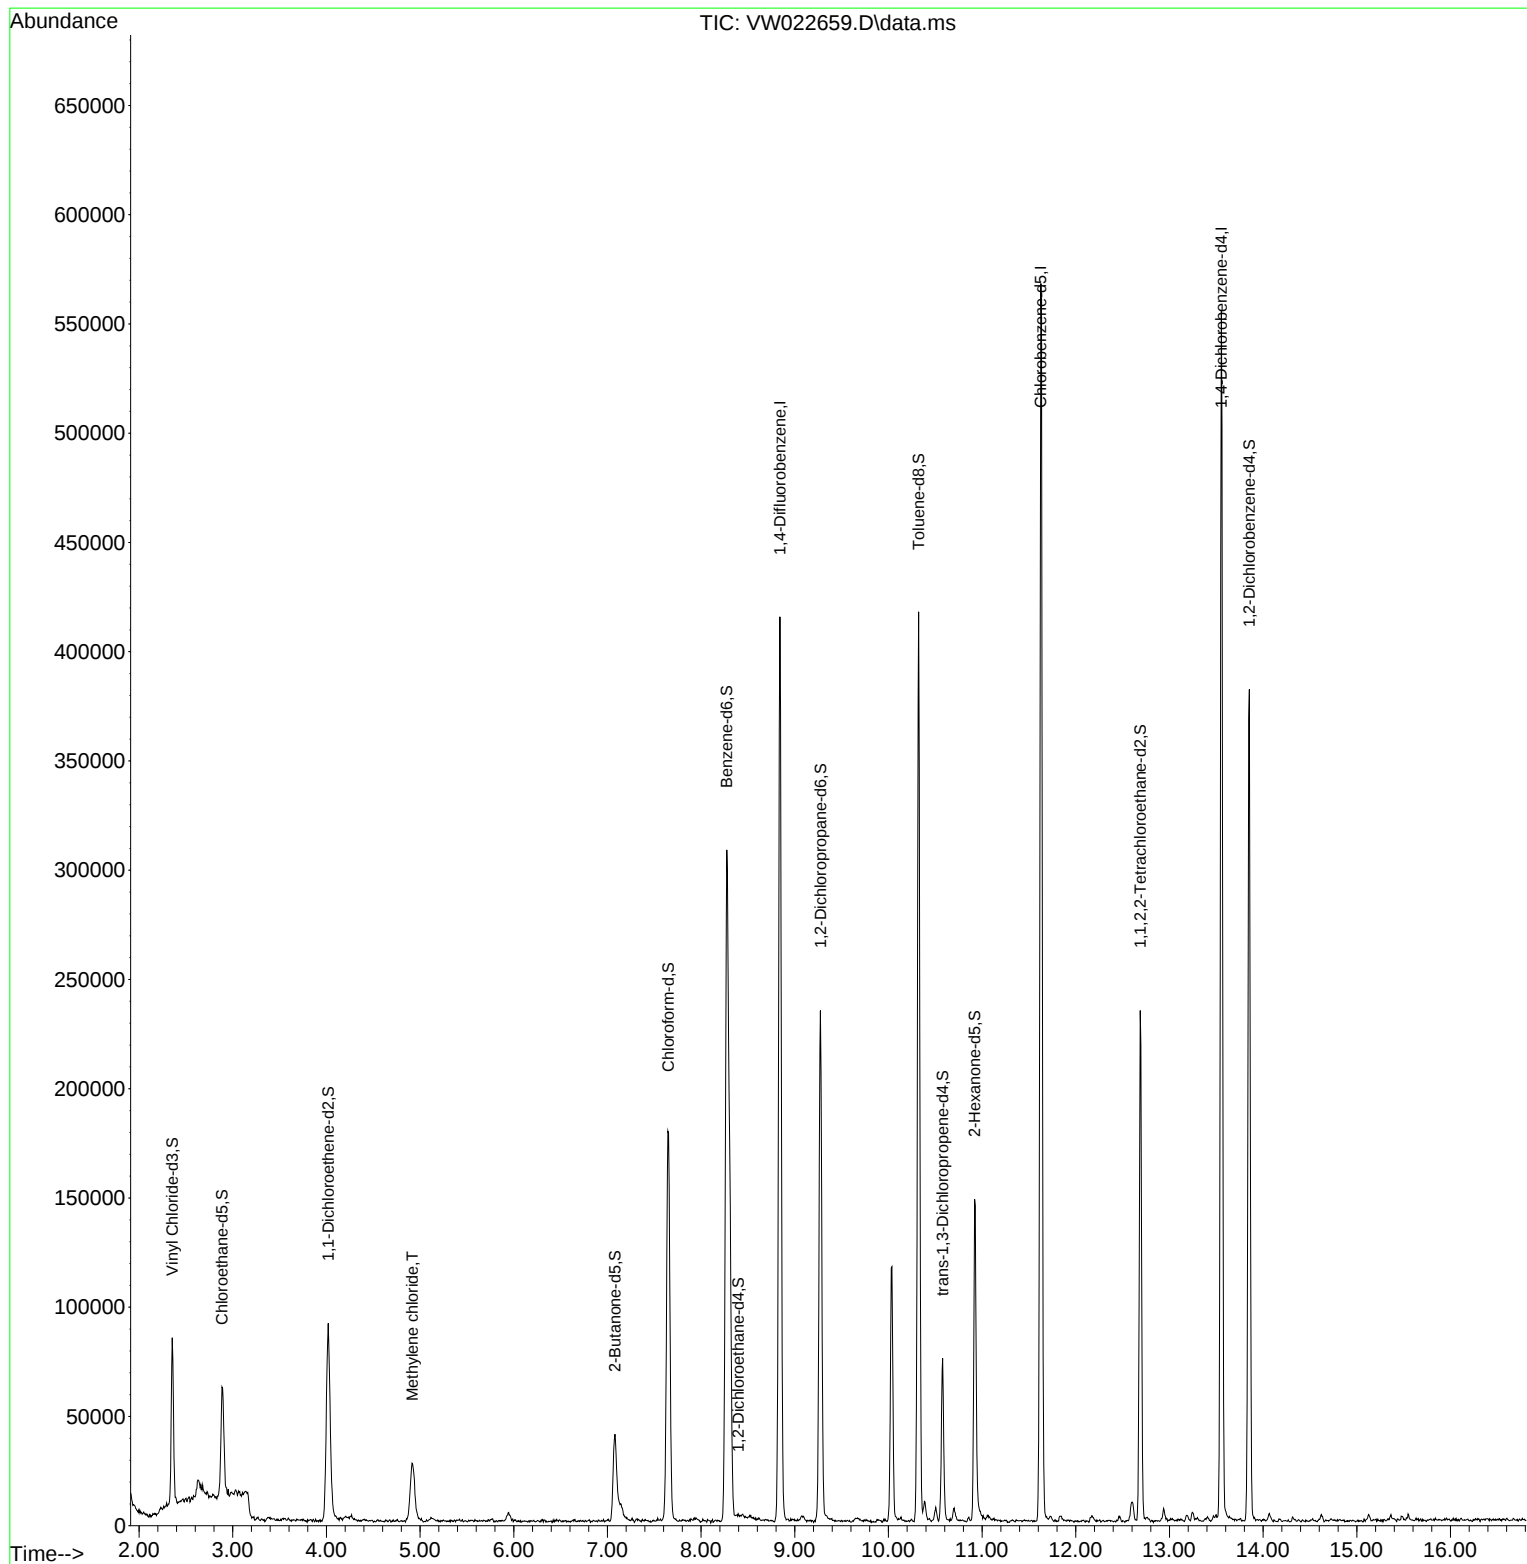

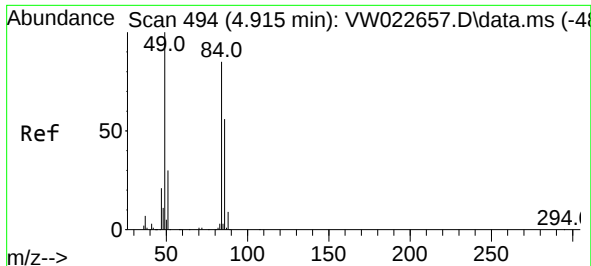

#16
Methylene chloride
Concen: 4.108 ug/L
RT: 4.915 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW022659.D
Acq: 28 Apr 2022 12:37

Instrument :
MSVOA_W
ClientSampleId :

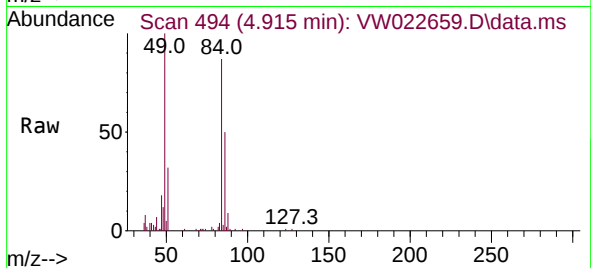

Tgt Ion: 84 Resp: 21117

Ion	Ratio	Lower	Upper
84	100		
86	56.8	42.8	79.4
49	114.6	94.2	175.0

