

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022675.D
 Acq On : 28 Apr 2022 21:10
 Operator : SY/VA
 Sample : N2603-02
 Misc : 6.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 29 02:21:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	247186	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	226755	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	99928	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	61483	11.251	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	45.000%
7) Chloroethane-d5	2.885	69	52672	15.380	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.520%
11) 1,1-Dichloroethene-d2	4.013	63	66979	9.450	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	37.800%#
21) 2-Butanone-d5	7.074	46	60544	63.461	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.920%
24) Chloroform-d	7.647	84	155229	20.091	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.360%
26) 1,2-Dichloroethane-d4	8.153	65	97	0.022	ug/L	-0.15
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.275	84	254771	18.390	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.560%
36) 1,2-Dichloropropane-d6	9.274	67	89117	22.228	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.920%
41) Toluene-d8	10.323	98	216390	15.948	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	63.800%
43) trans-1,3-Dichloroprop...	10.579	79	30982	16.374	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.480%
47) 2-Hexanone-d5	10.920	63	46947	62.939	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.880%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	105657	30.994	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	123.960%#
66) 1,2-Dichlorobenzene-d4	13.853	152	78601	22.207	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.840%
Target Compounds						
					Qvalue	
48) 2-Hexanone	10.920	43	9028	5.685	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022675.D
Acq On : 28 Apr 2022 21:10
Operator : SY/VA
Sample : N2603-02
Misc : 6.77g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Apr 29 02:21:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 02:06:41 2022
Response via : Initial Calibration

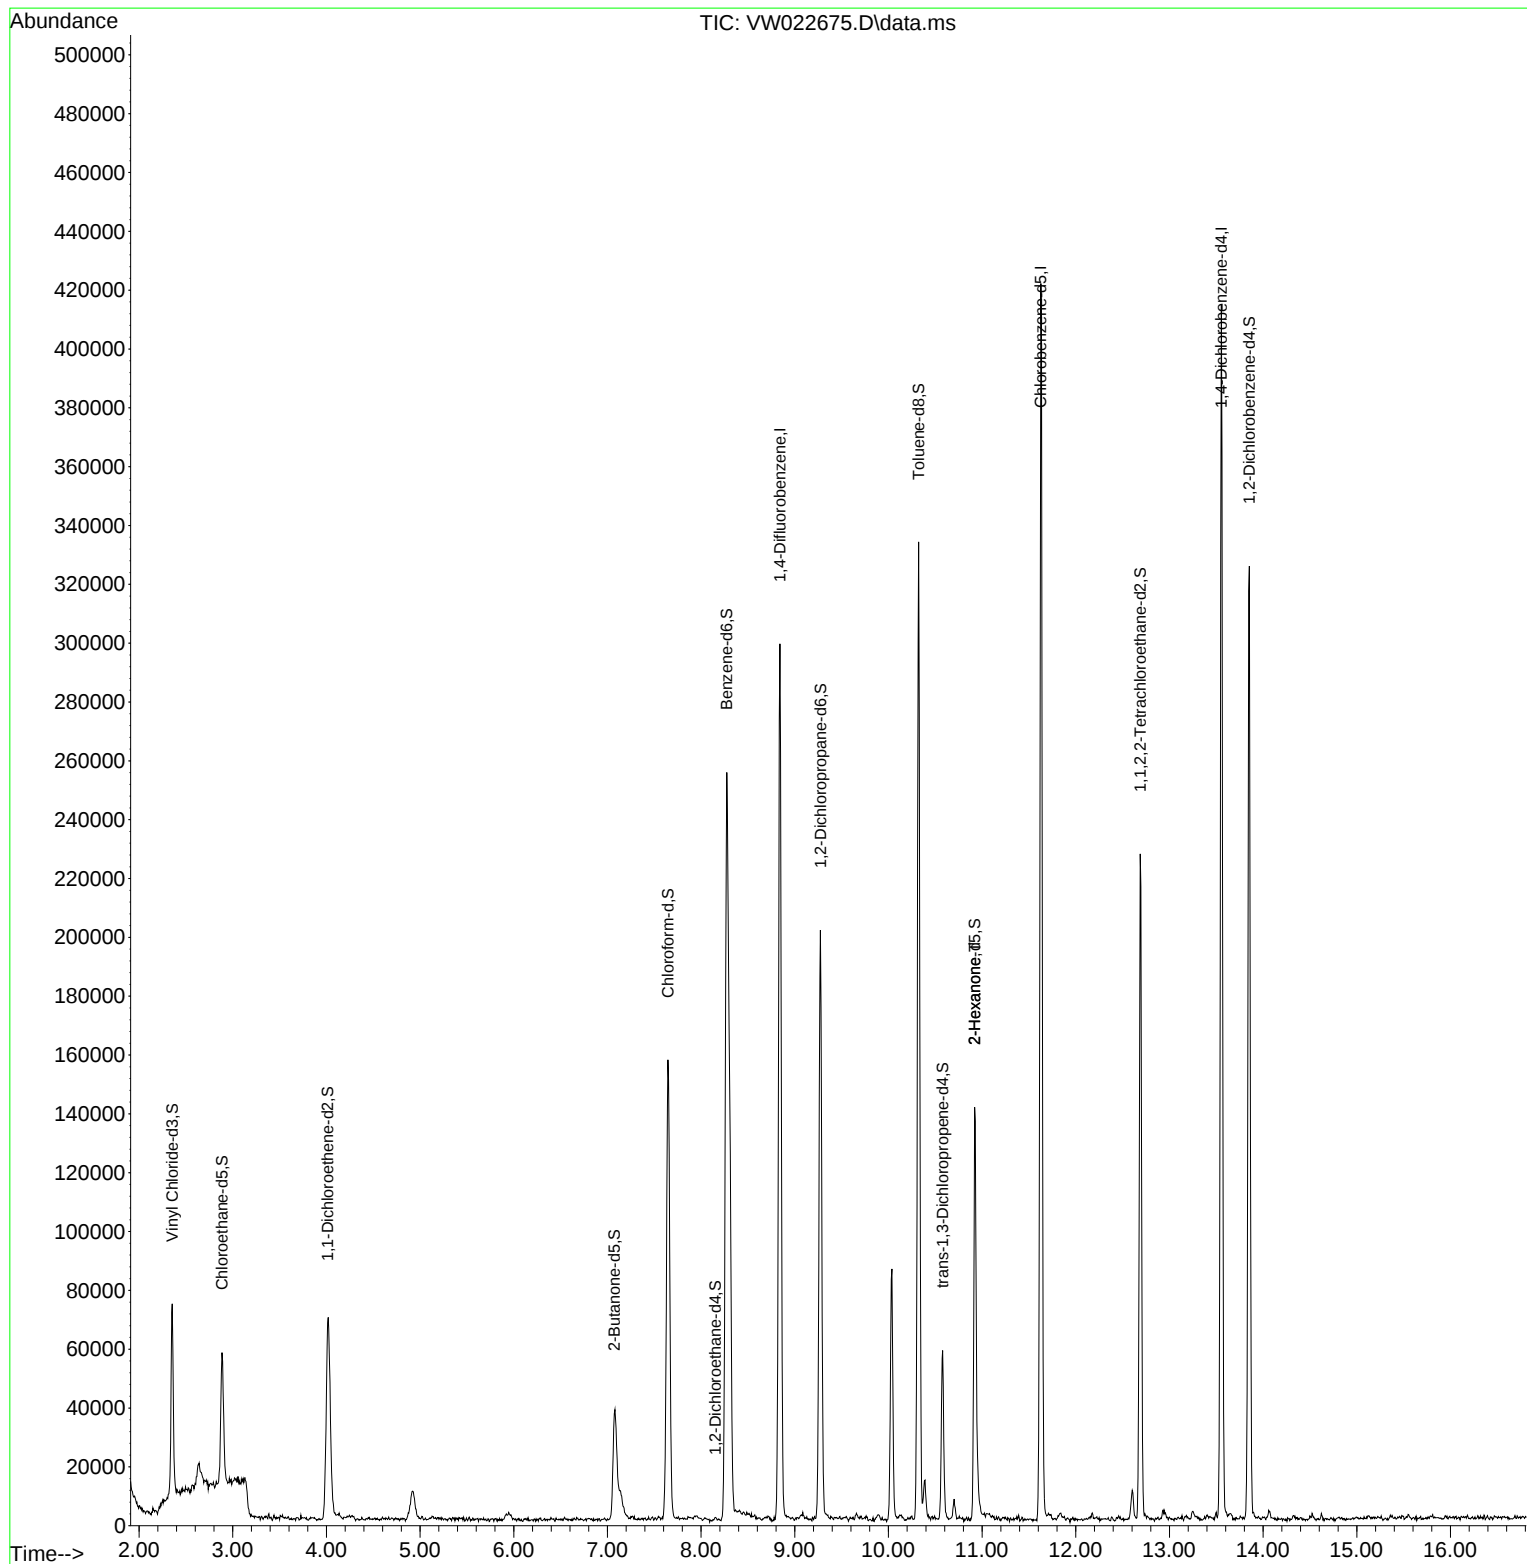

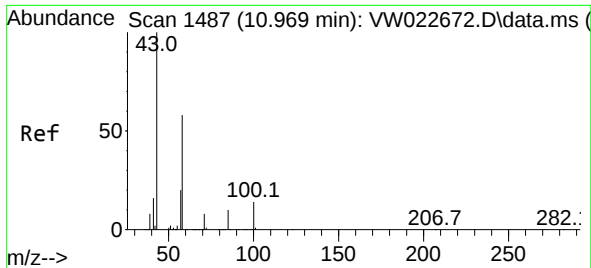

#48
 2-Hexanone
 Concen: 5.685 ug/L
 RT: 10.920 min Scan# 14
 Delta R.T. -0.049 min
 Lab File: VW022675.D
 Acq: 28 Apr 2022 21:10

Instrument :
 MSVOA_W
 ClientSampleId :

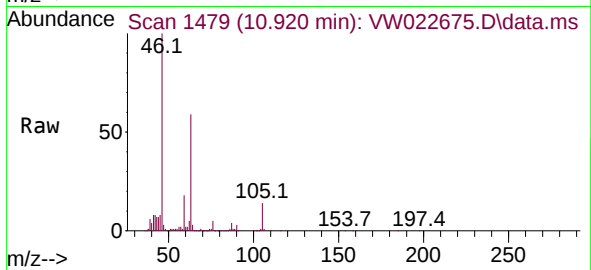

Tgt Ion: 43	Resp:	9028
Ion	Ratio	Lower Upper
43	100	
58	18.1	41.6 62.4#
57	18.2	14.5 21.7
100	1.3	9.3 13.9#

