

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022682.D
 Acq On : 28 Apr 2022 23:58
 Operator : SY/VA
 Sample : N2603-04RE
 Misc : 5.63g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 29 02:22:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	221398	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	160692	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	40921	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	61209	12.506	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.040%
7) Chloroethane-d5	2.892	69	55910	18.227	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.920%
11) 1,1-Dichloroethene-d2	4.013	63	65228	10.275	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	41.120%#
21) 2-Butanone-d5	7.080	46	33693	39.430	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.860%
24) Chloroform-d	7.647	84	152451	22.030	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.120%
26) 1,2-Dichloroethane-d4	8.305	65	90157	22.802	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.200%
32) Benzene-d6	8.275	84	229786	23.405	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.640%
36) 1,2-Dichloropropane-d6	9.275	67	82729	29.118	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	116.480%
41) Toluene-d8	10.323	98	169233	17.600	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.400%
43) trans-1,3-Dichloroprop...	10.579	79	20240	15.095	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	60.360%
47) 2-Hexanone-d5	10.927	63	23892	45.199	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.400%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	75671	31.324	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	125.280%#
66) 1,2-Dichlorobenzene-d4	13.853	152	30551	21.078	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.320%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	2083	0.502	ug/L #	63
48) 2-Hexanone	10.921	43	4747	4.218	ug/L #	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022682.D
Acq On : 28 Apr 2022 23:58
Operator : SY/VA
Sample : N2603-04RE
Misc : 5.63g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Apr 29 02:22:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 02:06:41 2022
Response via : Initial Calibration

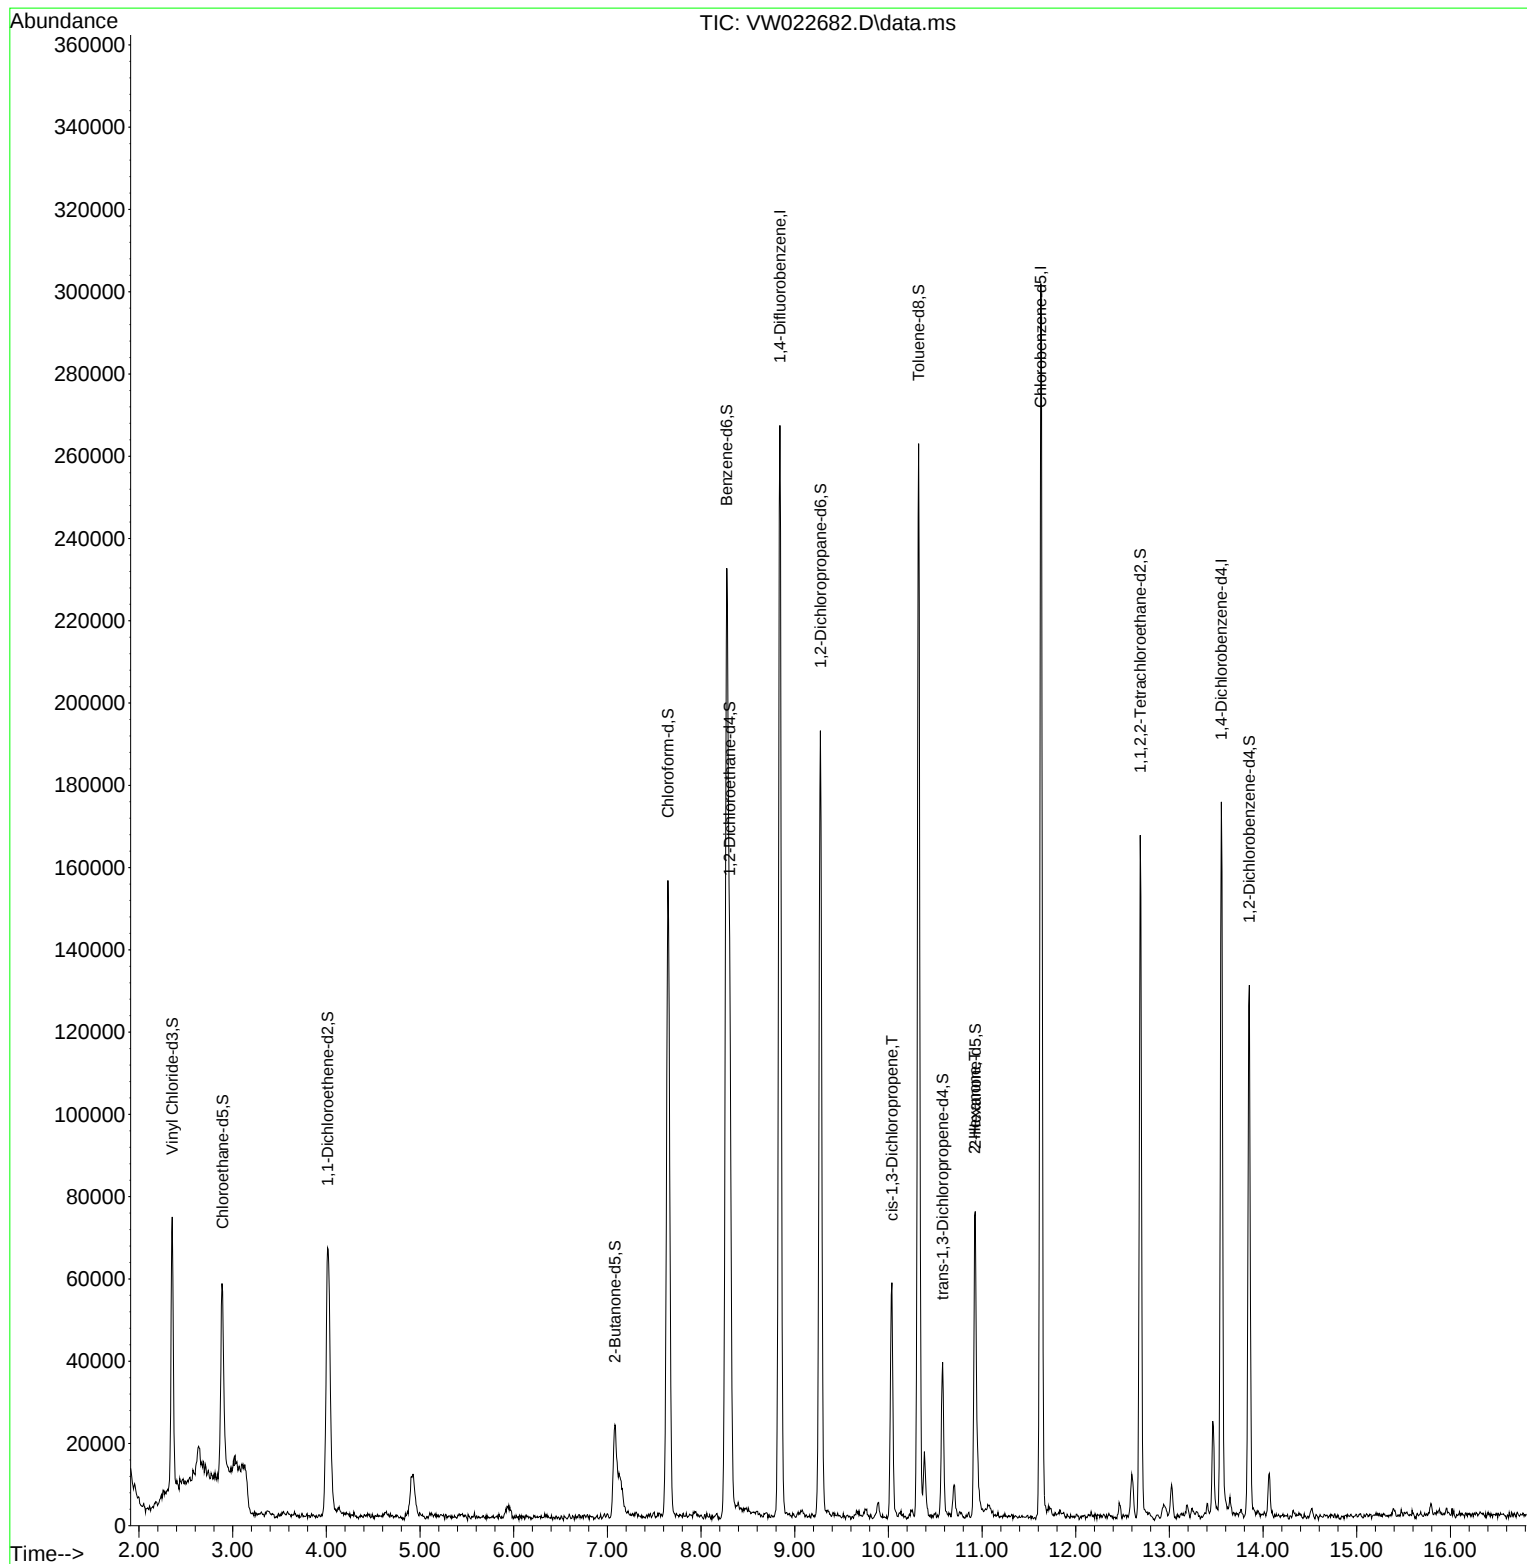

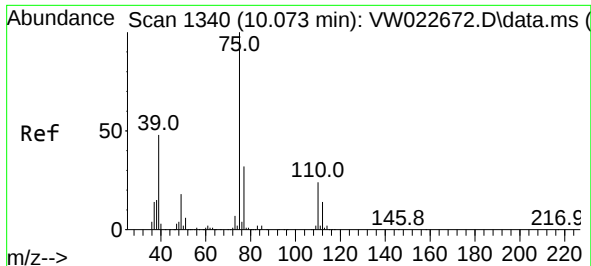

#39

cis-1,3-Dichloropropene

Concen: 0.502 ug/L

RT: 10.037 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW022682.D

Acq: 28 Apr 2022 23:58

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 75 Resp: 2083

Ion Ratio Lower Upper

75 100

77 53.2 22.6 42.0#

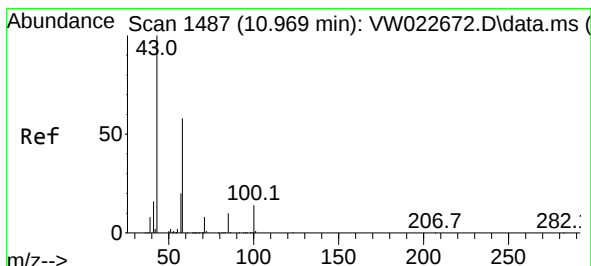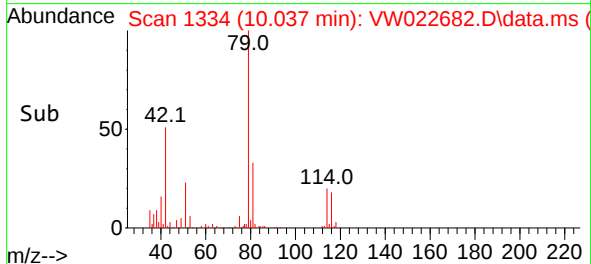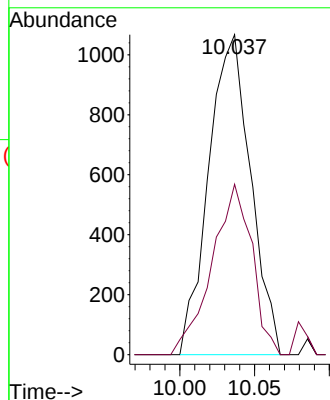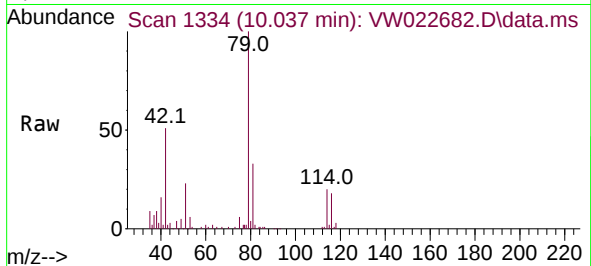

#48

2-Hexanone

Concen: 4.218 ug/L

RT: 10.921 min Scan# 1479

Delta R.T. -0.049 min

Lab File: VW022682.D

Acq: 28 Apr 2022 23:58

Tgt Ion: 43 Resp: 4747

Ion Ratio Lower Upper

43 100

58 9.0 41.6 62.4#

57 25.8 14.5 21.7#

100 1.6 9.3 13.9#

