




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022665.D
Acq On : 28 Apr 2022 15:02
Operator : SY/VA
Sample : N2562-15RE
Misc : 5.50g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW476RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 01:11:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 01:08:57 2022
Response via : Initial Calibration

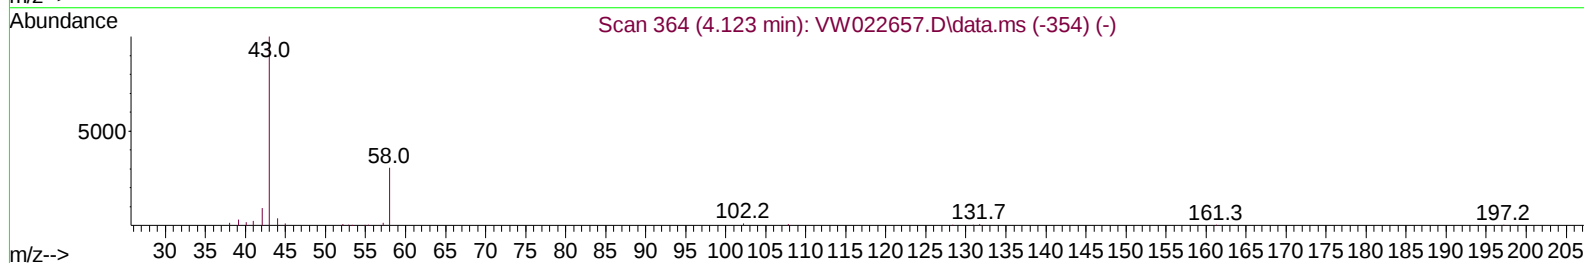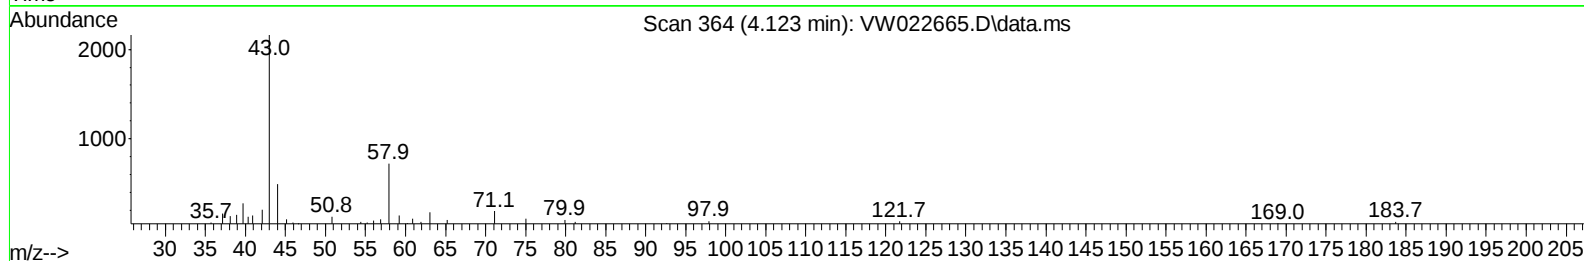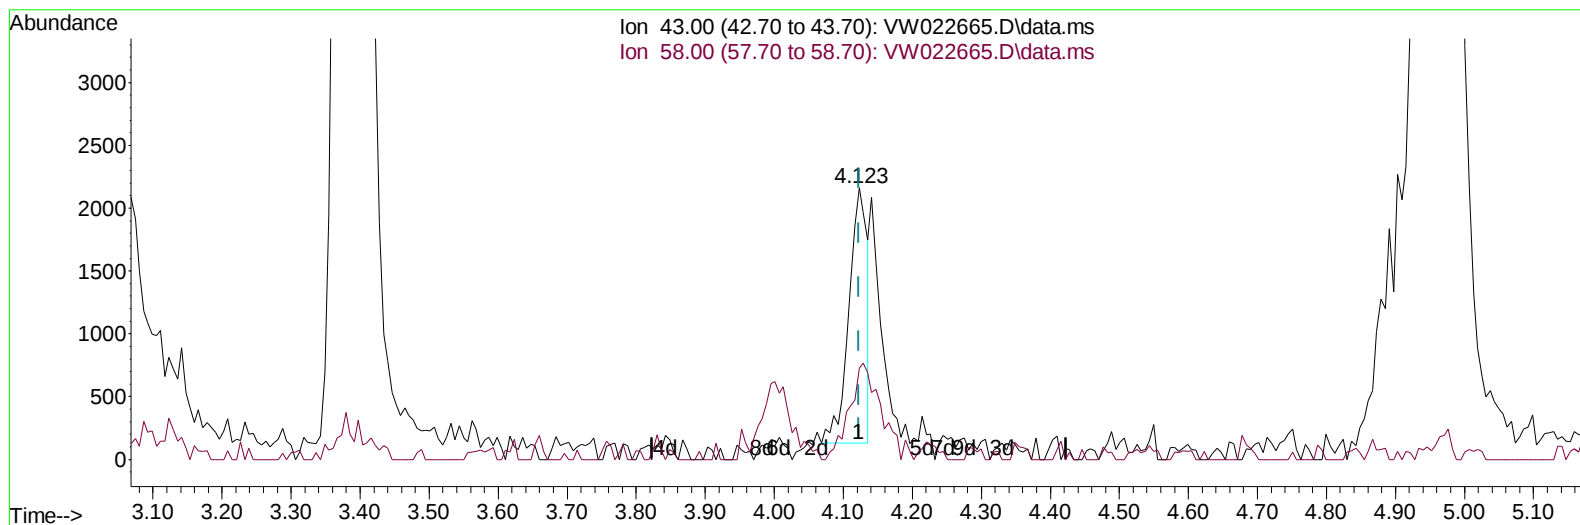

TIC: VW022665.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 4.80 ug/L

response 3754

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	55.91
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022665.D
 Acq On : 28 Apr 2022 15:02
 Operator : SY/VA
 Sample : N2562-15RE
 Misc : 5.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW476RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 01:11:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 01:08:57 2022
 Response via : Initial Calibration

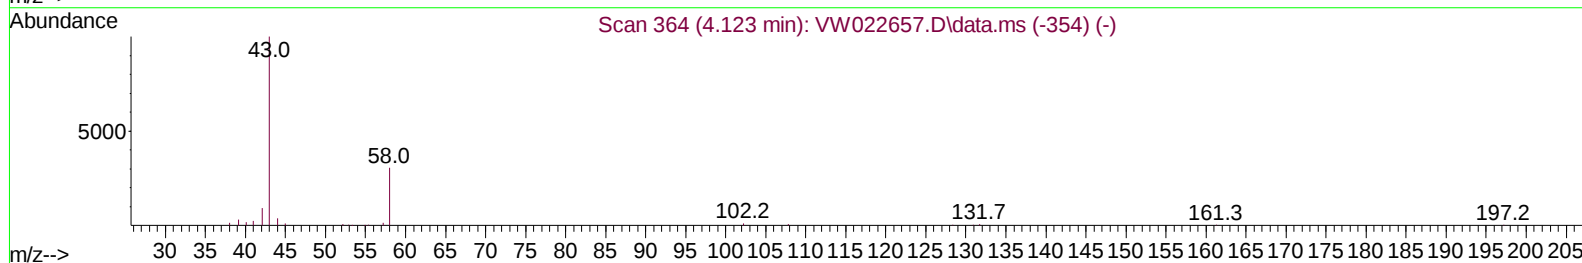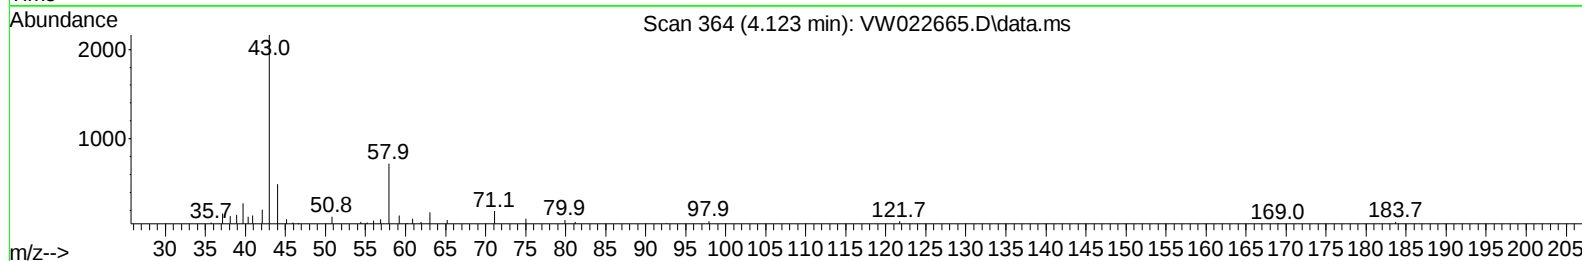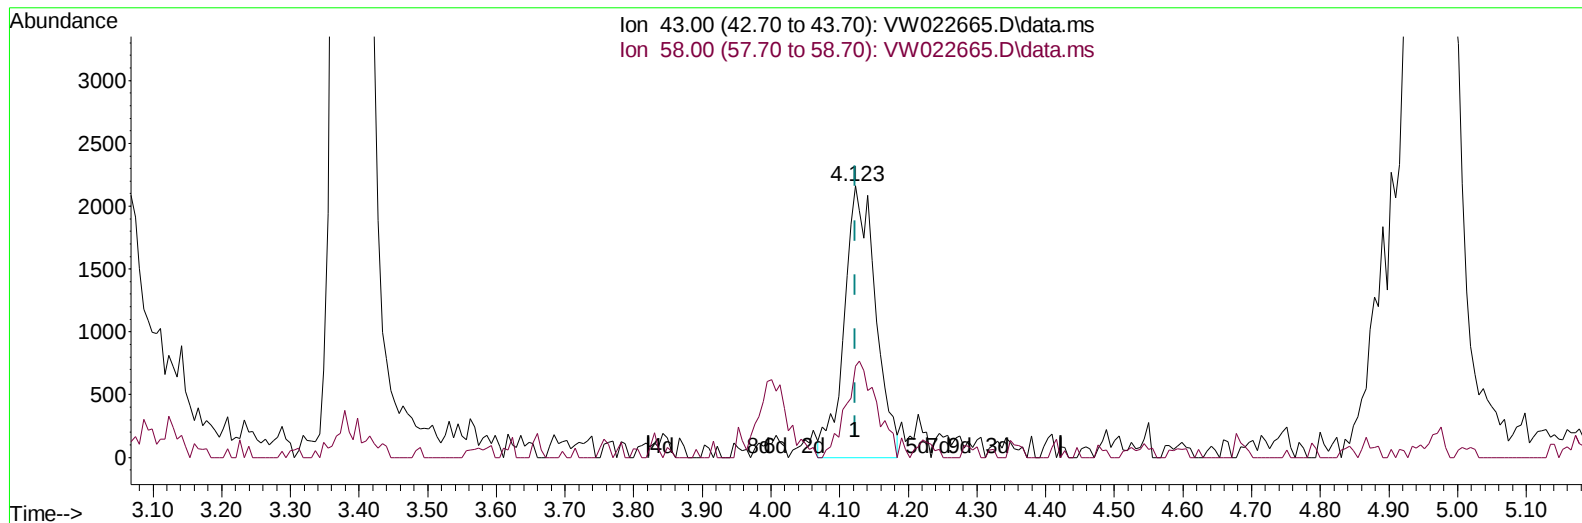

TIC: VW022665.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 8.72 ug/L m

response 6821

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	30.77
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022665.D
 Acq On : 28 Apr 2022 15:02
 Operator : SY/VA
 Sample : N2562-15RE
 Misc : 5.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW476RE

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:11:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 01:08:57 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.848	114		297580	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		202780	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		49534	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		85314	12.968	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	51.880%		
7) Chloroethane-d5	2.885	69		68882	16.707	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	66.840%		
11) 1,1-Dichloroethene-d2	4.019	63		91019	10.667	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	42.680%#		
21) 2-Butanone-d5	7.080	46		84754	73.793	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	147.580%#		
24) Chloroform-d	7.653	84		198169	21.305	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	85.240%		
26) 1,2-Dichloroethane-d4	8.305	65		115858	21.801	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	87.200%		
32) Benzene-d6	8.275	84		327971	26.473	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	105.880%		
36) 1,2-Dichloropropane-d6	9.274	67		108878	30.368	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	121.480%#		
41) Toluene-d8	10.323	98		239721	19.757	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	79.040%		
43) trans-1,3-Dichloroprop...	10.573	79		30186	17.840	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	71.360%		
47) 2-Hexanone-d5	10.921	63		58700	88.000	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	176.000%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		106579	34.961	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	139.840%#		
66) 1,2-Dichlorobenzene-d4	13.853	152		46543	26.528	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	106.120%		
Target Compounds							
						Qvalue	
13) Acetone	4.123	43		6821m	8.723	ug/L	
14) Carbon disulfide	4.385	76		26807	2.034	ug/L	98
16) Methylene chloride	4.915	84		20666	4.615	ug/L	85
29) Cyclohexane	7.958	56		27567	4.750	ug/L	93
33) Benzene	8.323	78		80829	5.871	ug/L	100
35) Methylcyclohexane	9.335	83		36520	5.522	ug/L	93
42) Toluene	10.384	91		159562	10.114	ug/L	96
52) Ethylbenzene	11.731	91		33197	1.877	ug/L	92
53) m,p-Xylene	11.835	106		13613	2.025	ug/L	80
54) o-Xylene	12.164	106		5894	0.917	ug/L	89
60) Isopropylbenzene	12.463	105		4771	0.580	ug/L #	88
62) 1,3,5-Trimethylbenzene	12.938	105		3430	0.758	ug/L	100
63) 1,2,4-Trimethylbenzene	13.249	105		9321	1.355	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022665.D
Acq On : 28 Apr 2022 15:02
Operator : SY/VA
Sample : N2562-15RE
Misc : 5.50g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW476RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 01:11:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 01:08:57 2022
Response via : Initial Calibration

