




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022666.D
Acq On : 28 Apr 2022 15:32
Operator : SY/VA
Sample : N2603-03
Misc : 6.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW484

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 01:11:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 01:08:57 2022
Response via : Initial Calibration

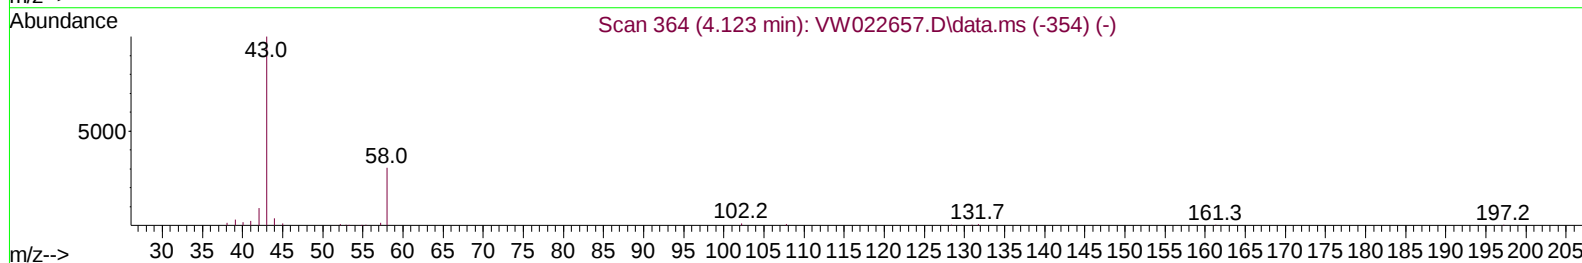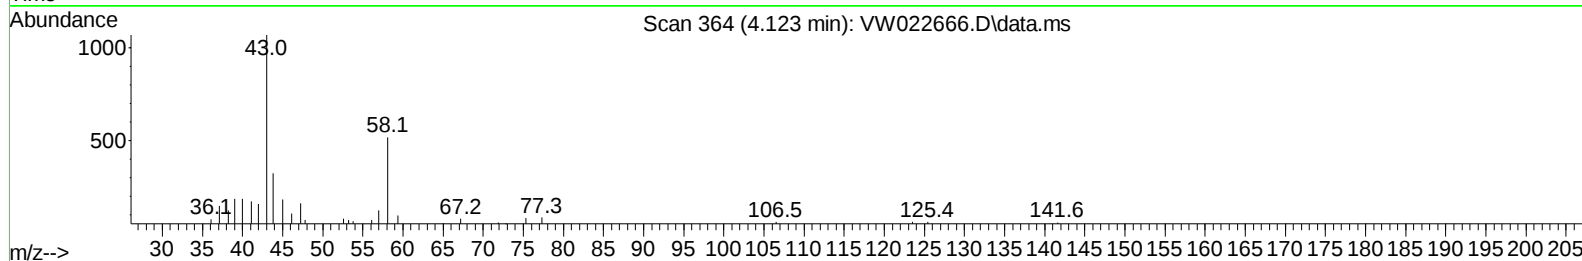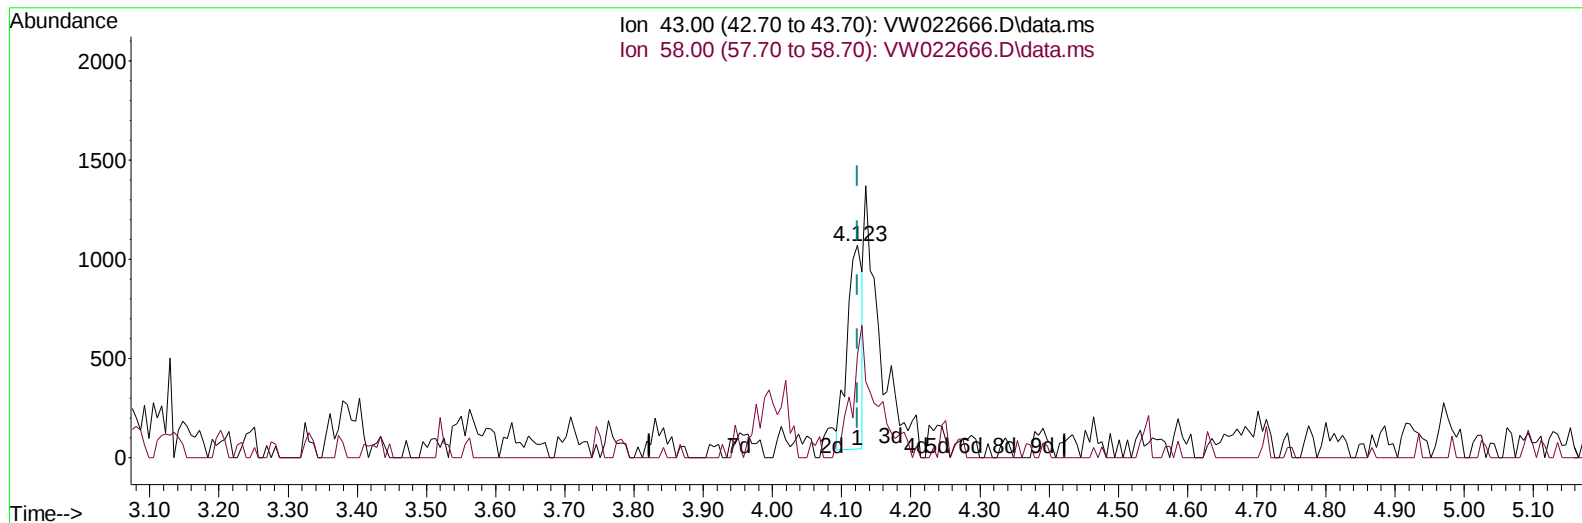

TIC: VW022666.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 2.83 ug/L

response 1536

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	20.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022666.D
 Acq On : 28 Apr 2022 15:32
 Operator : SY/VA
 Sample : N2603-03
 Misc : 6.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW484

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:11:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 01:08:57 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

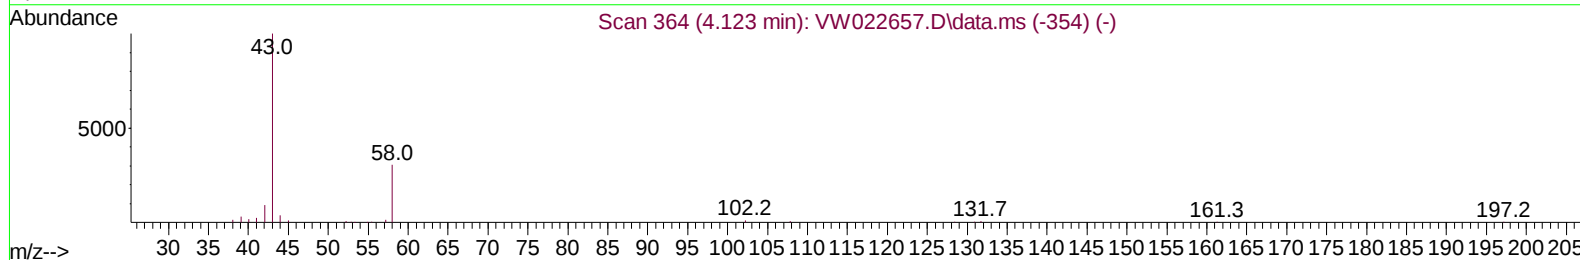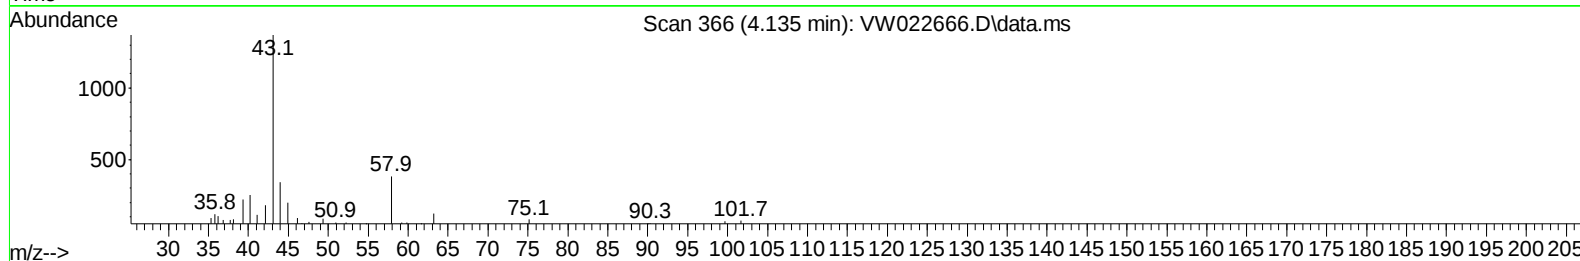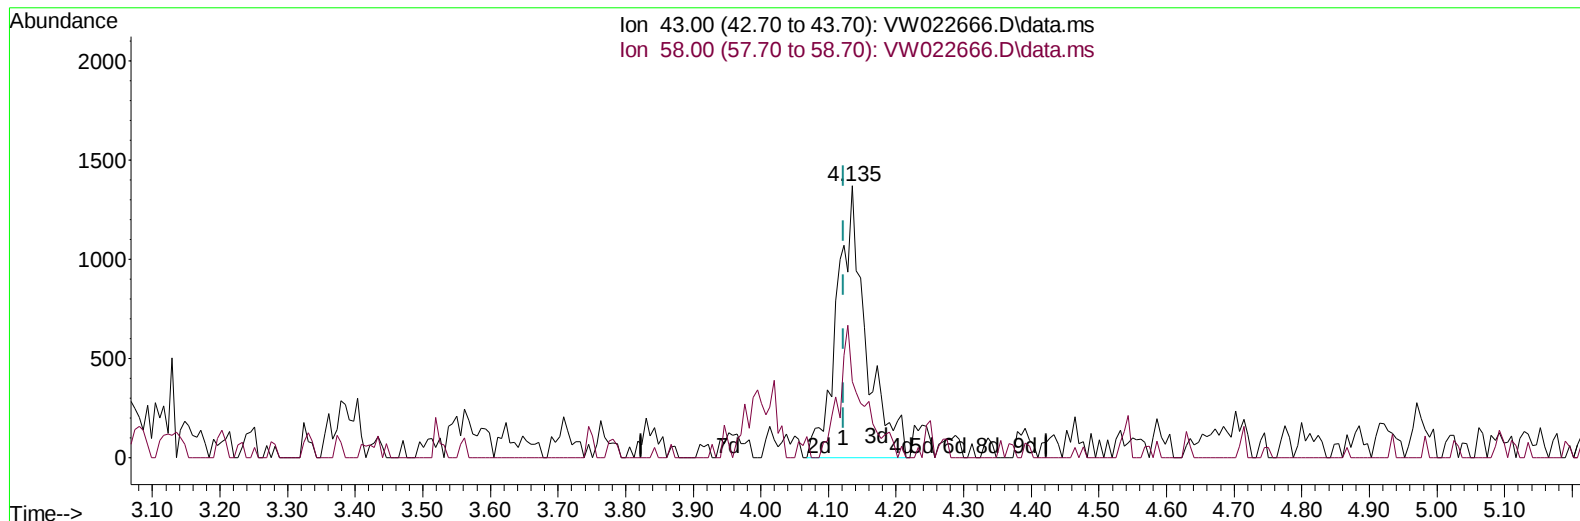

TIC: VW022666.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 7.52 ug/L m

response 4077

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	7.82
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022666.D
 Acq On : 28 Apr 2022 15:32
 Operator : SY/VA
 Sample : N2603-03
 Misc : 6.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW484

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 01:11:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 01:08:57 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		206445	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		108358	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		21677	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		74414	16.305	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	65.240%		
7) Chloroethane-d5	2.879	69		59776	20.899	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	83.600%		
11) 1,1-Dichloroethene-d2	4.013	63		64484	10.894	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	43.560%#		
21) 2-Butanone-d5	7.074	46		70818	88.879	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	177.760%#		
24) Chloroform-d	7.647	84		149954	23.239	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	92.960%		
26) 1,2-Dichloroethane-d4	8.305	65		84599	22.946	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	91.800%		
32) Benzene-d6	8.275	84		230553	34.825	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	139.320%#		
36) 1,2-Dichloropropane-d6	9.274	67		83941	43.814	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	175.240%#		
41) Toluene-d8	10.323	98		136876	21.110	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	84.440%		
43) trans-1,3-Dichloroprop...	10.573	79		16233	17.954	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	71.800%		
47) 2-Hexanone-d5	10.927	63		44472	124.765	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	249.540%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		91664	56.270	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	225.080%#		
66) 1,2-Dichlorobenzene-d4	13.847	152		21122	27.510	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	110.040%		
Target Compounds							
13) Acetone	4.135	43		4077m	7.515	ug/L	
16) Methylene chloride	4.909	84		11871	3.821	ug/L	80
42) Toluene	10.384	91		9878	1.172	ug/L	100
62) 1,3,5-Trimethylbenzene	12.938	105		902	0.455	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022666.D
Acq On : 28 Apr 2022 15:32
Operator : SY/VA
Sample : N2603-03
Misc : 6.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW484

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 01:11:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 01:08:57 2022
Response via : Initial Calibration

