




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022675.D
 Acq On : 28 Apr 2022 21:10
 Operator : SY/VA
 Sample : N2603-02
 Misc : 6.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW483

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

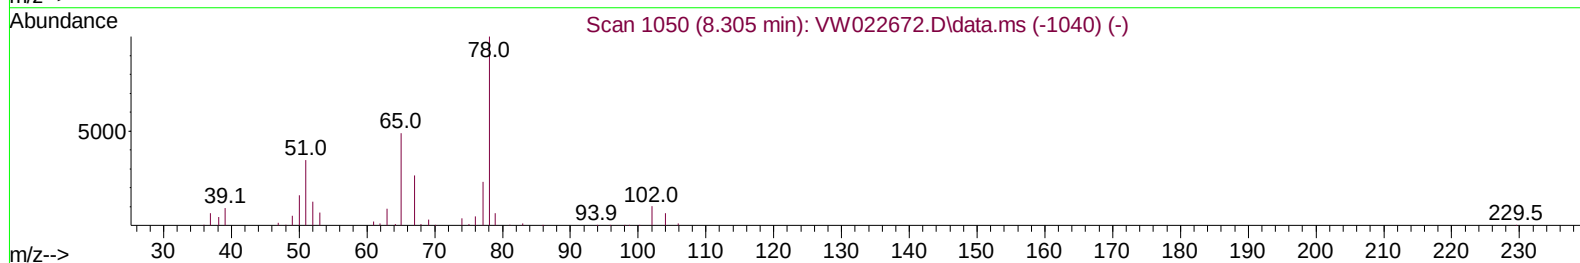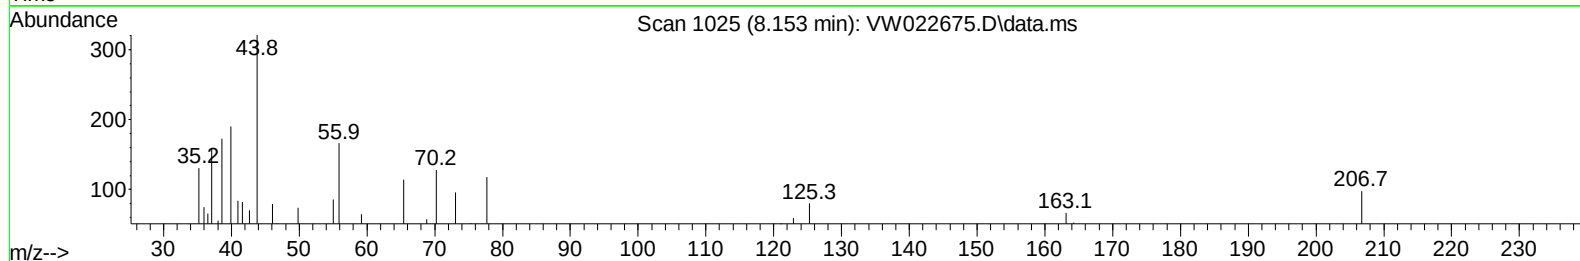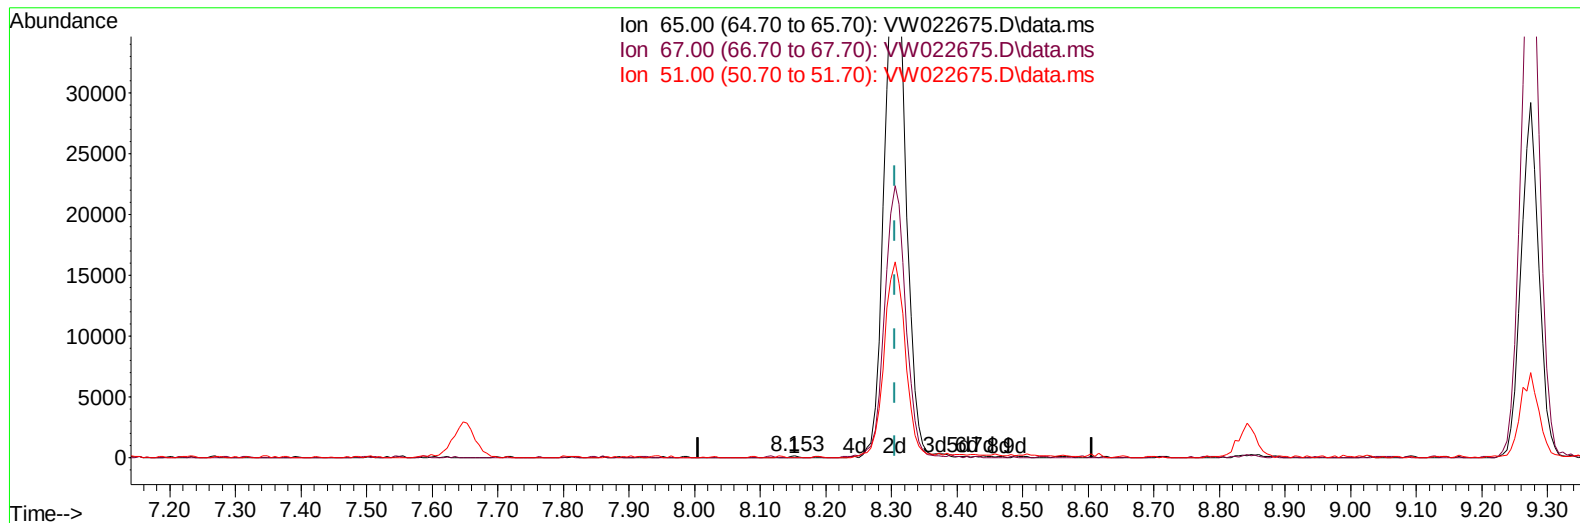

TIC: VW022675.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.153min (-0.153) 0.02 ug/L

response 97

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	52.58
51.00	99.30	79.38
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022675.D
 Acq On : 28 Apr 2022 21:10
 Operator : SY/VA
 Sample : N2603-02
 Misc : 6.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW483

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

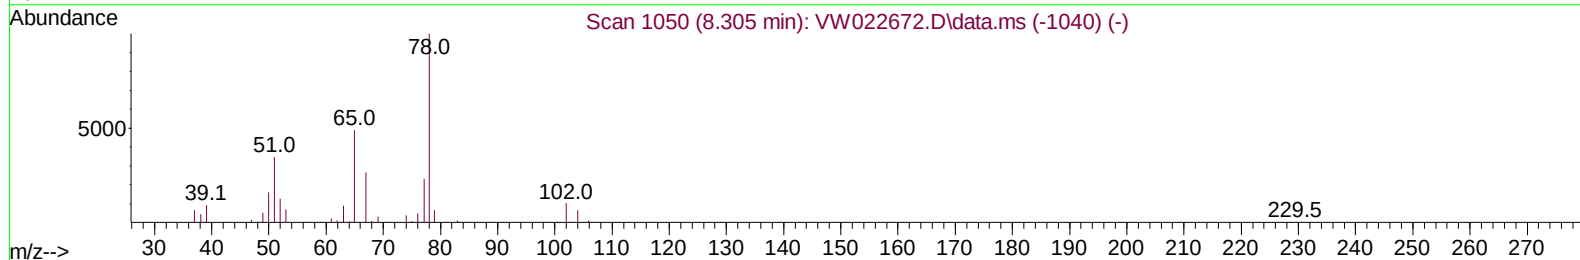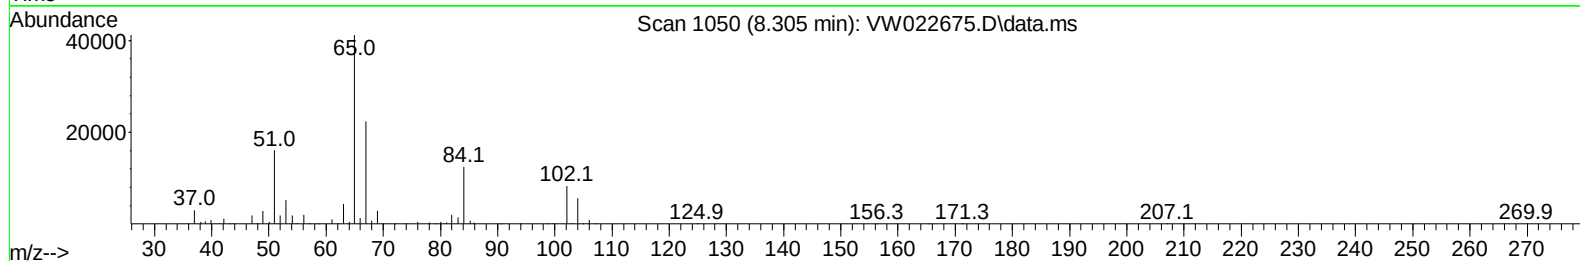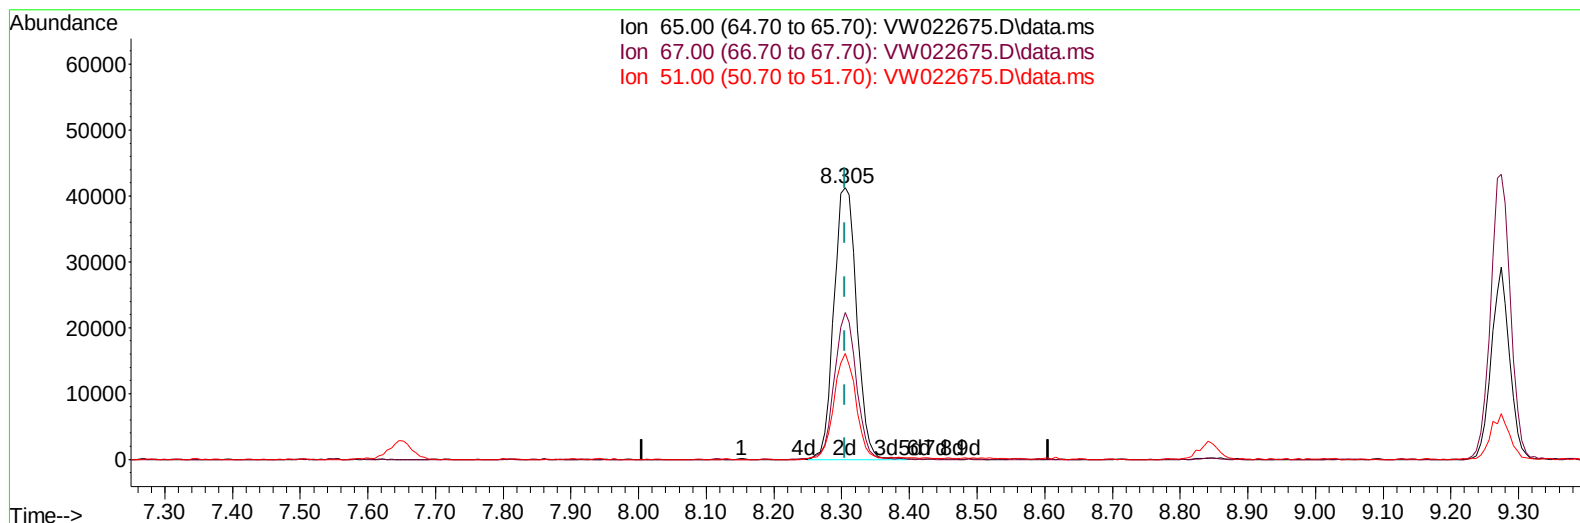

TIC: VW022675.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 21.75 ug/L m

response 96006

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.05#
51.00	99.30	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022675.D
 Acq On : 28 Apr 2022 21:10
 Operator : SY/VA
 Sample : N2603-02
 Misc : 6.77g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW483

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	247186	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	226755	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	99928	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	61483	11.251	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	45.000%	
7) Chloroethane-d5	2.885	69	52672	15.380	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	61.520%	
11) 1,1-Dichloroethene-d2	4.013	63	66979	9.450	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	37.800%#	
21) 2-Butanone-d5	7.074	46	60544	63.461	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	126.920%	
24) Chloroform-d	7.647	84	155229	20.091	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	80.360%	
26) 1,2-Dichloroethane-d4	8.305	65	96006m	21.748	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	87.000%	
32) Benzene-d6	8.275	84	254771	18.390	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	73.560%	
36) 1,2-Dichloropropane-d6	9.274	67	89117	22.228	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	88.920%	
41) Toluene-d8	10.323	98	216390	15.948	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	63.800%	
43) trans-1,3-Dichloroprop...	10.579	79	30982	16.374	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	65.480%	
47) 2-Hexanone-d5	10.920	63	46947	62.939	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	125.880%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	105657	30.994	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	123.960%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	78601	22.207	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	88.840%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022675.D
Acq On : 28 Apr 2022 21:10
Operator : SY/VA
Sample : N2603-02
Misc : 6.77g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW483

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 02:06:41 2022
Response via : Initial Calibration

