




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022676.D
 Acq On : 28 Apr 2022 21:34
 Operator : SY/VA
 Sample : N2603-01
 Misc : 7.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW482

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

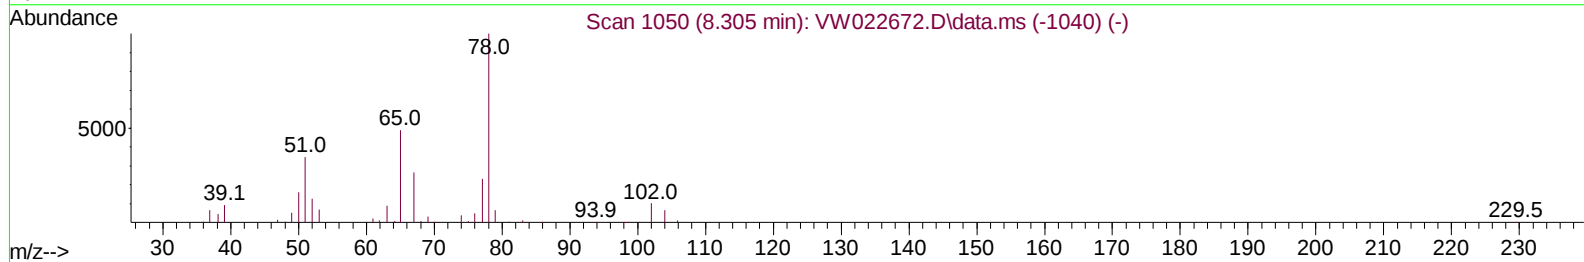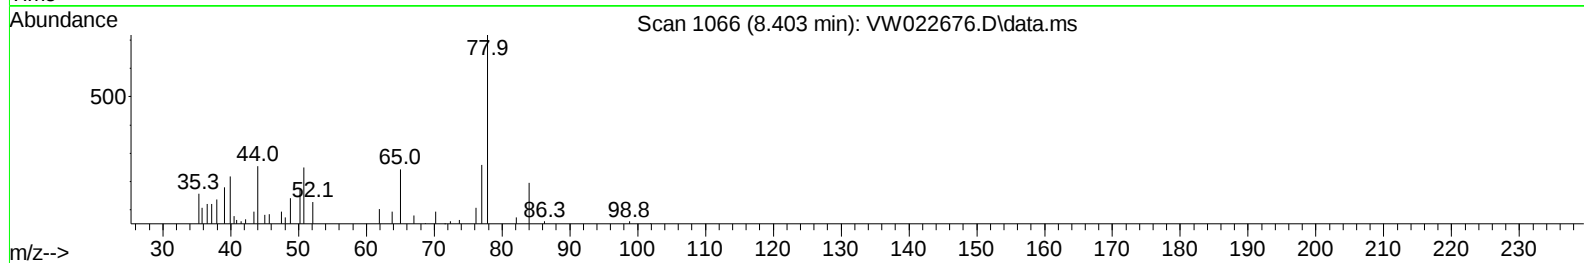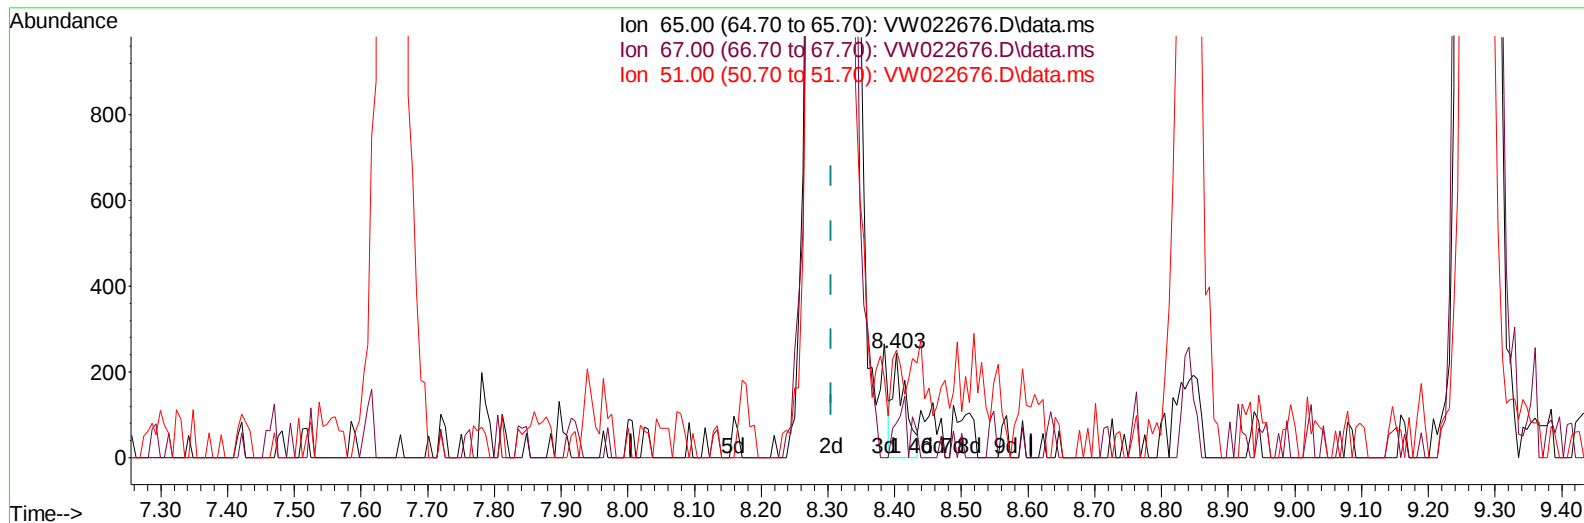

TIC: VW022676.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.403min (+ 0.097) 0.07 ug/L

response 325

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	44.00
51.00	99.30	95.08
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022676.D
 Acq On : 28 Apr 2022 21:34
 Operator : SY/VA
 Sample : N2603-01
 Misc : 7.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW482

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

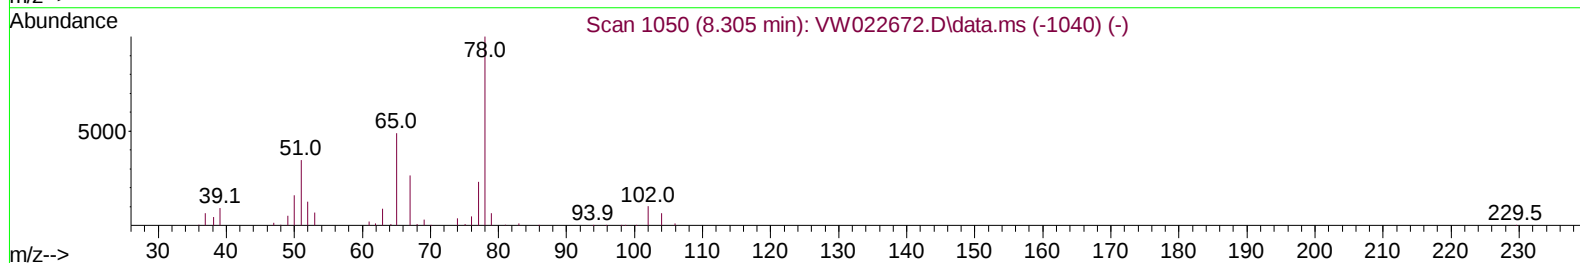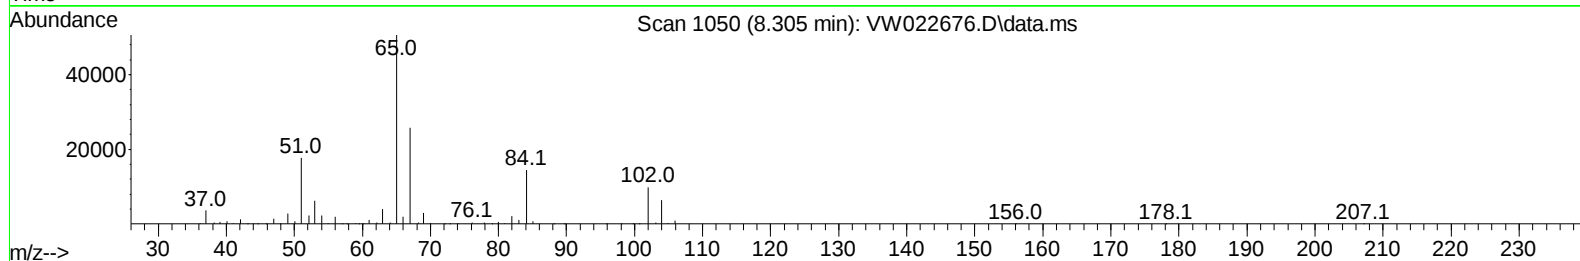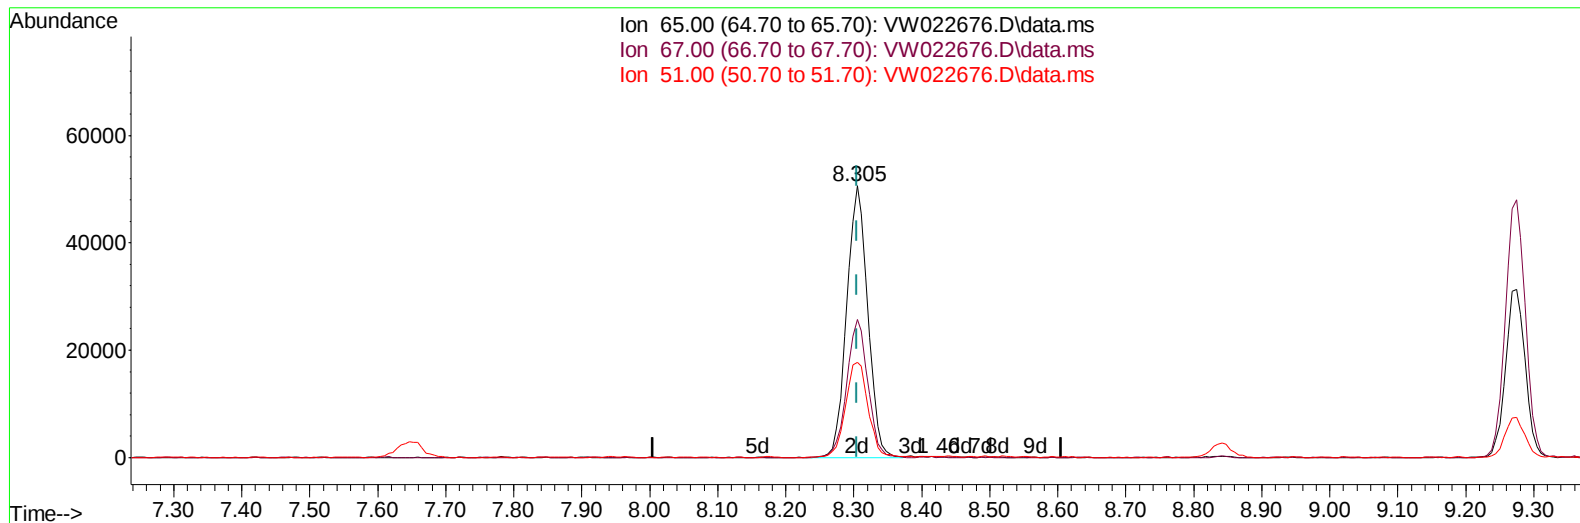

TIC: VW022676.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 23.35 ug/L m

response 108265

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.13#
51.00	99.30	0.29#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022676.D
 Acq On : 28 Apr 2022 21:34
 Operator : SY/VA
 Sample : N2603-01
 Misc : 7.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW482

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		259667	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		230619	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		94985	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		72300	12.595	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	50.360%	
7) Chloroethane-d5	2.885	69		58513	16.264	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	65.040%	
11) 1,1-Dichloroethene-d2	4.013	63		77138	10.360	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	41.440%#	
21) 2-Butanone-d5	7.074	46		66395	66.249	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	132.500%	
24) Chloroform-d	7.653	84		176277	21.719	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	86.880%	
26) 1,2-Dichloroethane-d4	8.305	65		108265m	23.346	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	93.400%	
32) Benzene-d6	8.275	84		291379	20.680	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	82.720%	
36) 1,2-Dichloropropane-d6	9.274	67		98272	24.101	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	96.400%	
41) Toluene-d8	10.323	98		239945	17.388	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	69.560%	
43) trans-1,3-Dichloroprop...	10.579	79		35265	18.326	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	73.320%	
47) 2-Hexanone-d5	10.920	63		53441	70.445	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	140.880%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		112144	32.346	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	129.400%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		78648	23.377	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	93.520%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022676.D
Acq On : 28 Apr 2022 21:34
Operator : SY/VA
Sample : N2603-01
Misc : 7.12g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW482

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 02:06:41 2022
Response via : Initial Calibration

