




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022679.D
 Acq On : 28 Apr 2022 22:46
 Operator : SY/VA
 Sample : N2603-08
 Misc : 5.55g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW489

Manual IntegrationsAPPROVED

Quant Time: Apr 29 02:21:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

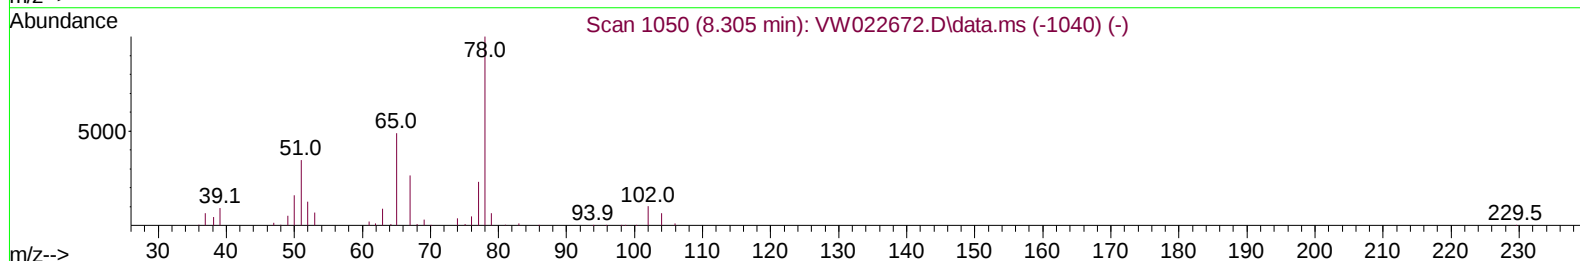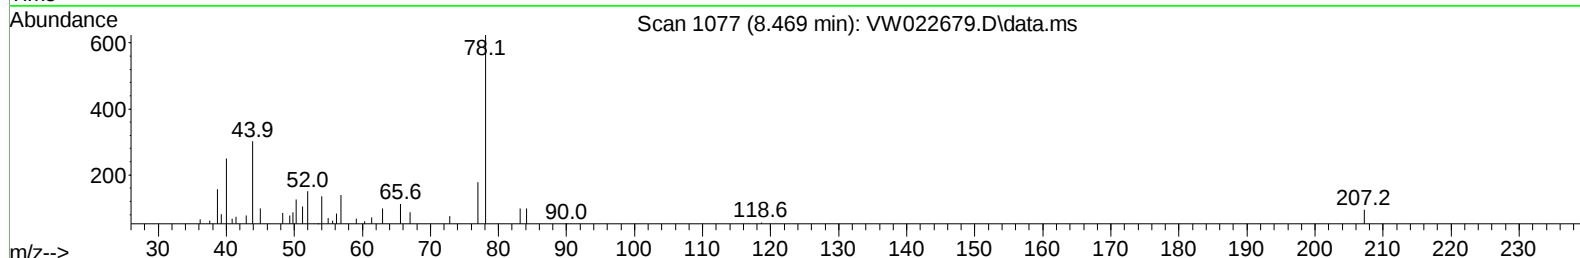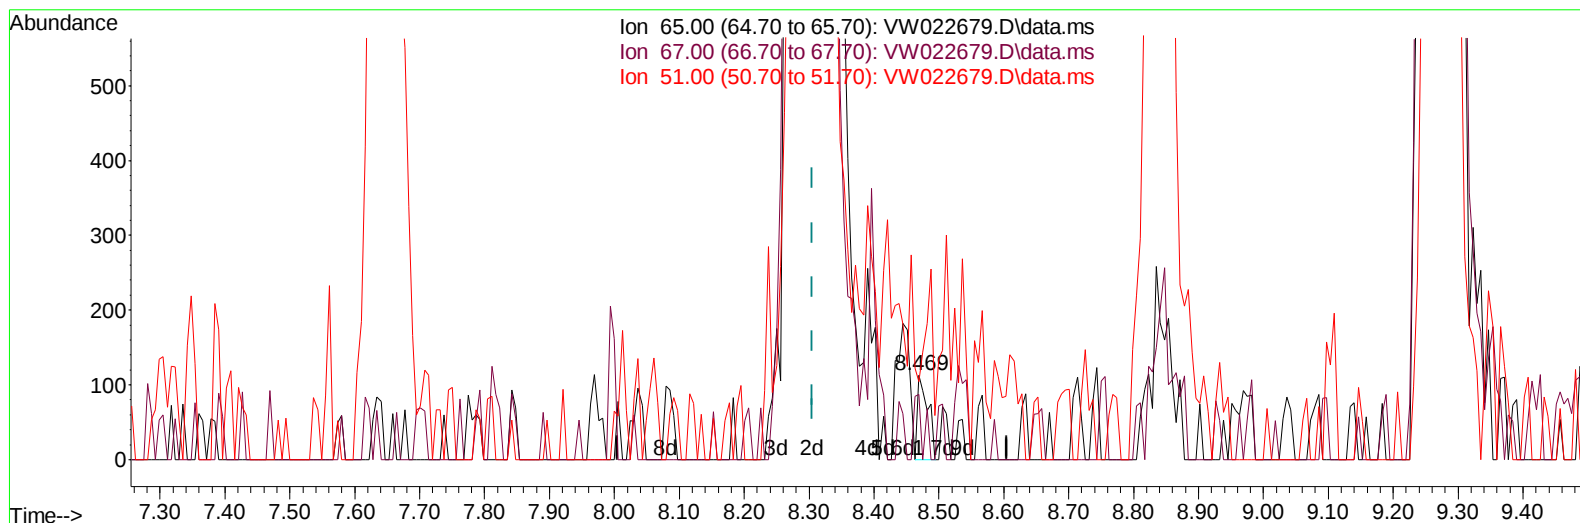

TIC: VW022679.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.469min (+ 0.164) 0.03 ug/L

response 126

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	50.00
51.00	99.30	107.94
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022679.D
 Acq On : 28 Apr 2022 22:46
 Operator : SY/VA
 Sample : N2603-08
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW489

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

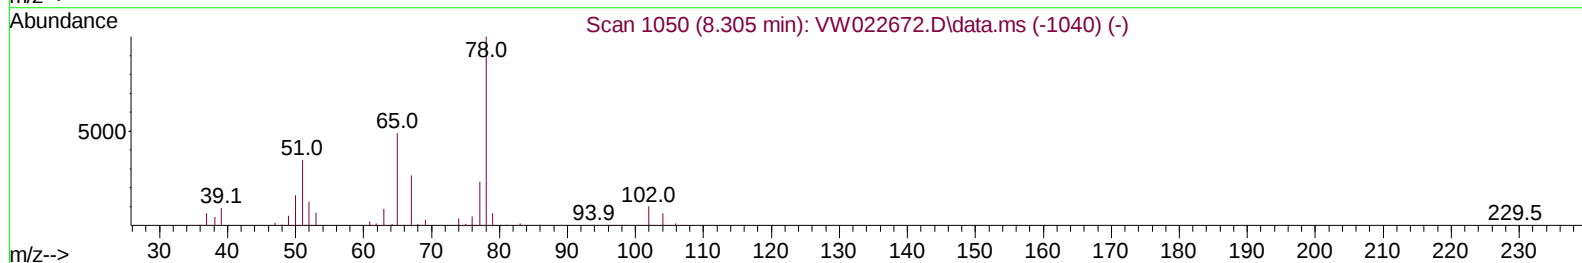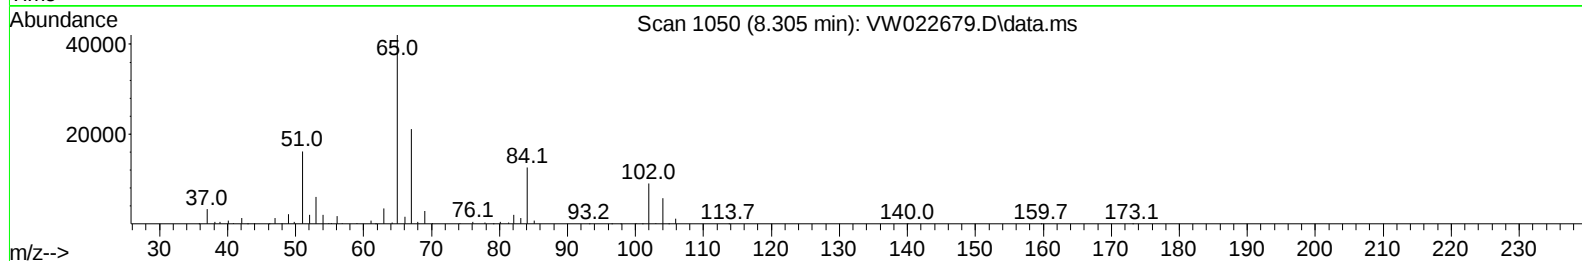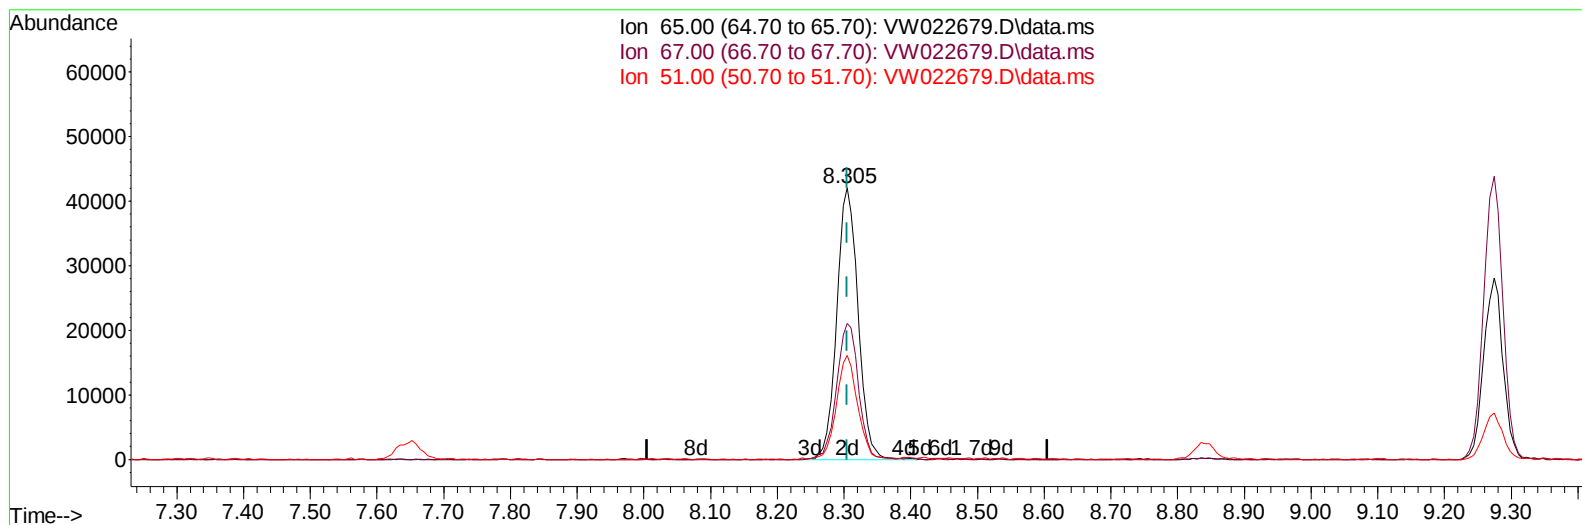

TIC: VW022679.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 20.05 ug/L m

response 93324

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.07#
51.00	99.30	0.15#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022679.D
 Acq On : 28 Apr 2022 22:46
 Operator : SY/VA
 Sample : N2603-08
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW489

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	260676	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	242108	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	104691	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	60673	10.528	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	42.120%	
7) Chloroethane-d5	2.885	69	51671	14.307	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	57.240%	
11) 1,1-Dichloroethene-d2	4.013	63	67443	9.023	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	36.080%#	
21) 2-Butanone-d5	7.073	46	54373	54.043	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.080%	
24) Chloroform-d	7.646	84	155072	19.032	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	76.120%	
26) 1,2-Dichloroethane-d4	8.305	65	93324m	20.046	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	80.200%	
32) Benzene-d6	8.274	84	257068	17.379	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	69.520%	
36) 1,2-Dichloropropane-d6	9.274	67	87873	20.528	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	82.120%	
41) Toluene-d8	10.323	98	224604	15.504	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	62.000%	
43) trans-1,3-Dichloroprop...	10.573	79	29317	14.512	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	58.040%	
47) 2-Hexanone-d5	10.920	63	45147	56.688	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	113.380%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	101731	27.950	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	111.800%	
66) 1,2-Dichlorobenzene-d4	13.853	152	78371	21.135	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	84.520%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022679.D
Acq On : 28 Apr 2022 22:46
Operator : SY/VA
Sample : N2603-08
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW489

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:21:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 02:06:41 2022
Response via : Initial Calibration

