




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022681.D
 Acq On : 28 Apr 2022 23:34
 Operator : SY/VA
 Sample : N2603-03RE
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW484RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:22:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

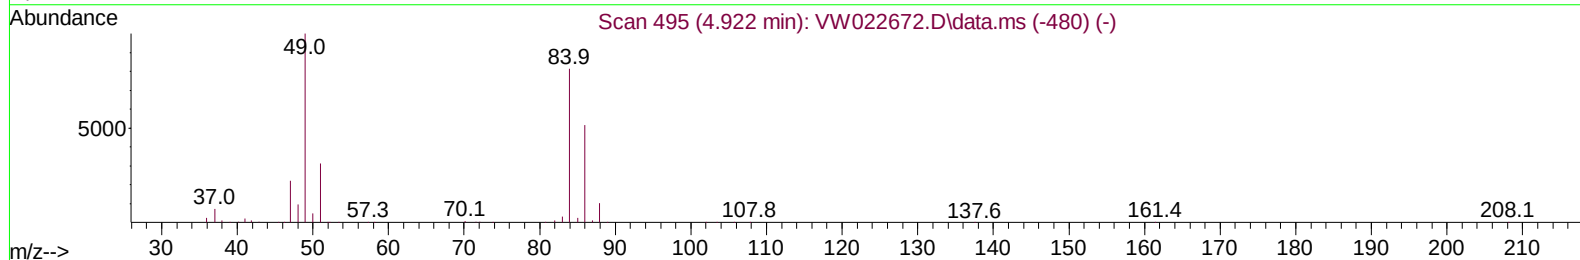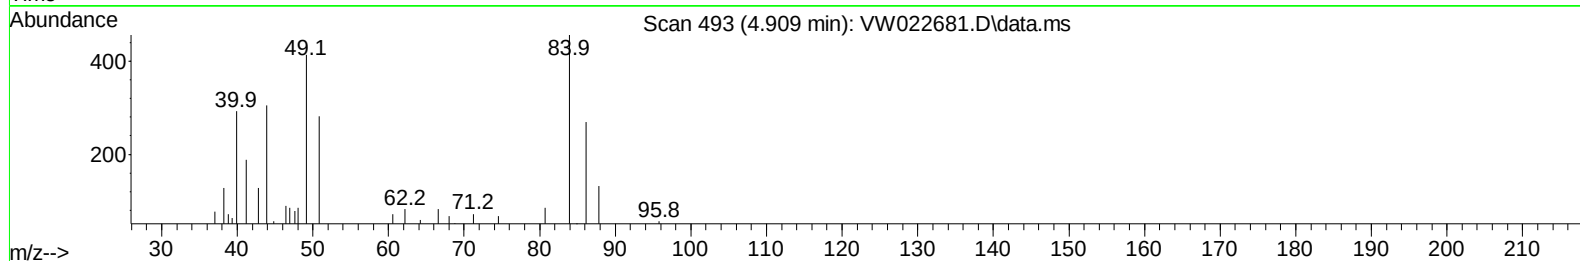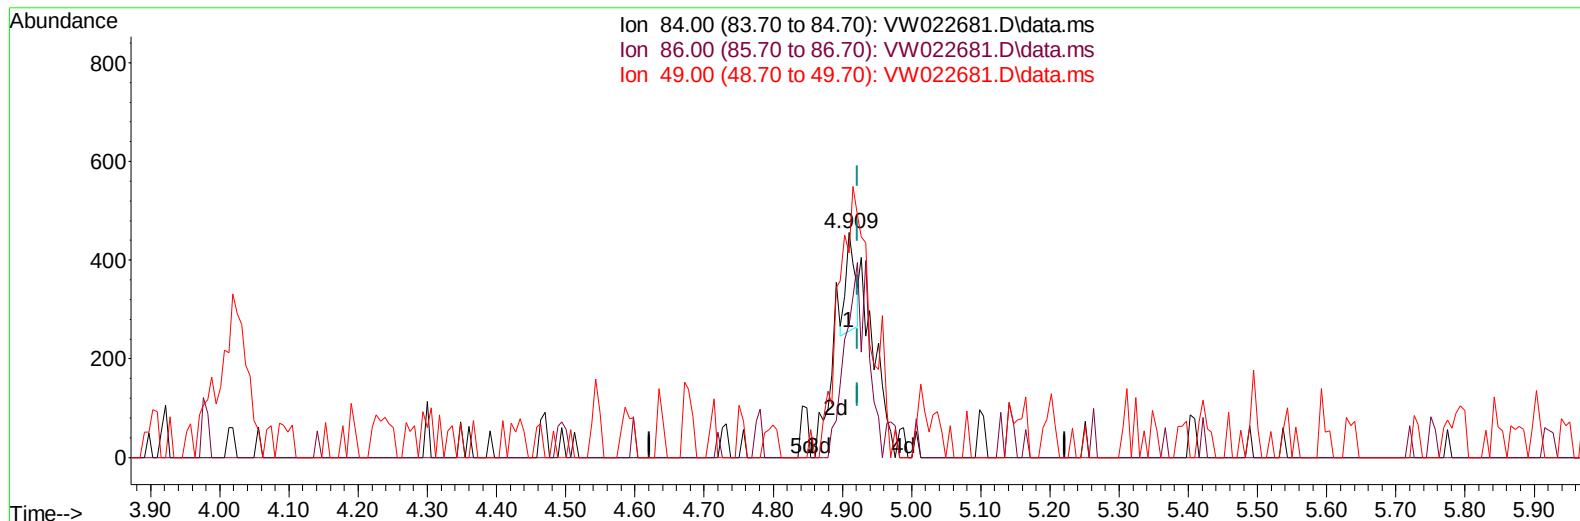

TIC: VW022681.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.012) 0.45 ug/L

response 182

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.10	58.99
49.00	134.60	90.79#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022681.D
 Acq On : 28 Apr 2022 23:34
 Operator : SY/VA
 Sample : N2603-03RE
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW484RE

Manual IntegrationsAPPROVED

Quant Time: Apr 29 02:22:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

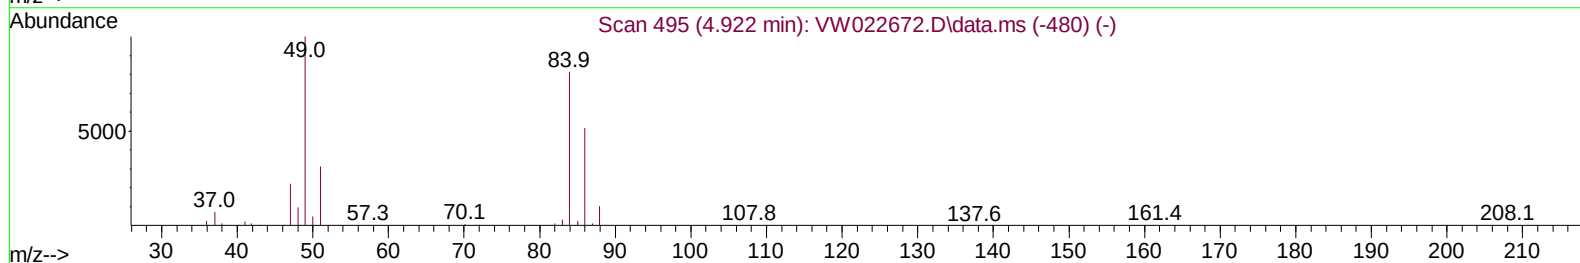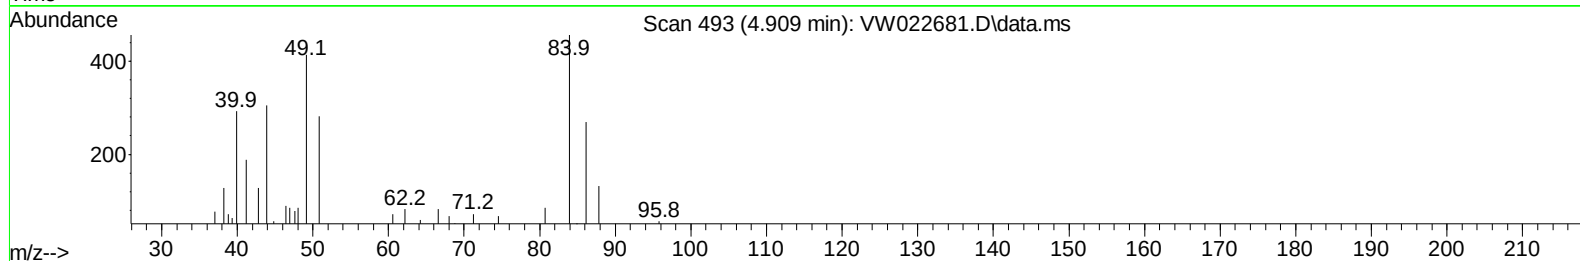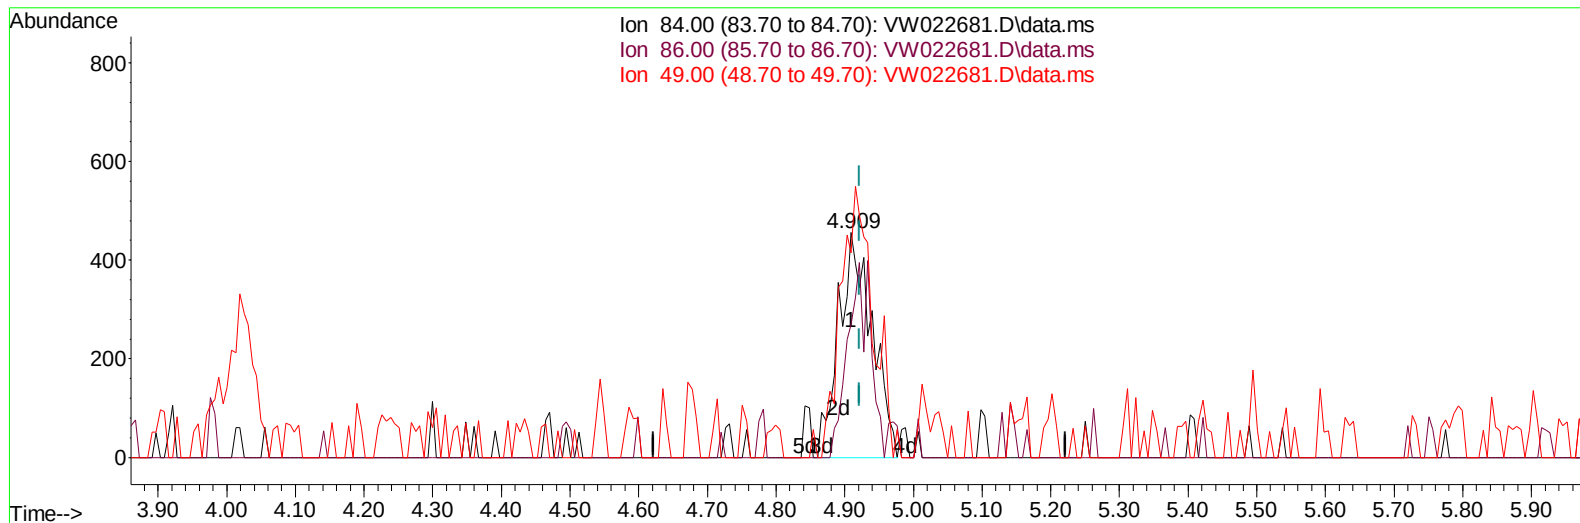

TIC: VW022681.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.012) 3.82 ug/L m

response 1539

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.10	58.99
49.00	134.60	90.79#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022681.D
 Acq On : 28 Apr 2022 23:34
 Operator : SY/VA
 Sample : N2603-03RE
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW484RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:22:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 02:06:41 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		26784	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		9940	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		1382	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		14747	24.906	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	99.640%	
7) Chloroethane-d5	2.885	69		17044	45.930	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	183.720%#	
11) 1,1-Dichloroethene-d2	4.013	63		12125	15.788	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	63.160%	
21) 2-Butanone-d5	7.086	46		11270	109.020	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	218.040%#	
24) Chloroform-d	7.653	84		23406	27.958	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	111.840%	
26) 1,2-Dichloroethane-d4	8.305	65		13963	29.191	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	116.760%	
32) Benzene-d6	8.281	84		32745	53.919	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	215.680%#	
36) 1,2-Dichloropropane-d6	9.274	67		11577	65.874	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	263.480%#	
41) Toluene-d8	10.323	98		14402	24.214	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	96.840%	
43) trans-1,3-Dichloroprop...	10.579	79		1662	20.038	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	80.160%	
47) 2-Hexanone-d5	10.926	63		4491	137.349	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	274.700%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		10363	69.349	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	277.400%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		1282	26.190	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	104.760%	
Target Compounds							
13) Acetone	4.135	43		1212	17.220	ug/L	69
16) Methylene chloride	4.909	84		1539m	3.819	ug/L	
42) Toluene	10.384	91		1277	1.651	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022681.D
Acq On : 28 Apr 2022 23:34
Operator : SY/VA
Sample : N2603-03RE
Misc : 7.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW484RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 02:22:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 02:06:41 2022
Response via : Initial Calibration

