

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
 Data File : VW022658.D
 Acq On : 28 Apr 2022 12:12
 Operator : SY/VA
 Sample : VW0428SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK488

Quant Time: Apr 29 01:09:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 01:08:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	300605	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	292113	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	156024	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	113599	17.094	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.360%
7) Chloroethane-d5	2.891	69	83493	20.047	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.200%
11) 1,1-Dichloroethene-d2	4.013	63	133556	15.495	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.960%
21) 2-Butanone-d5	7.080	46	54628	47.085	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.160%
24) Chloroform-d	7.647	84	205924	21.916	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.680%
26) 1,2-Dichloroethane-d4	8.305	65	115661	21.545	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.160%
32) Benzene-d6	8.274	84	397114	22.251	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	9.274	67	115252	22.315	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.280%
41) Toluene-d8	10.323	98	376124	21.518	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.080%
43) trans-1,3-Dichloroprop...	10.579	79	46959	19.266	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.080%
47) 2-Hexanone-d5	10.920	63	44294	46.096	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.200%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	102635	23.371	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.480%
66) 1,2-Dichlorobenzene-d4	13.853	152	130245	23.568	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.280%
Target Compounds						
13) Acetone	4.129	43	4153	5.257	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042822\
Data File : VW022658.D
Acq On : 28 Apr 2022 12:12
Operator : SY/VA
Sample : VW0428SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK488

Quant Time: Apr 29 01:09:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 01:08:57 2022
Response via : Initial Calibration

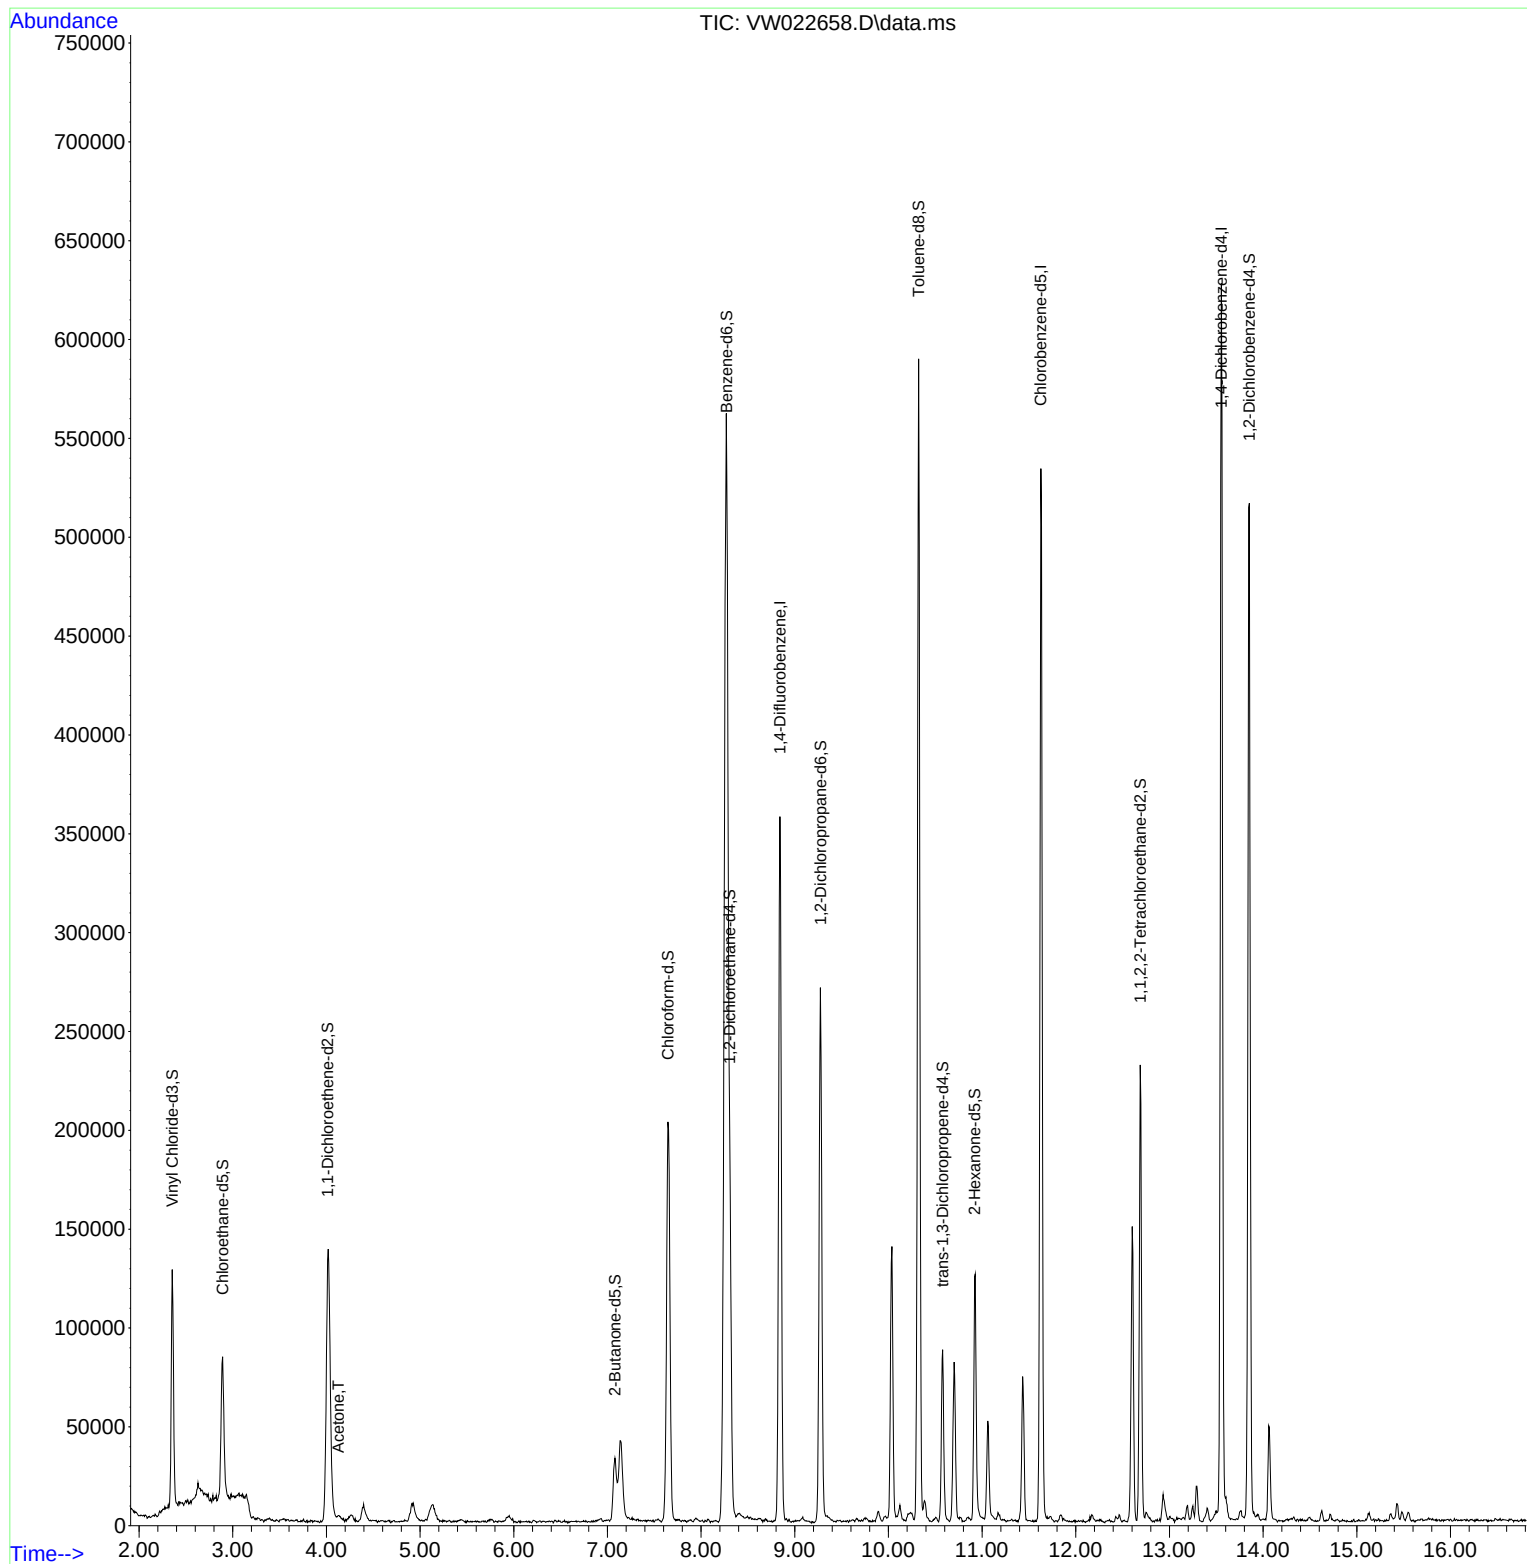

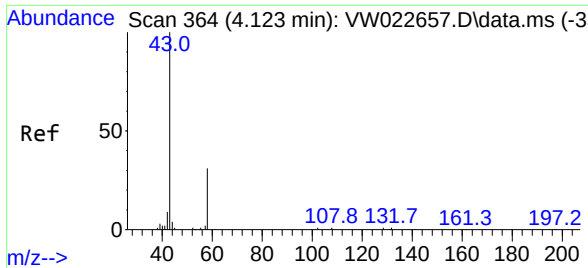

#13
 Acetone
 Concen: 5.257 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022658.D
 Acq: 28 Apr 2022 12:12

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK488

Tgt Ion: 43 Resp: 4153

Ion	Ratio	Lower	Upper
43	100		
58	22.8	0.0	57.0

