

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW042920\
 Data File : VW015378.D
 Acq On : 29 Apr 2020 14:26
 Operator : SY/VA
 Sample : L2392-03
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Quant Time: Apr 30 08:57:35 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042820S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 30 08:26:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	399531	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	352394	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	181792	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	64804	22.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.12%
7) Chloroethane-d5	2.90	69	68048	20.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.40%
10) 1,1-Dichloroethene-d2	4.01	63	115171	15.67	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.68%
20) 2-Butanone-d5	7.07	46	38024	42.53	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.06%
24) Chloroform-d	7.65	84	182045	20.72	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.88%
26) 1,2-Dichloroethane-d4	8.30	65	96033	21.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.92%
29) Benzene-d6	8.27	84	364081	22.43	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.72%
33) 1,2-Dichloropropane-d6	9.27	67	98886	21.77	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.08%
37) Toluene-d8	10.32	98	369553	22.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.24%
38) trans-1,3-Dichloropropene-	10.57	79	47315	20.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.40%
39) 2-Hexanone-d5	10.92	63	35340	42.61	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.22%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	78806	20.50	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.00%
61) 1,2-Dichlorobenzene-d4	13.85	152	138145	21.87	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.48%


Target Compounds					Ovalue
13) Acetone	4.12	43	2271	3.016 ug/L	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW042920\
Data File : VW015378.D
Acq On : 29 Apr 2020 14:26
Operator : SY/VA
Sample : L2392-03
Misc : 5.02G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Apr 30 08:57:35 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042820S.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 30 08:26:20 2020
Response via : Initial Calibration

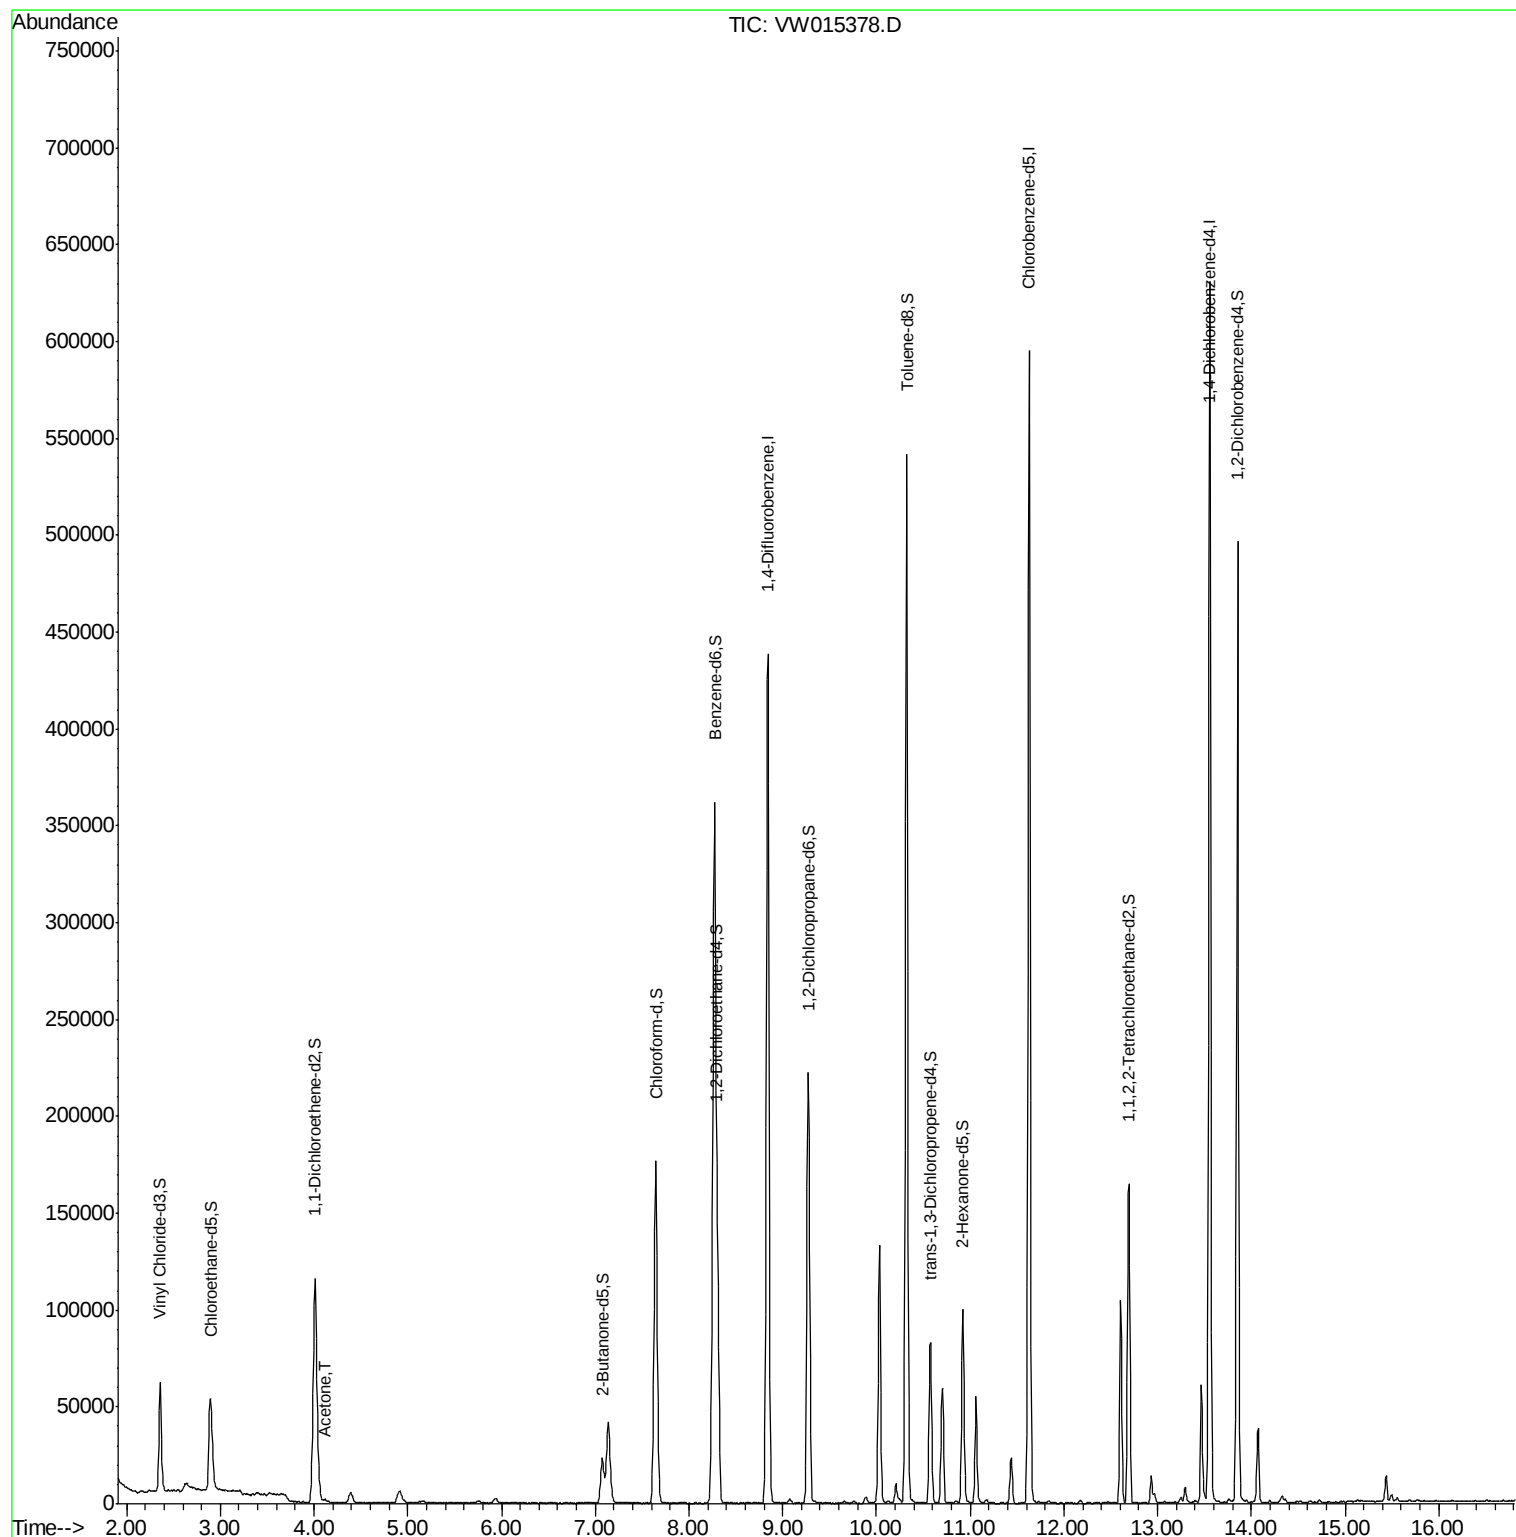

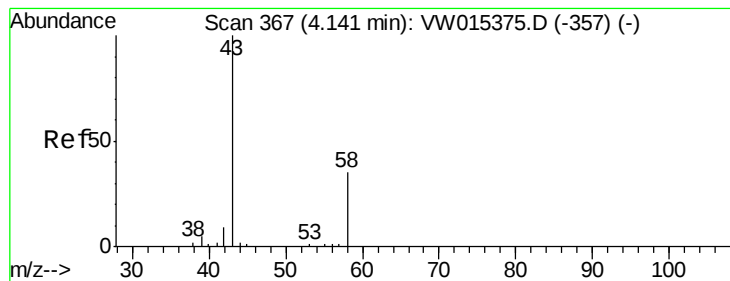

#13

Acetone

Concen: 3.016 ug/L

RT: 4.12 min Scan# 364

Delta R.T. -0.02 min

Lab File: VW015378.D

Acq: 29 Apr 2020 14:26

Instrument :

MSVOA_W

ClientSampleId :

VHBLK01

Tot Ion: 43 Resp: 2271

Ion Ratio Lower Upper

43 100

58 12.3 0.0 68.0

