


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW042920\
 Data File : VW015374.D
 Acq On : 29 Apr 2020 09:13
 Operator : SY/VA
 Sample : BFB26
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB26

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042820S.M
 Title : VOC Analysis
 Last Update : Thu Apr 30 08:26:20 2020

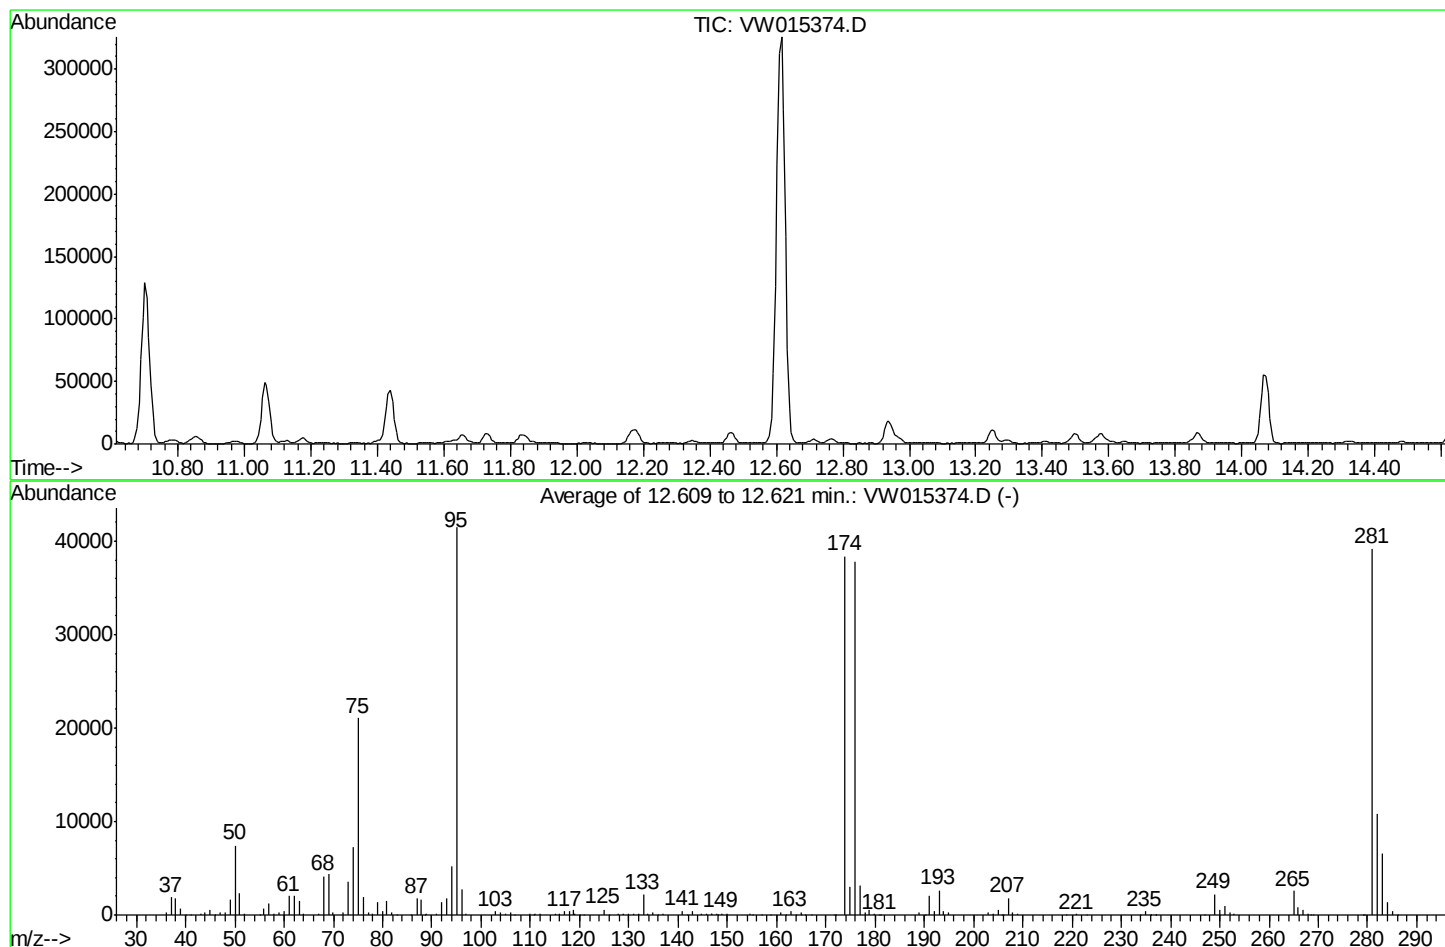

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	7418	PASS
75	95	30	80	50.7	21037	PASS
95	95	100	100	100.0	41482	PASS
96	95	5	9	6.8	2813	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.6	38400	PASS
175	174	5	9	7.7	2963	PASS
176	174	95	101	98.4	37776	PASS
177	176	5	9	8.5	3193	PASS

m/z	Abundance
36.00	338.0
37.00	1692.0
38.00	1746.0
39.00	682.0
40.00	129.0
41.00	109.0
43.00	231.0
43.90	471.0
45.00	758.0
46.00	106.0
47.00	358.0
47.90	215.0
49.00	1672.0
50.00	6517.0
51.00	2083.0
52.00	90.0
55.00	167.0
55.90	574.0
57.00	1278.0
58.00	96.0
59.00	485.0
60.00	404.0
61.00	1914.0
62.00	1655.0
63.00	1287.0
63.90	149.0
66.90	130.0
68.00	3815.0
69.00	4184.0
69.90	297.0
72.00	166.0
73.00	4175.0
74.00	6919.0
75.00	19624.0
76.00	1681.0
77.10	296.0
78.10	159.0
78.80	1264.0
79.90	396.0
80.90	1434.0
81.90	290.0
83.00	71.0
86.90	1544.0
87.90	1268.0
89.00	161.0
90.80	145.0
92.00	1179.0
93.00	1564.0
94.00	4491.0
95.00	37984.0
96.00	2673.0
97.00	91.0
103.00	531.0
104.00	346.0
105.00	121.0
105.90	181.0
106.90	74.0
109.90	280.0
110.70	207.0
111.00	170.0
111.80	159.0
115.00	227.0
115.90	174.0
116.90	376.0
117.90	448.0
118.80	809.0
120.00	102.0
120.80	133.0
124.90	886.0
127.90	128.0
128.90	96.0
129.90	162.0
130.90	113.0
132.00	152.0
133.00	3458.0
134.90	424.0
135.80	51.0
137.00	79.0
141.00	299.0
142.00	56.0
143.00	310.0
144.90	103.0
145.90	62.0
147.00	337.0
147.80	168.0
148.80	224.0
149.80	87.0
154.70	112.0
157.00	55.0
158.80	67.0
160.90	362.0
162.00	83.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

162.90	624.0
164.00	131.0
164.90	399.0
165.90	59.0
167.00	74.0
168.90	150.0
171.70	68.0
173.90	31864.0
174.90	2457.0
175.90	30392.0
176.90	3014.0
178.00	349.0
178.90	901.0
179.90	171.0
180.80	153.0
189.00	367.0
190.90	3029.0
192.00	562.0
192.90	3835.0
193.90	668.0
194.90	395.0
202.90	513.0
204.10	150.0
205.00	865.0
205.80	196.0
207.00	2530.0
208.00	444.0
209.00	327.0
218.90	70.0
220.90	190.0
223.00	60.0
234.00	69.0
234.90	504.0
235.90	99.0
236.00	104.0
236.90	140.0
246.90	96.0
248.90	3257.0
249.90	844.0
250.90	1451.0
252.00	251.0
252.90	181.0
265.00	3532.0
266.00	1194.0
267.00	810.0
267.90	204.0
268.50	54.0
269.00	74.0
279.10	107.0
281.00	53416.0
282.00	15808.0
283.00	9429.0
284.00	1838.0
284.90	514.0
286.00	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

m/z	Abundance
36.00	316.0
37.00	2082.0
38.00	1872.0
39.00	857.0
40.00	129.0
41.10	60.0
43.00	168.0
44.00	554.0
45.00	683.0
45.90	70.0
46.90	290.0
48.00	280.0
49.00	1619.0
50.00	8632.0
51.00	2731.0
51.90	155.0
54.90	187.0
56.00	703.0
57.00	1331.0
58.10	123.0
59.10	420.0
60.00	496.0
61.00	2378.0
62.00	2266.0
63.00	1564.0
64.00	182.0
66.90	161.0
68.00	4325.0
69.00	4711.0
70.00	333.0
71.90	233.0
73.00	4036.0
74.00	7971.0
75.00	23128.0
76.00	2215.0
77.00	211.0
78.00	117.0
78.90	1527.0
79.90	491.0
80.90	1737.0
81.90	405.0
82.90	57.0
87.00	2034.0
87.90	1934.0
88.90	112.0
90.90	199.0
92.00	1486.0
93.00	2144.0
94.00	5913.0
95.00	44808.0
96.00	3353.0
97.00	122.0
102.90	358.0
103.90	383.0
104.90	145.0
105.90	252.0
106.80	64.0
109.90	142.0
110.90	174.0
111.90	108.0
115.00	196.0
115.90	226.0
116.90	511.0
118.00	359.0
118.80	664.0
125.00	687.0
126.10	101.0
127.80	171.0
128.90	93.0
129.90	190.0
130.90	135.0
131.90	72.0
133.00	2037.0
134.90	264.0
136.90	90.0
141.00	506.0
141.90	81.0
143.00	460.0
144.90	99.0
145.90	111.0
146.90	358.0
147.90	159.0
148.90	139.0
149.80	103.0
154.70	112.0
157.00	81.0
158.90	79.0
160.80	221.0
162.90	451.0
163.90	82.0
164.90	307.0
167.00	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

168.80	152.0
173.90	41968.0
175.00	3143.0
175.90	41680.0
176.90	3550.0
177.90	312.0
178.90	590.0
179.90	118.0
181.00	115.0
189.00	175.0
190.10	109.0
190.90	2064.0
191.90	431.0
193.00	2772.0
193.90	453.0
194.90	293.0
203.00	288.0
204.10	81.0
204.90	572.0
206.10	109.0
207.00	1905.0
207.90	339.0
208.80	177.0
220.90	108.0
234.80	237.0
235.00	237.0
237.10	79.0
246.70	66.0
249.00	2156.0
250.00	600.0
250.90	980.0
251.90	262.0
252.90	109.0
265.00	2748.0
265.90	810.0
266.90	594.0
267.90	147.0
268.90	95.0
279.30	87.0
281.00	41048.0
281.90	10565.0
282.90	6489.0
284.00	1513.0
285.00	486.0
286.00	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

m/z	Abundance
35.90	339.0
37.00	1893.0
38.00	1678.0
39.00	721.0
40.00	156.0
43.00	62.0
44.00	474.0
45.00	423.0
46.90	321.0
48.00	210.0
49.00	1661.0
50.00	7106.0
51.00	2264.0
51.90	111.0
54.90	94.0
56.00	689.0
57.00	1170.0
57.90	58.0
59.00	112.0
60.00	328.0
61.00	1769.0
62.00	2111.0
63.00	1506.0
64.10	177.0
67.00	202.0
68.00	4317.0
69.00	4386.0
69.90	334.0
71.90	268.0
73.00	2514.0
74.00	6743.0
75.00	20360.0
76.00	1865.0
77.10	238.0
77.90	199.0
78.90	1404.0
79.90	444.0
80.90	1423.0
81.90	313.0
85.70	53.0
86.90	1695.0
87.90	1714.0
88.70	105.0
90.90	170.0
92.00	1265.0
93.00	1678.0
94.00	5423.0
95.00	41656.0
96.00	2413.0
96.90	108.0
103.00	159.0
103.90	218.0
104.90	112.0
105.90	261.0
111.00	143.0
112.00	62.0
114.90	131.0
115.90	217.0
117.00	307.0
117.90	261.0
119.00	436.0
125.10	208.0
127.80	207.0
128.90	58.0
129.80	179.0
130.90	81.0
133.00	1015.0
133.70	280.0
134.90	192.0
137.00	105.0
140.90	460.0
142.90	464.0
144.80	76.0
145.80	70.0
146.70	235.0
148.10	86.0
149.00	64.0
149.80	56.0
154.70	68.0
155.00	71.0
157.10	67.0
158.80	70.0
161.00	128.0
162.90	154.0
165.10	118.0
169.00	194.0
172.10	99.0
173.90	41368.0
174.90	3290.0
175.90	41256.0
176.90	3017.0
177.90	142.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

178.90	285.0
180.00	69.0
188.90	175.0
191.00	1086.0
192.00	210.0
193.00	1317.0
194.00	217.0
195.00	166.0
203.00	165.0
204.90	361.0
206.90	1069.0
207.80	177.0
208.90	110.0
220.90	60.0
235.00	197.0
248.90	1309.0
249.90	329.0
251.00	534.0
252.00	181.0
265.00	1500.0
265.90	412.0
266.90	384.0
267.90	131.0
278.90	87.0
281.00	23464.0
282.00	6103.0
283.00	3720.0
283.90	777.0
285.00	242.0
286.10	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

Scan 1749 (12.566 min): VW015374.D
BFB26

m/z	Abundance
39.90	129.0
41.20	52.0
44.00	206.0
55.00	88.0
69.00	104.0
73.10	56.0
119.10	64.0
146.90	103.0
169.00	221.0
280.90	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26