

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042921\
 Data File : VW018842.D
 Acq On : 29 Apr 2021 13:42
 Operator : SY/VA
 Sample : VW0429SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK111

Manual Integrations
 APPROVED

MMDadoda
 4/30/2021 4:52:17 PM

Quant Time: Apr 30 02:10:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 02:09:50 2021
 Response via : Initial Calibration

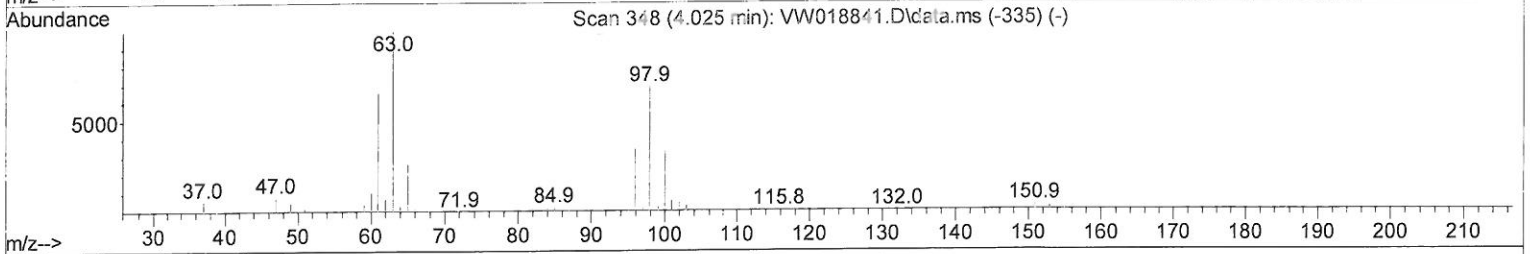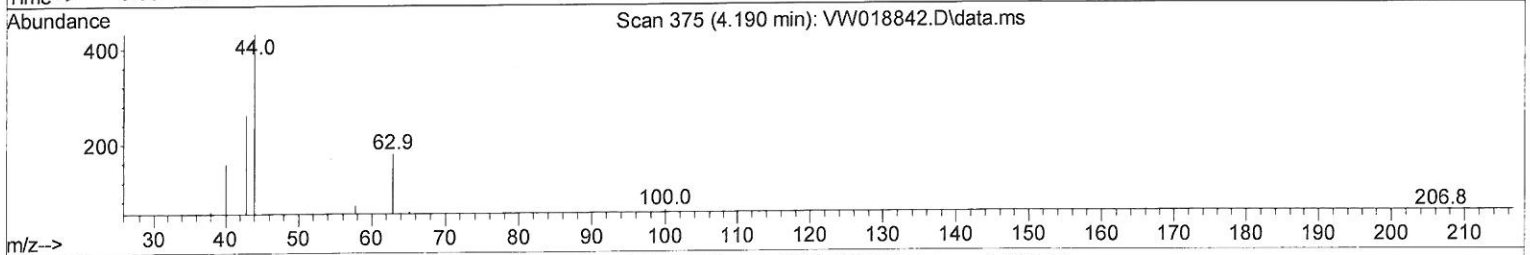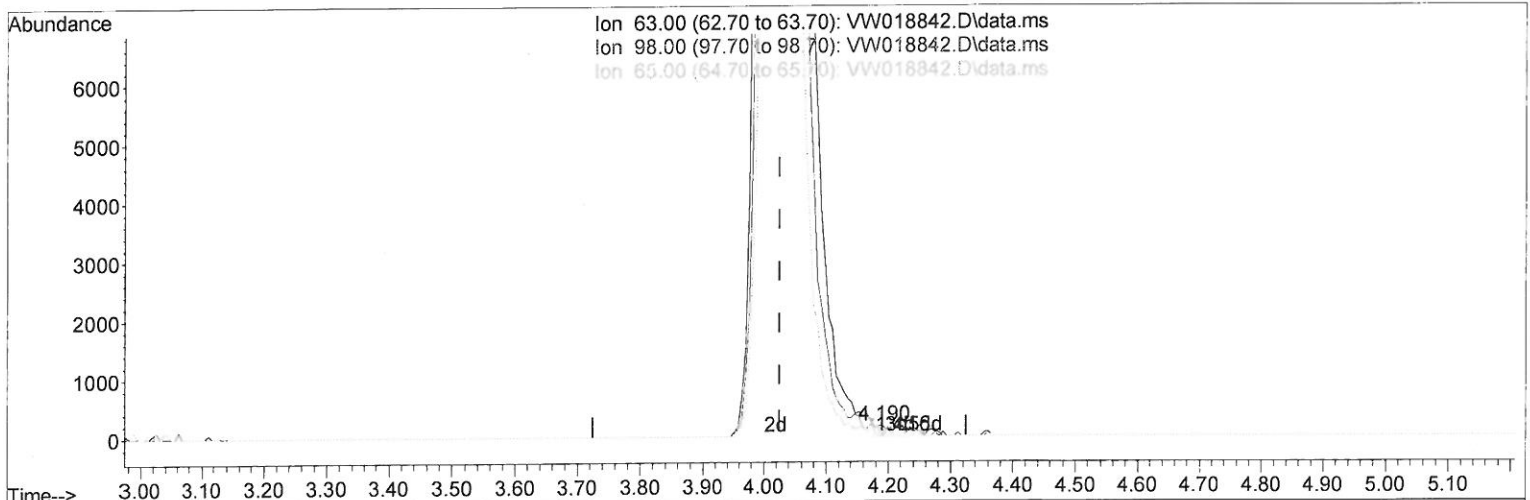

TIC: VW018842.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.190min (+ 0.164) 0.02 ug/L

response 249

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.20	88.76
65.00	23.70	27.31
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042921\
 Data File : VW018842.D
 Acq On : 29 Apr 2021 13:42
 Operator : SY/VA
 Sample : VW0429SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK111

Manual Integrations
 APPROVED

MMDadoda
 4/30/2021 4:52:17 PM

Quant Time: Apr 30 02:10:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 02:09:50 2021
 Response via : Initial Calibration

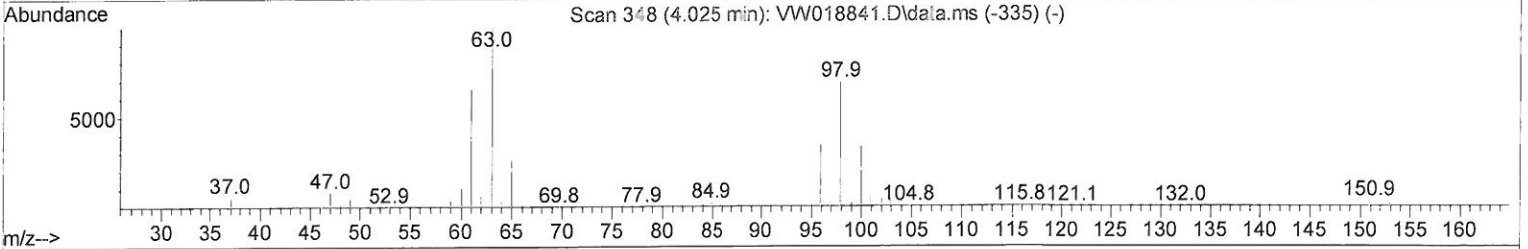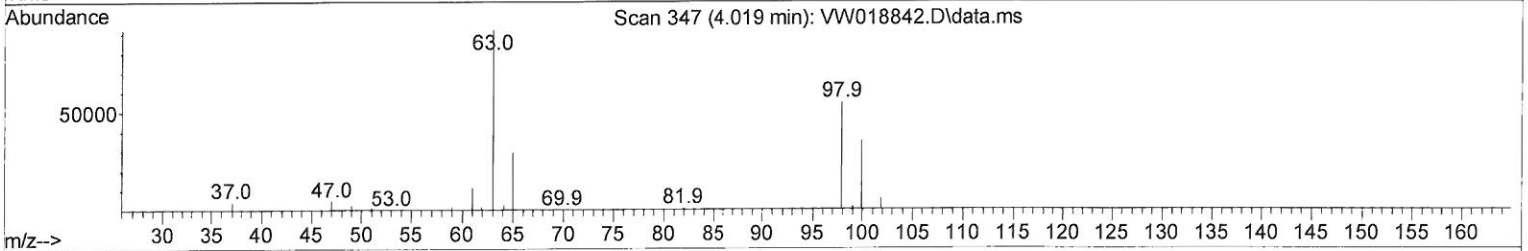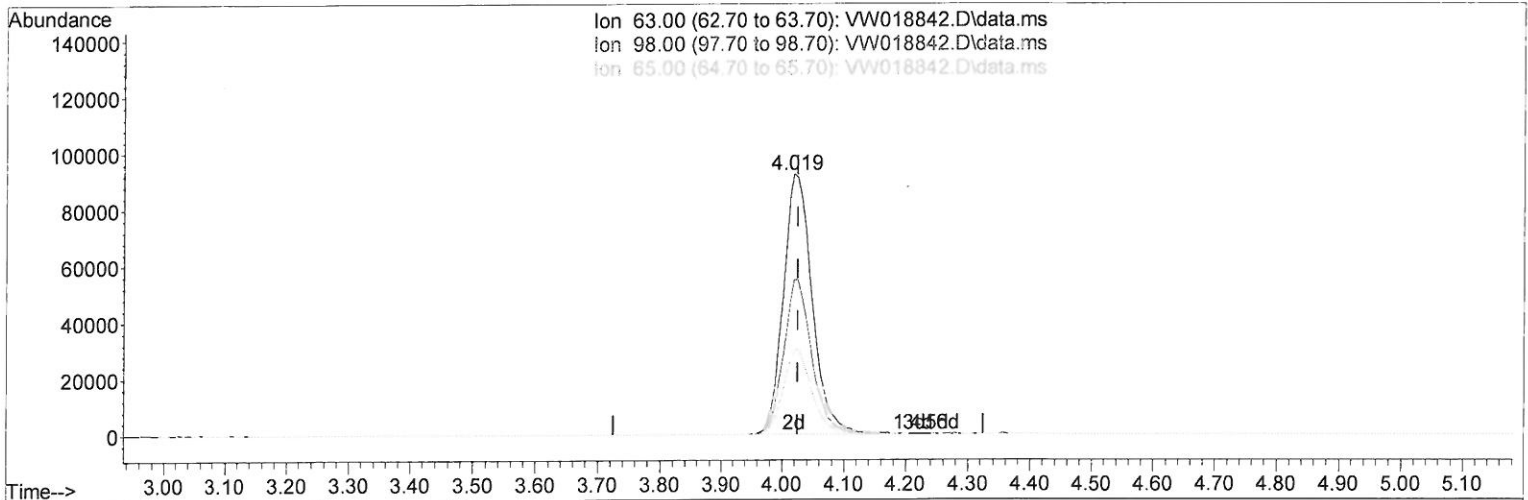

TIC: VW018842.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.006) 19.74 ug/L m

response 297246

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.20	0.07#
65.00	23.70	0.02#
0.00	0.00	0.00

04/30/2021 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042921\
 Data File : VW018842.D
 Acq On : 29 Apr 2021 13:42
 Operator : SY/VA
 Sample : VW0429SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK111

Manual Integrations
 APPROVED

MMDadoda
 4/30/2021 4:52:17 PM

Quant Time: Apr 30 02:10:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 02:09:50 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene		8.841	114	591013	25.00	ug/L	0.00
28) Chlorobenzene-d5		11.634	117	529667	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.560	152	259186	25.00	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.361	65	205821	27.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.60%	
7) Chloroethane-d5		2.891	69	156317	26.61	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.44%	
11) 1,1-Dichloroethene-d2		4.019	63	297246m	19.74	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.96%	
21) 2-Butanone-d5		7.086	46	110646	56.03	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.06%	
24) Chloroform-d		7.653	84	403956	26.04	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.16%	
26) 1,2-Dichloroethane-d4		8.305	65	234559	27.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.28%	
32) Benzene-d6		8.281	84	817103	27.30	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.20%	
36) 1,2-Dichloropropane-d6		9.274	67	244372	27.52	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.08%	
41) Toluene-d8		10.323	98	748260	26.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	107.24%	
43) trans-1,3-Dichloroprop...		10.579	79	108193	26.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	107.24%	
47) 2-Hexanone-d5		10.926	63	93659	58.92	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.84%	
56) 1,1,2,2-Tetrachloroeth...		12.694	84	208738	27.75	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.00%	
66) 1,2-Dichlorobenzene-d4		13.853	152	251419	28.31	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	113.24%	
Target Compounds							Qvalue
16) Methylene chloride		4.921	84	25412	2.60	ug/L	95
42) Toluene		10.390	91	13890	0.40	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042921\
Data File : VW018842.D
Acq On : 29 Apr 2021 13:42
Operator : SY/VA
Sample : VW0429SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK111

Manual Integrations
APPROVED

MMDadoda
4/30/2021 4:52:17 PM

Quant Time: Apr 30 02:10:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 30 02:09:50 2021
Response via : Initial Calibration

