

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042921\
 Data File : VW018844.D
 Acq On : 29 Apr 2021 14:42
 Operator : SY/VA
 Sample : M2177-18
 Misc : 6.45G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG588

Quant Time: Apr 30 02:10:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 02:09:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	657295	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	580768	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	258796	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	217682	25.81	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 103.24%			
7) Chloroethane-d5	2.892	69	170100	26.04	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 104.16%			
11) 1,1-Dichloroethene-d2	4.025	63	325155	19.42	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 77.68%			
21) 2-Butanone-d5	7.080	46	89445	40.73	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 81.46%			
24) Chloroform-d	7.647	84	436700	25.31	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 101.24%			
26) 1,2-Dichloroethane-d4	8.311	65	239458	24.85	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 99.40%			
32) Benzene-d6	8.275	84	897393	27.35	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 109.40%			
36) 1,2-Dichloropropane-d6	9.275	67	264323	27.15	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 108.60%			
41) Toluene-d8	10.323	98	834836	27.28	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 109.12%			
43) trans-1,3-Dichloroprop...	10.579	79	105102	23.76	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 95.04%			
47) 2-Hexanone-d5	10.927	63	77851	44.66	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 89.32%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	182167	22.08	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 88.32%			
66) 1,2-Dichlorobenzene-d4	13.853	152	231399	26.09	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 104.36%			
Target Compounds					Qvalue	
13) Acetone	4.141	43	9169	5.45	ug/L	84
14) Carbon disulfide	4.385	76	24365	0.97	ug/L #	90
16) Methylene chloride	4.916	84	48415	4.46	ug/L	89
42) Toluene	10.390	91	15074	0.39	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042921\
Data File : VW018844.D
Acq On : 29 Apr 2021 14:42
Operator : SY/VA
Sample : M2177-18
Misc : 6.45G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG588

Quant Time: Apr 30 02:10:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 30 02:09:50 2021
Response via : Initial Calibration




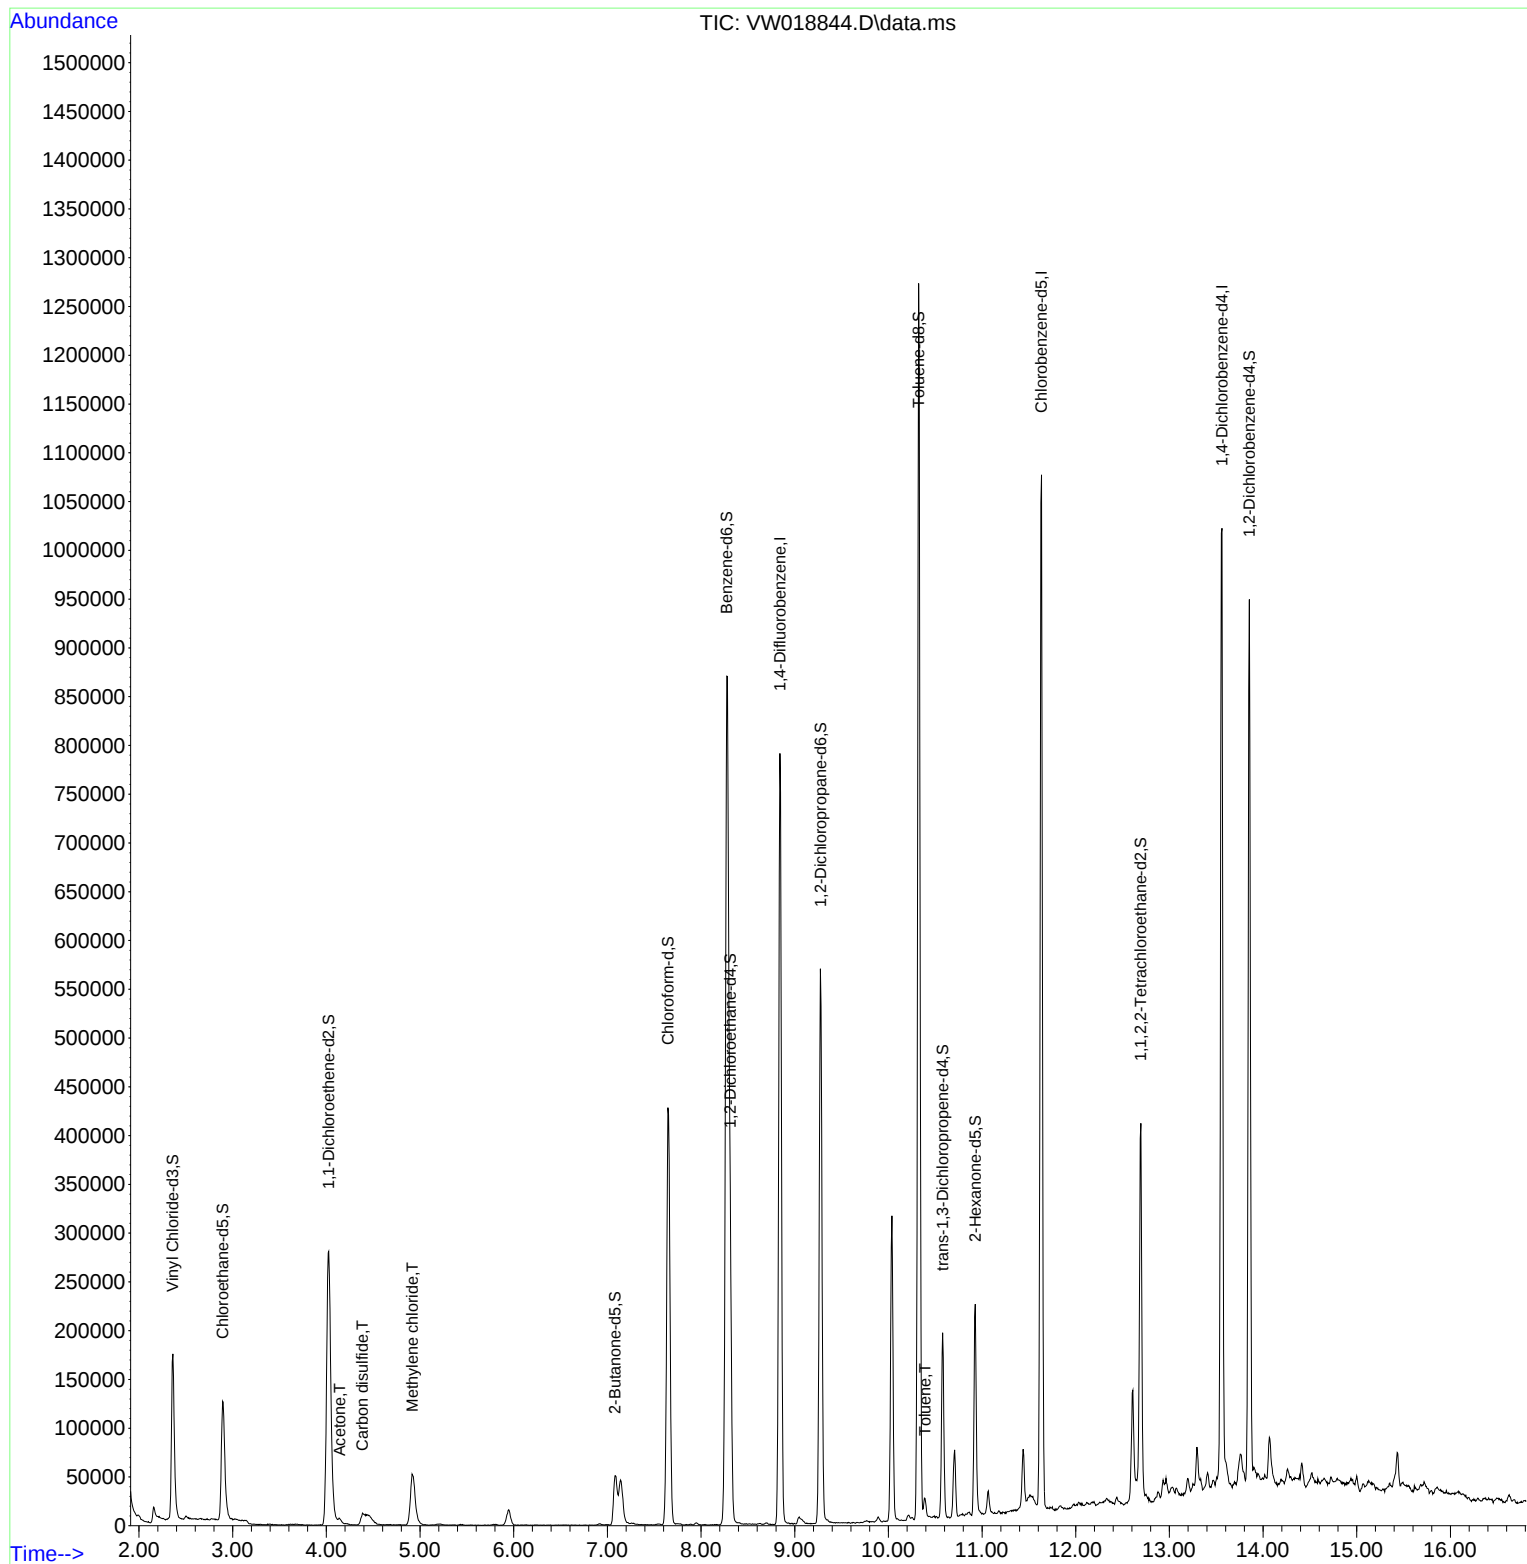


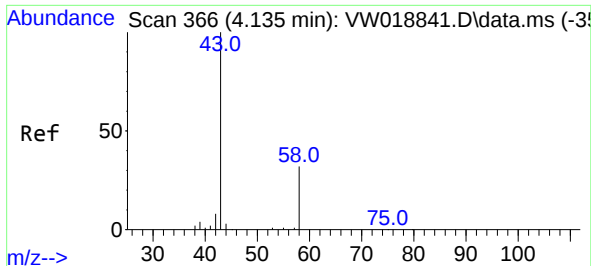

#13
Acetone
Concen: 5.45 ug/L
RT: 4.141 min Scan# 367
Delta R.T. 0.006 min
Lab File: VW018844.D
Acq: 29 Apr 2021 14:42




Instrument :
MSVOA_W
ClientSampled :
BG588


Tgt Ion: 43 Resp: 9169
Ion Ratio Lower Upper
43 100
58 35.2 0.0 53.8

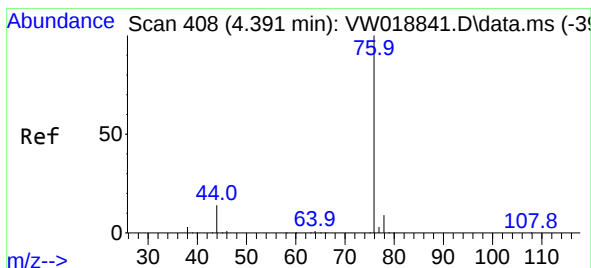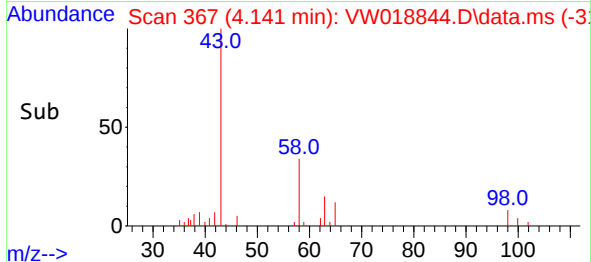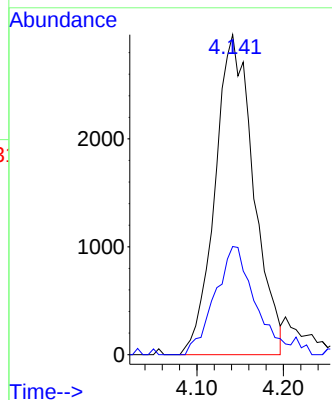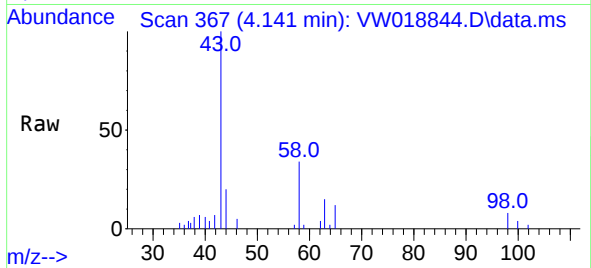

#14
Carbon disulfide
Concen: 0.97 ug/L
RT: 4.385 min Scan# 407
Delta R.T. -0.006 min
Lab File: VW018844.D
Acq: 29 Apr 2021 14:42

Tgt Ion: 76 Resp: 24365
Ion Ratio Lower Upper
76 100
78 12.8 7.4 11.0#


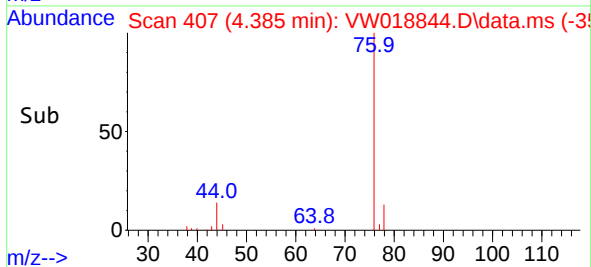
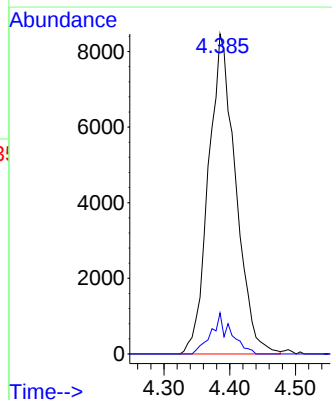
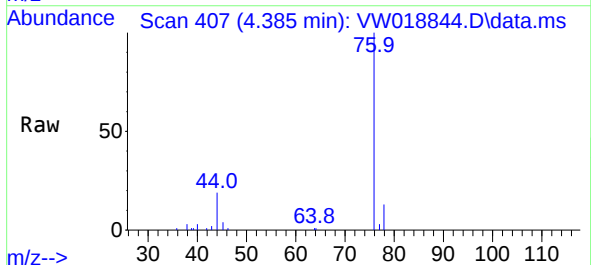


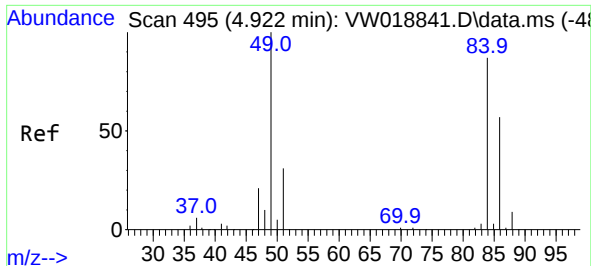

#16
Methylene chloride
Concen: 4.46 ug/L
RT: 4.916 min Scan# 494
Delta R.T. -0.006 min
Lab File: VW018844.D
Acq: 29 Apr 2021 14:42

Instrument :
MSVOA_W
ClientSampleId :
BG588

Tgt Ion: 84 Resp: 48415
Ion Ratio Lower Upper
84 100
86 63.2 45.3 84.1
49 105.3 86.6 160.8

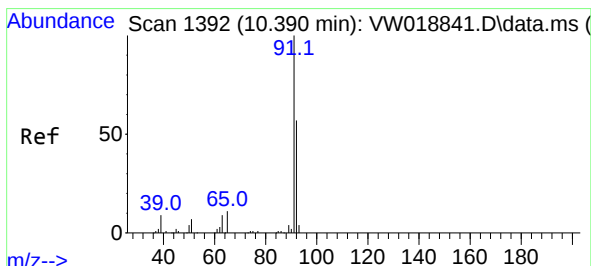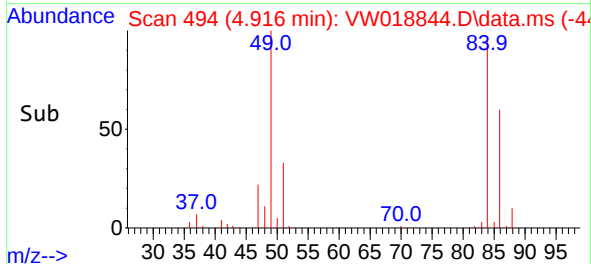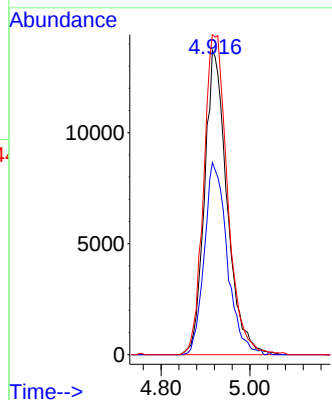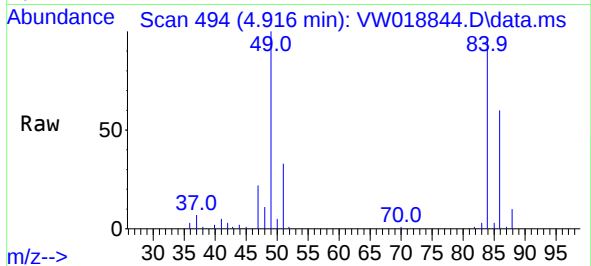

#42
Toluene
Concen: 0.39 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. 0.000 min
Lab File: VW018844.D
Acq: 29 Apr 2021 14:42

Tgt Ion: 91 Resp: 15074
Ion Ratio Lower Upper
91 100
92 52.9 39.5 73.3

