

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW043021\
 Data File : VW018876.D
 Acq On : 30 Apr 2021 13:10
 Operator : SY/VA
 Sample : M2232-11
 Misc : 5.34G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5A1

Manual Integrations
 APPROVED

MMDadoda
 5/3/2021 2:52:50 PM

Quant Time: Apr 30 22:55:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 22:53:19 2021
 Response via : Initial Calibration

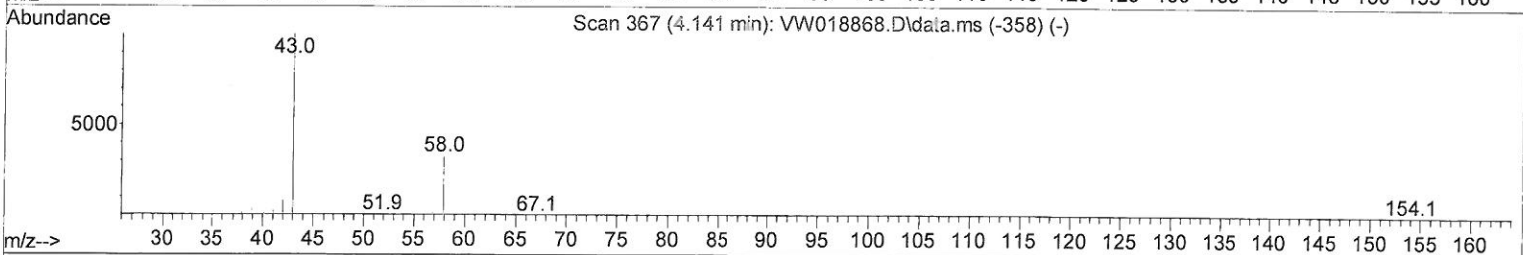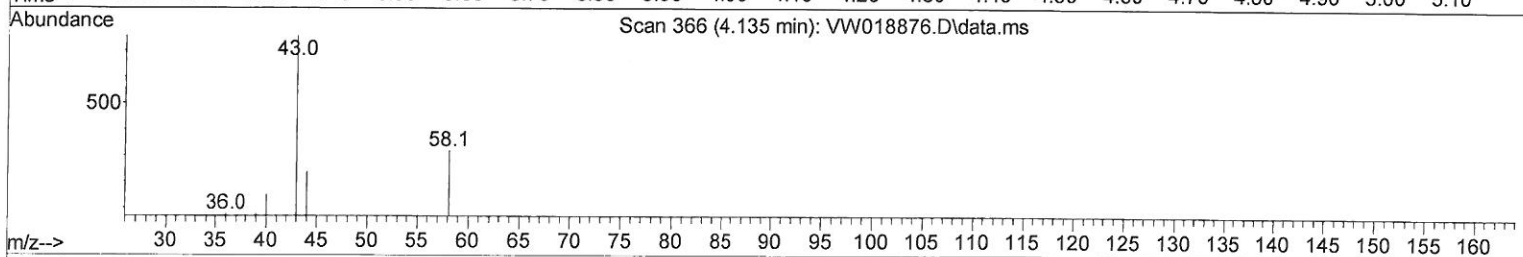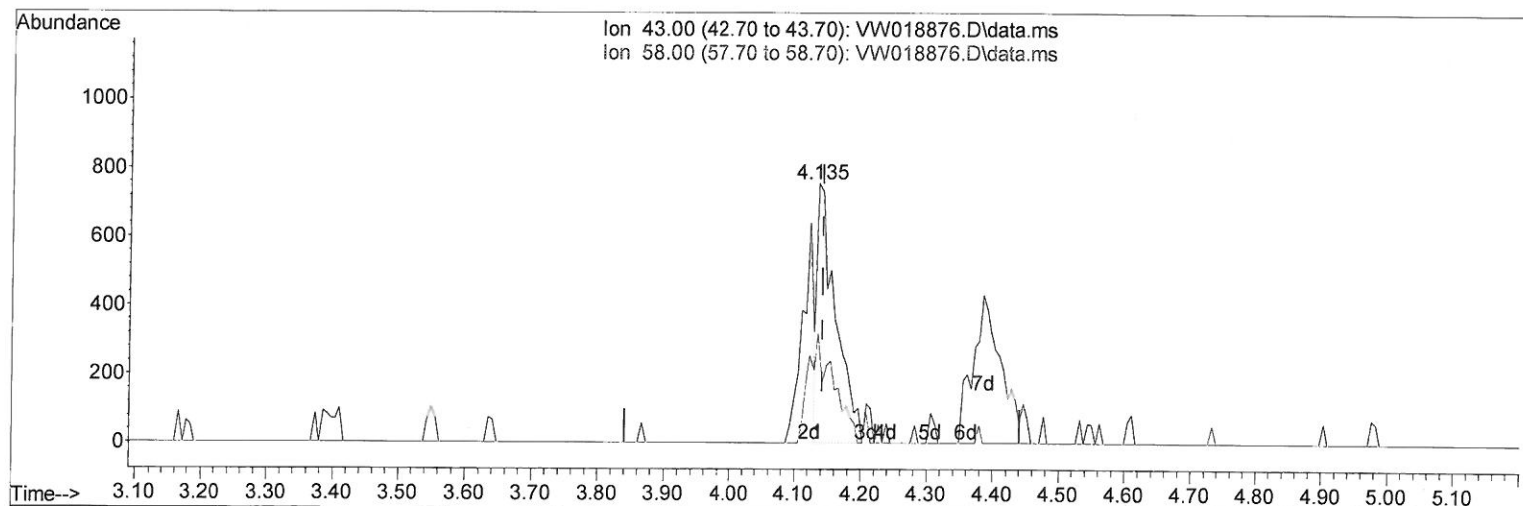

TIC: VW018876.D\data.ms

(13) Acetone (T)

4.135min (-0.006) 9.52 ug/L

response 1446

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	12.59
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW043021\
 Data File : VW018876.D
 Acq On : 30 Apr 2021 13:10
 Operator : SY/VA
 Sample : M2232-11
 Misc : 5.34G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5A1

Manual Integrations
 APPROVED

MMDadoda
 5/3/2021 2:52:50 PM

Quant Time: Apr 30 22:55:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 22:53:19 2021
 Response via : Initial Calibration

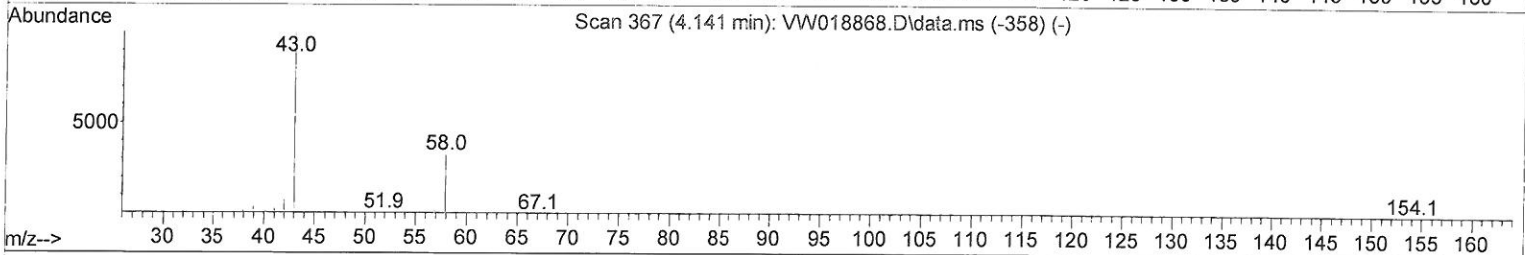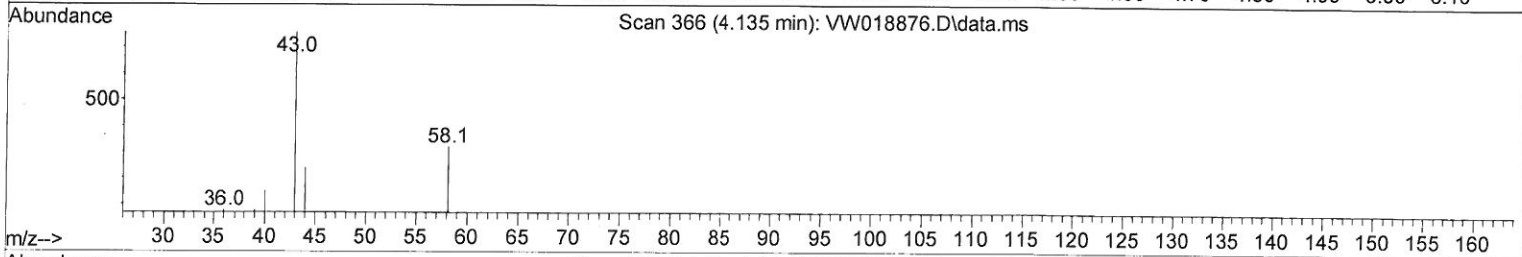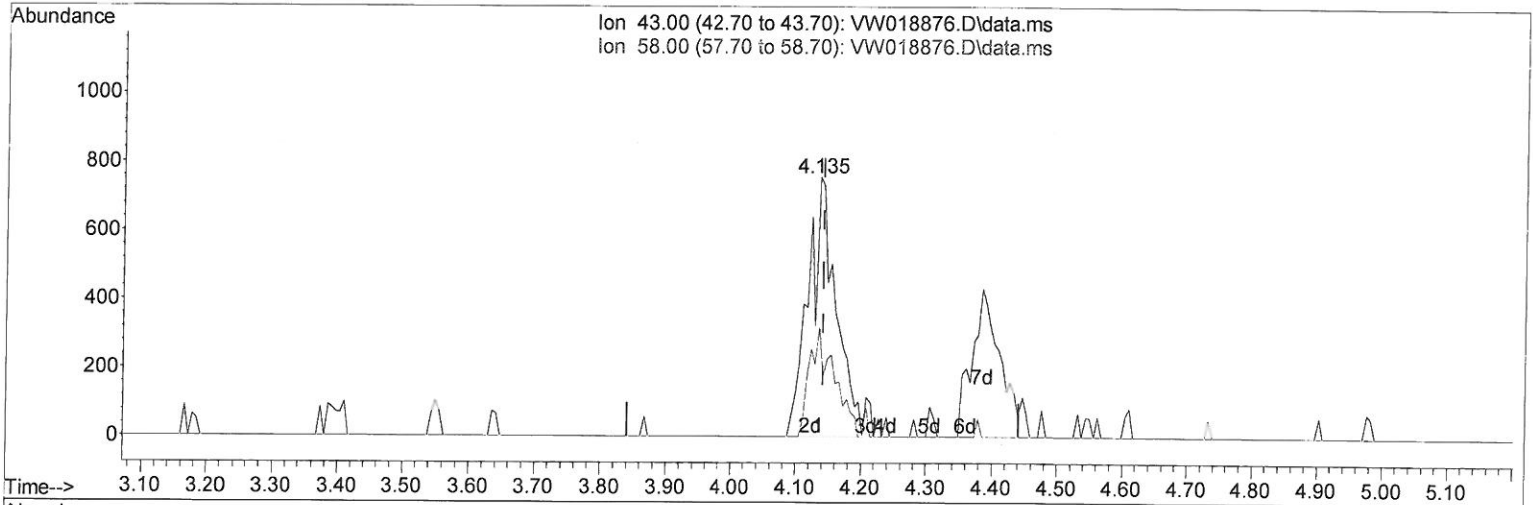

TIC: VW018876.D\data.ms

(13) Acetone (T)

4.135min (-0.006) 14.62 ug/L m

505/03/21 Sy

response 2219

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	8.20
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW043021\
 Data File : VW018876.D
 Acq On : 30 Apr 2021 13:10
 Operator : SY/VA
 Sample : M2232-11
 Misc : 5.34G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5A1

Manual Integrations
 APPROVED

MMDadoda
 5/3/2021 2:52:50 PM

Quant Time: Apr 30 22:55:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 22:53:19 2021
 Response via : Initial Calibration

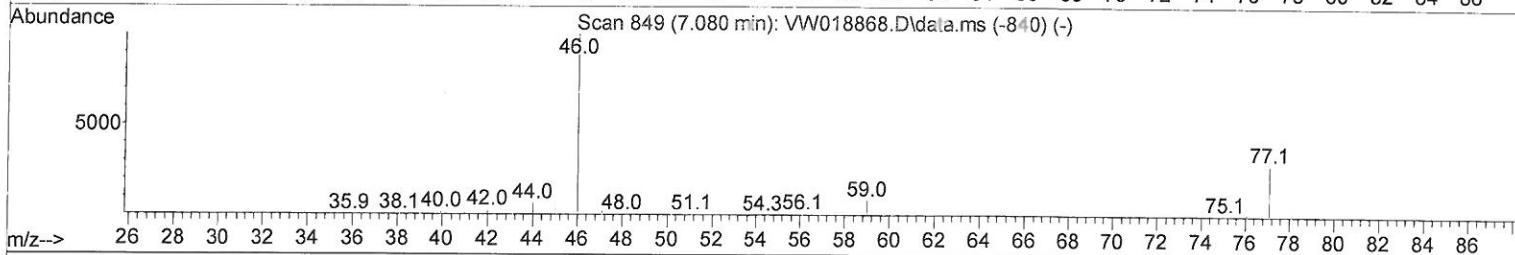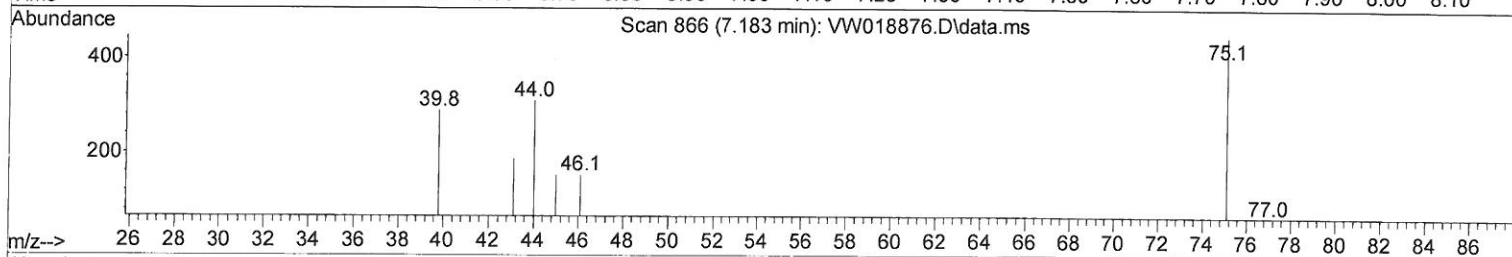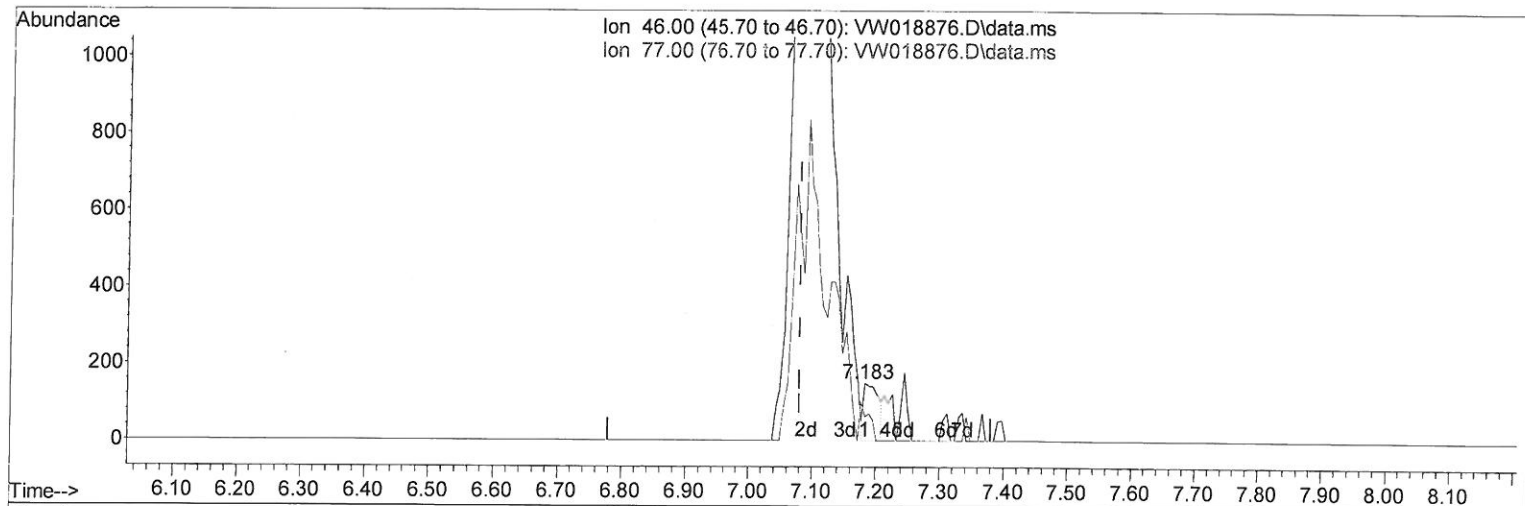

TIC: VW018876.D\data.ms

(21) 2-Butanone-d5 (S)

7.183min (+ 0.103) 1.22 ug/L

response 242

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	26.80	24.79
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW043021\
 Data File : VW018876.D
 Acq On : 30 Apr 2021 13:10
 Operator : SY/VA
 Sample : M2232-11
 Misc : 5.34G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5A1

Manual Integrations
 APPROVED

MMDadoda
 5/3/2021 2:52:50 PM

Quant Time: Apr 30 22:55:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 22:53:19 2021
 Response via : Initial Calibration

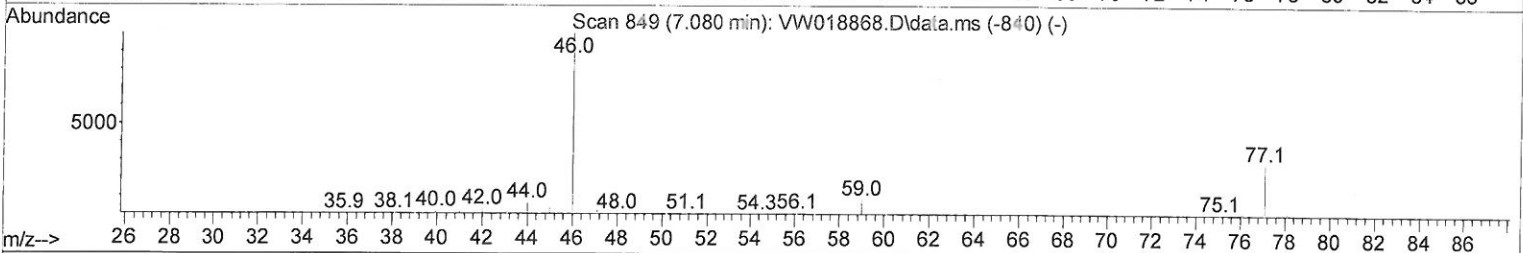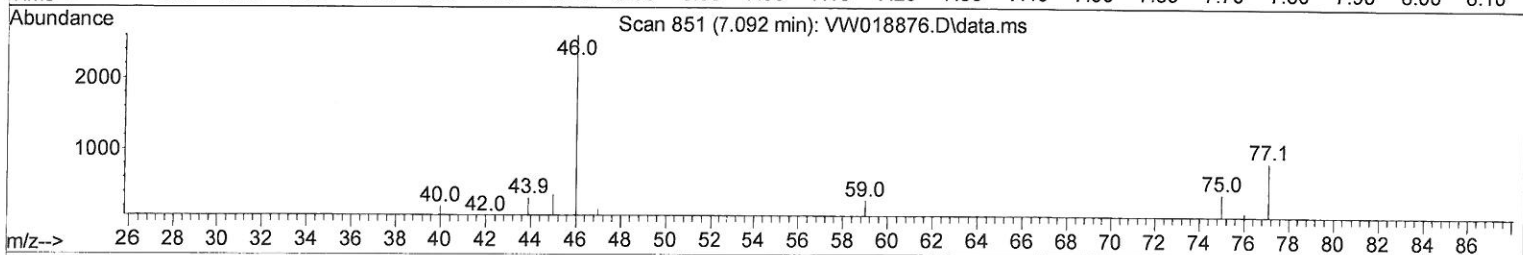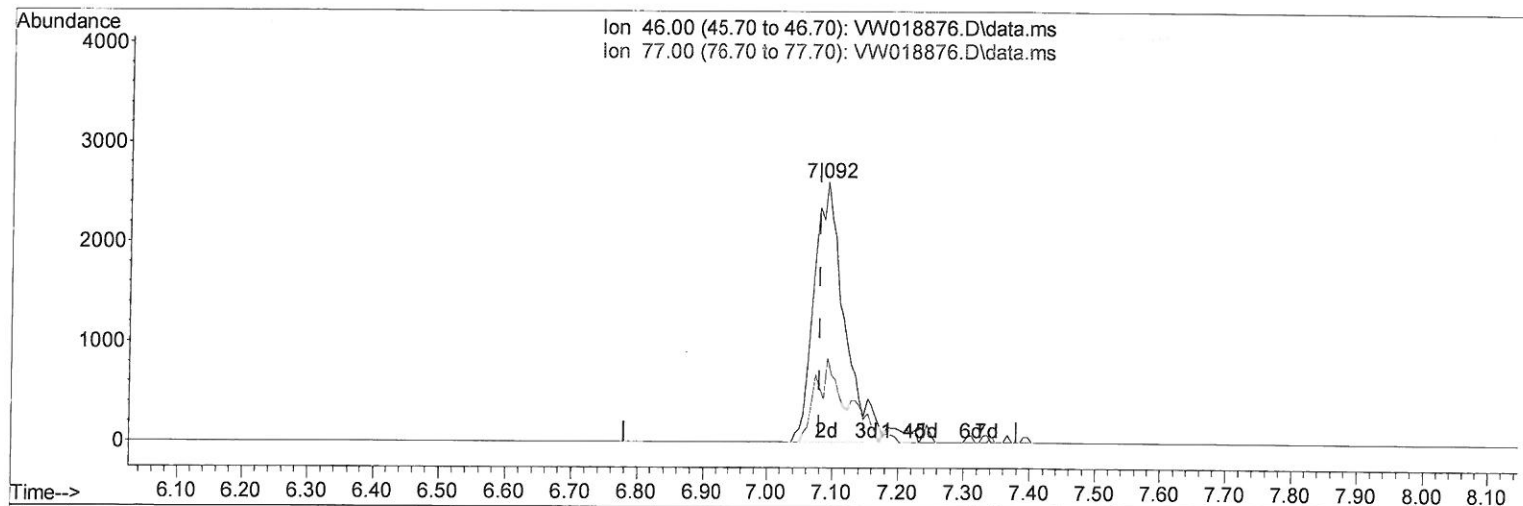

TIC: VW018876.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.012) 40.22 ug/L m

response 7970

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	26.80	0.75#
0.00	0.00	0.00
0.00	0.00	0.00

05/03/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW043021\
 Data File : VW018876.D
 Acq On : 30 Apr 2021 13:10
 Operator : SY/VA
 Sample : M2232-11
 Misc : 5.34G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5A1

Manual Integrations
 APPROVED

MMDadoda
 5/3/2021 2:52:50 PM

Quant Time: Apr 30 22:55:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 22:53:19 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	59309	25.00	ug/L	0.00
28) Chlorobenzene-d5		11.634	117	44766	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.560	152	13844	25.00	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.355	65	20822	27.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.48%	
7) Chloroethane-d5		2.891	69	16989	28.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.28%	
11) 1,1-Dichloroethene-d2		4.025	63	29978	19.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.36%	
21) 2-Butanone-d5		7.092	46	7970m	40.22	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.44%	
24) Chloroform-d		7.653	84	36430	23.40	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.60%	
26) 1,2-Dichloroethane-d4		8.311	65	20567	23.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.60%	
32) Benzene-d6		8.275	84	75627	29.90	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	119.60%	
36) 1,2-Dichloropropane-d6		9.274	67	21668	28.88	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.52%	
41) Toluene-d8		10.323	98	63228	26.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	107.20%	
43) trans-1,3-Dichloroprop...		10.579	79	5938	17.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.64%	
47) 2-Hexanone-d5		10.927	63	6559	48.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.64%	
56) 1,1,2,2-Tetrachloroeth...		12.695	84	14526	22.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.40%	
66) 1,2-Dichlorobenzene-d4		13.853	152	11268	23.75	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.00%	
Target Compounds							Qvalue
13) Acetone		4.135	43	2219m	14.62	ug/L	
14) Carbon disulfide		4.391	76	8539	3.76	ug/L	100
16) Methylene chloride		4.928	84	3682	3.76	ug/L	93
42) Toluene		10.390	91	1381	0.47	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW043021\
Data File : VW018876.D
Acq On : 30 Apr 2021 13:10
Operator : SY/VA
Sample : M2232-11
Misc : 5.34G/10ML/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG5A1

Manual Integrations
APPROVED

MMDadoda
5/3/2021 2:52:50 PM

Quant Time: Apr 30 22:55:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 30 22:53:19 2021
Response via : Initial Calibration

