

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW043021\
 Data File : VW018884.D
 Acq On : 30 Apr 2021 16:21
 Operator : SY/VA
 Sample : VIBLK101
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK101

Quant Time: Apr 30 22:56:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 30 22:53:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	641321	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	593384	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	269423	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	159091	19.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.36%
7) Chloroethane-d5	2.897	69	131701	20.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.64%
11) 1,1-Dichloroethene-d2	4.025	63	251835	15.42	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.68%
21) 2-Butanone-d5	7.086	46	94629	44.16	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.32%
24) Chloroform-d	7.653	84	364064	21.63	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.52%
26) 1,2-Dichloroethane-d4	8.311	65	214572	22.82	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.28%
32) Benzene-d6	8.274	84	738955	22.04	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.16%
36) 1,2-Dichloropropane-d6	9.274	67	221468	22.27	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.08%
41) Toluene-d8	10.323	98	690393	22.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.32%
43) trans-1,3-Dichloroprop...	10.579	79	94166	20.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.32%
47) 2-Hexanone-d5	10.926	63	79839	44.83	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.66%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	185530	22.01	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.04%
66) 1,2-Dichlorobenzene-d4	13.853	152	223384	24.20	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.80%
Target Compounds						
16) Methylene chloride	4.921	84	40199	3.79	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW043021\
Data File : VW018884.D
Acq On : 30 Apr 2021 16:21
Operator : SY/VA
Sample : VIBLK101
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK101


Quant Time: Apr 30 22:56:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 30 22:53:19 2021
Response via : Initial Calibration

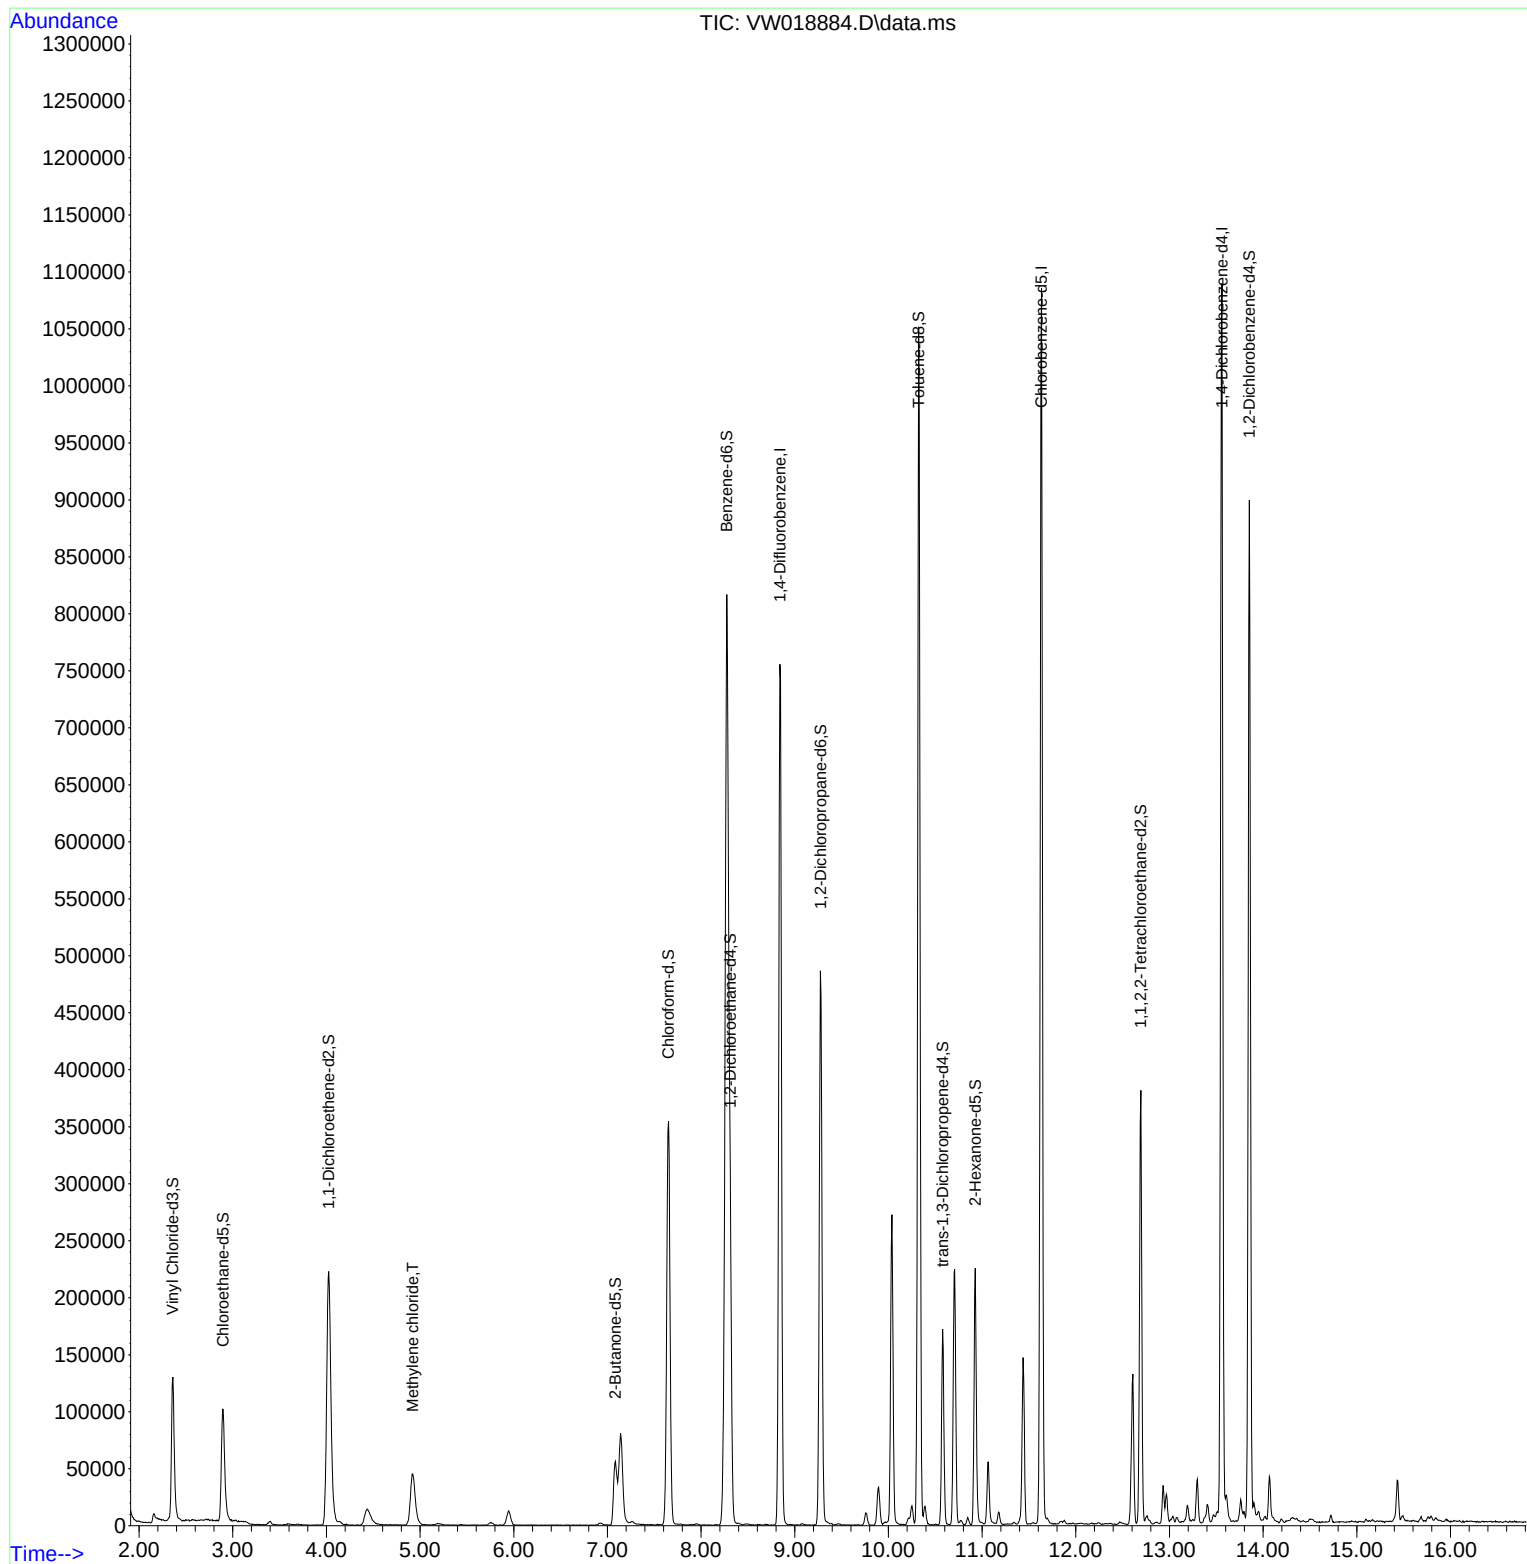

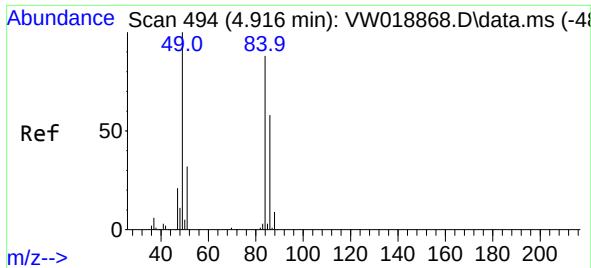

#16
Methylene chloride
Concen: 3.79 ug/L
RT: 4.921 min Scan# 495
Delta R.T. 0.006 min
Lab File: VW018884.D
Acq: 30 Apr 2021 16:21

Instrument :
MSVOA_W
ClientSampleId :
VIBLK101

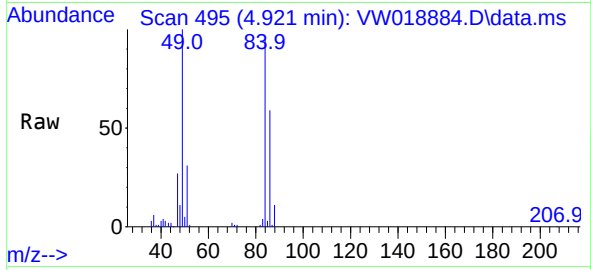

Tgt Ion:	84	Resp:	40199
Ion	Ratio	Lower	Upper
84	100		
86	62.4	45.3	84.1
49	105.8	86.6	160.8

