




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025779.D
 Acq On : 01 May 2023 15:41
 Operator : SY/MD
 Sample : VW0501SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK492

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

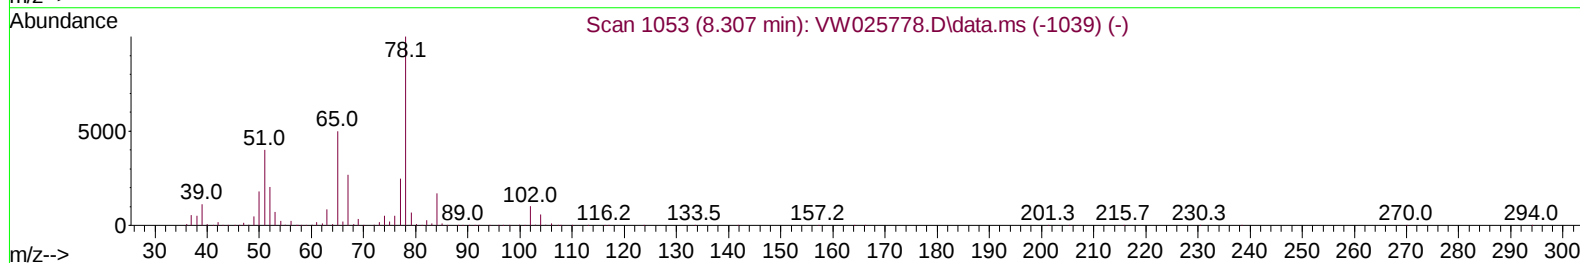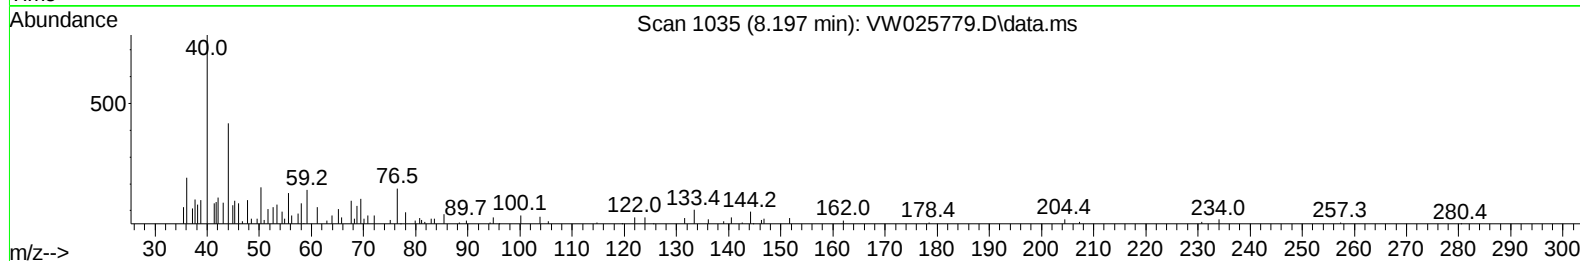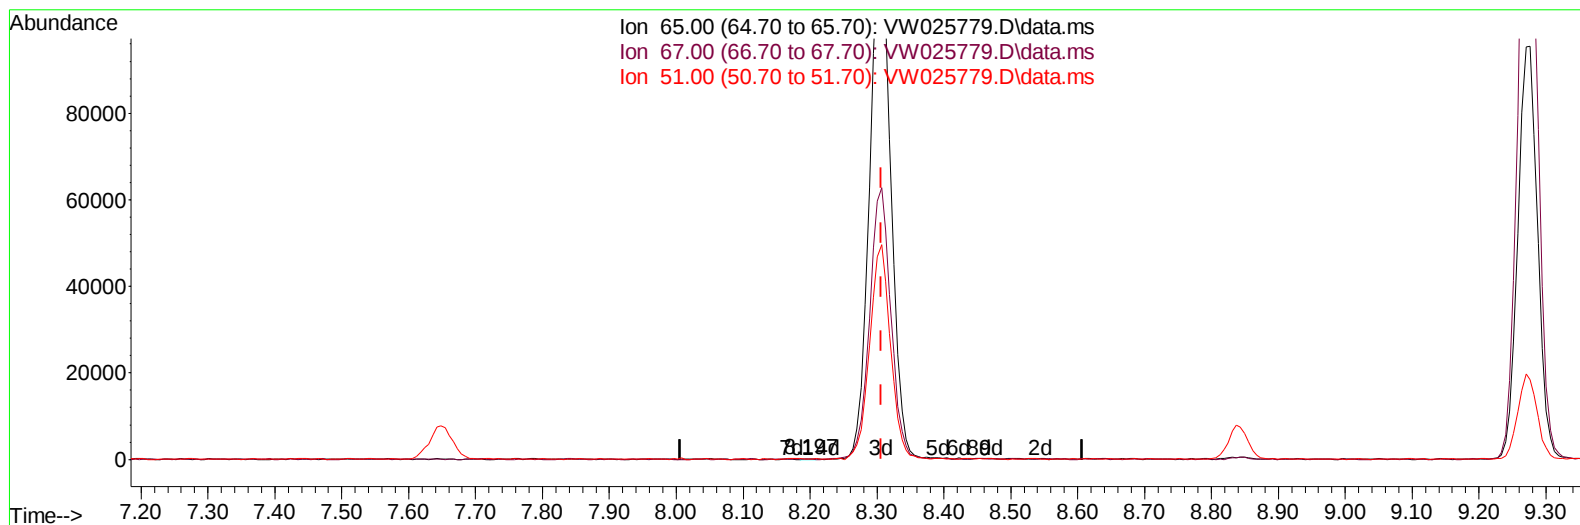

TIC: VW025779.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.197min (-0.110) 0.01 ug/L

response 131

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	66.41
51.00	112.30	118.32
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025779.D
 Acq On : 01 May 2023 15:41
 Operator : SY/MD
 Sample : VW0501SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK492

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

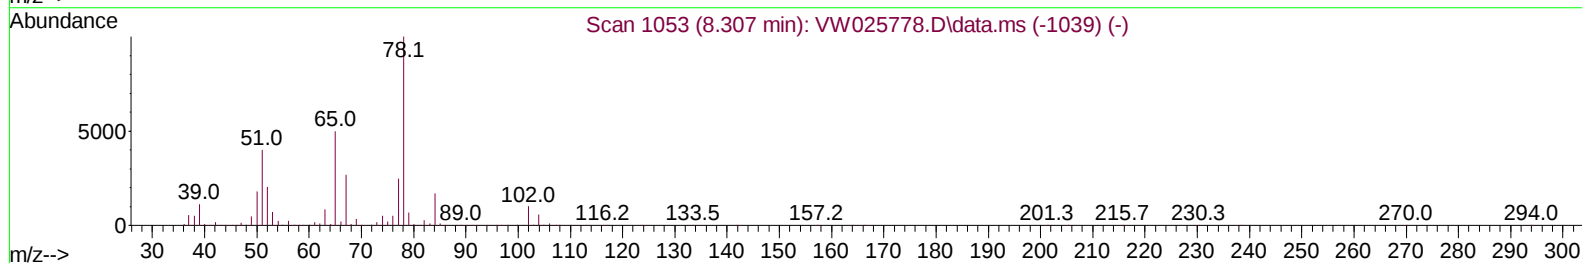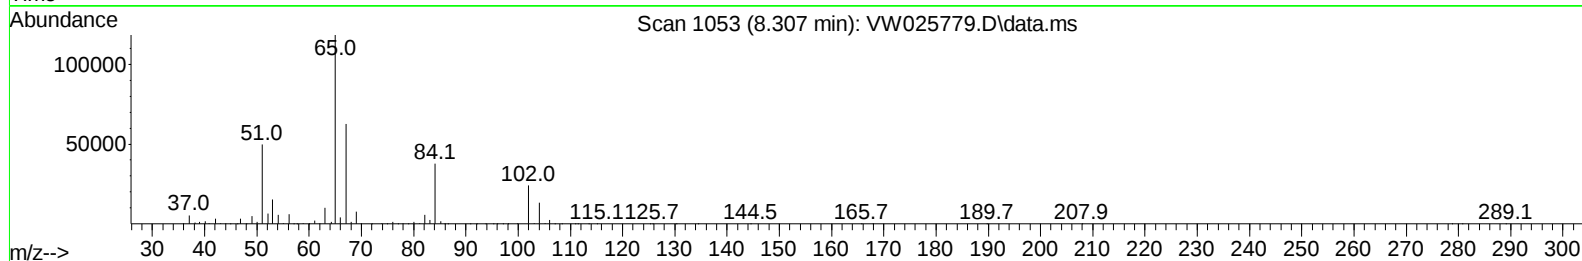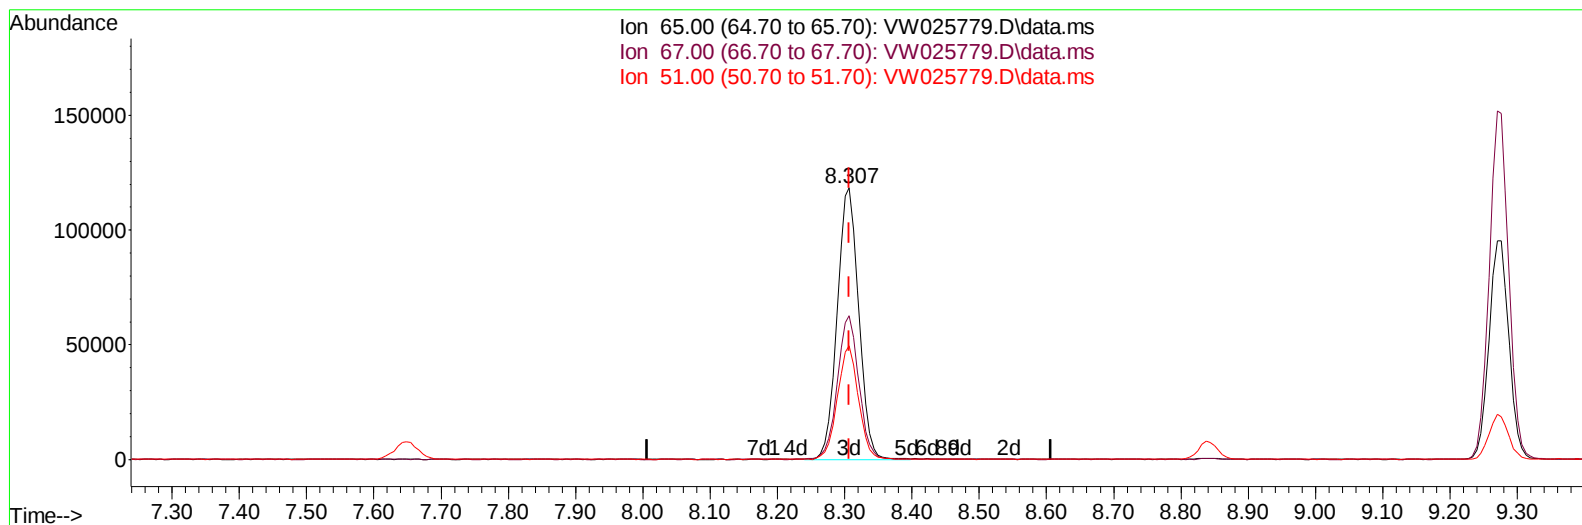

TIC: VW025779.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 25.20 ug/L m

response 262786

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.03#
51.00	112.30	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025779.D
 Acq On : 01 May 2023 15:41
 Operator : SY/MD
 Sample : VW0501SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK492

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		639491	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		567745	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		257393	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		243321	26.851	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	107.400%	
7) Chloroethane-d5	2.899	69		180212	26.824	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	107.280%	
11) 1,1-Dichloroethene-d2	4.027	65		118713	26.162	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	104.640%	
21) 2-Butanone-d5	7.075	46		155207	51.808	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	103.620%	
24) Chloroform-d	7.648	84		449782	24.392	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	97.560%	
26) 1,2-Dichloroethane-d4	8.307	65		262786m	25.202	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	100.800%	
32) Benzene-d6	8.270	84		949200	25.587	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	102.360%	
36) 1,2-Dichloropropane-d6	9.270	67		304944	25.691	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	102.760%	
41) Toluene-d8	10.325	98		843179	25.489	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	101.960%	
43) trans-1,3-Dichloroprop...	10.575	79		118496	24.629	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	98.520%	
47) 2-Hexanone-d5	10.922	63		105705	52.226	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	104.460%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		229724	25.393	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	101.560%	
66) 1,2-Dichlorobenzene-d4	13.849	152		257754	27.470	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	109.880%	
Target Compounds							
16) Methylene chloride	4.923	84		42918	3.254	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
Data File : VW025779.D
Acq On : 01 May 2023 15:41
Operator : SY/MD
Sample : VW0501SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK492

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 02 01:41:17 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
Supervised By :Mahesh Dadoda 05/02/2023

