




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025781.D
 Acq On : 01 May 2023 16:29
 Operator : SY/MD
 Sample : 02526-16
 Misc : 5.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCG0

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

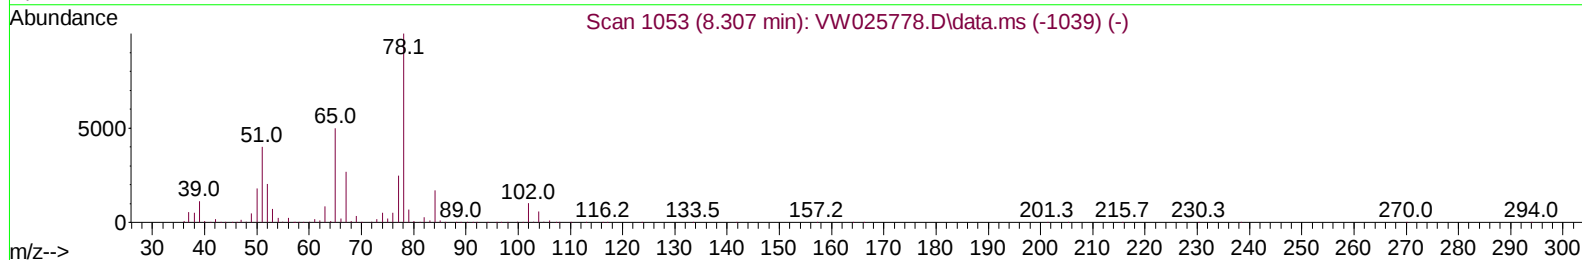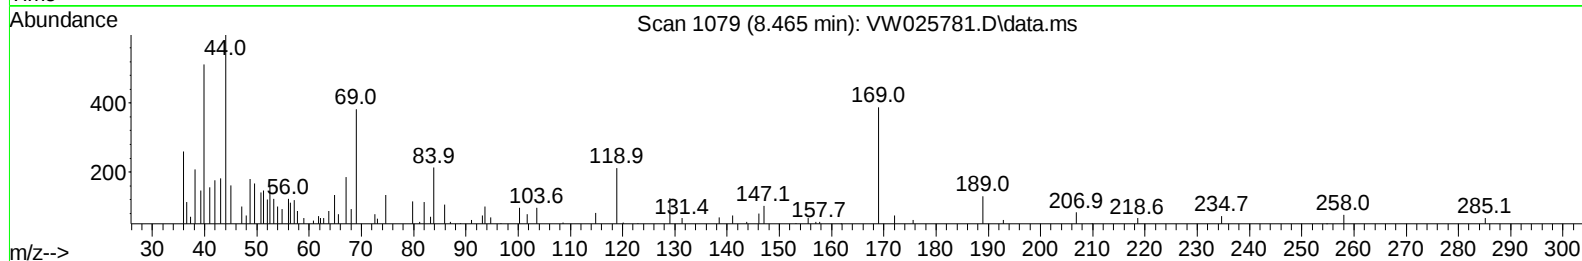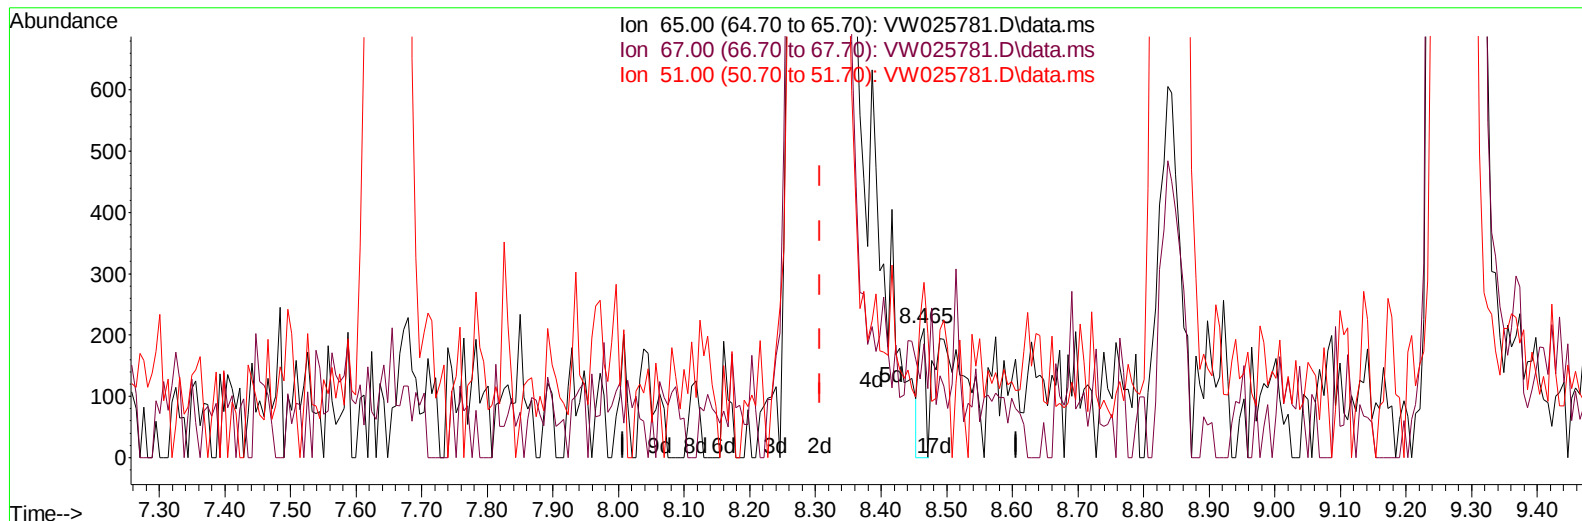

TIC: VW025781.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.465min (+ 0.159) 0.01 ug/L

response 146

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	37.67
51.00	112.30	112.33
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025781.D
 Acq On : 01 May 2023 16:29
 Operator : SY/MD
 Sample : 02526-16
 Misc : 5.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCG0

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

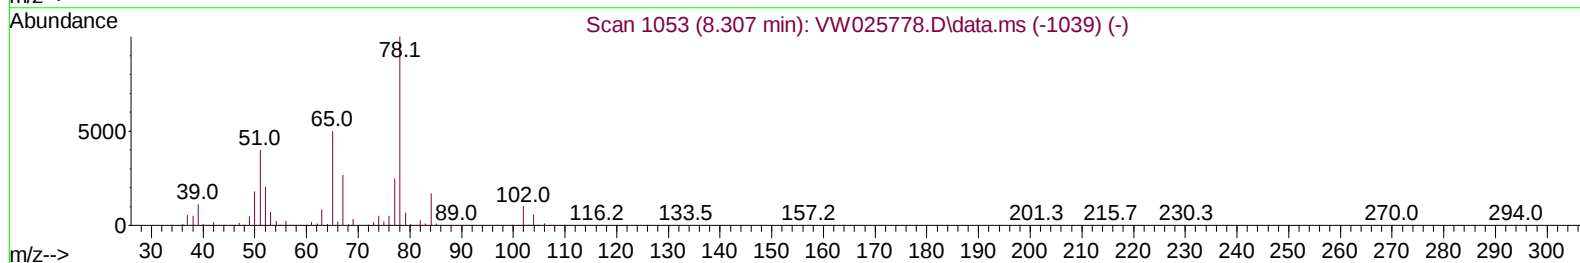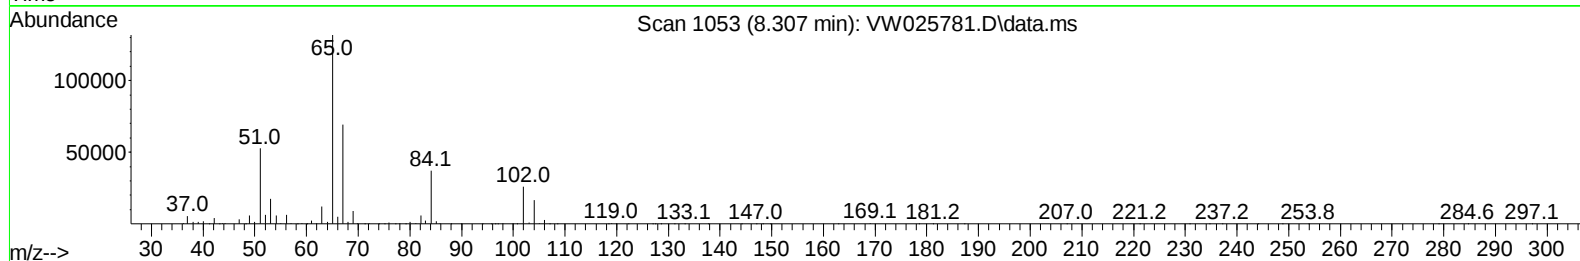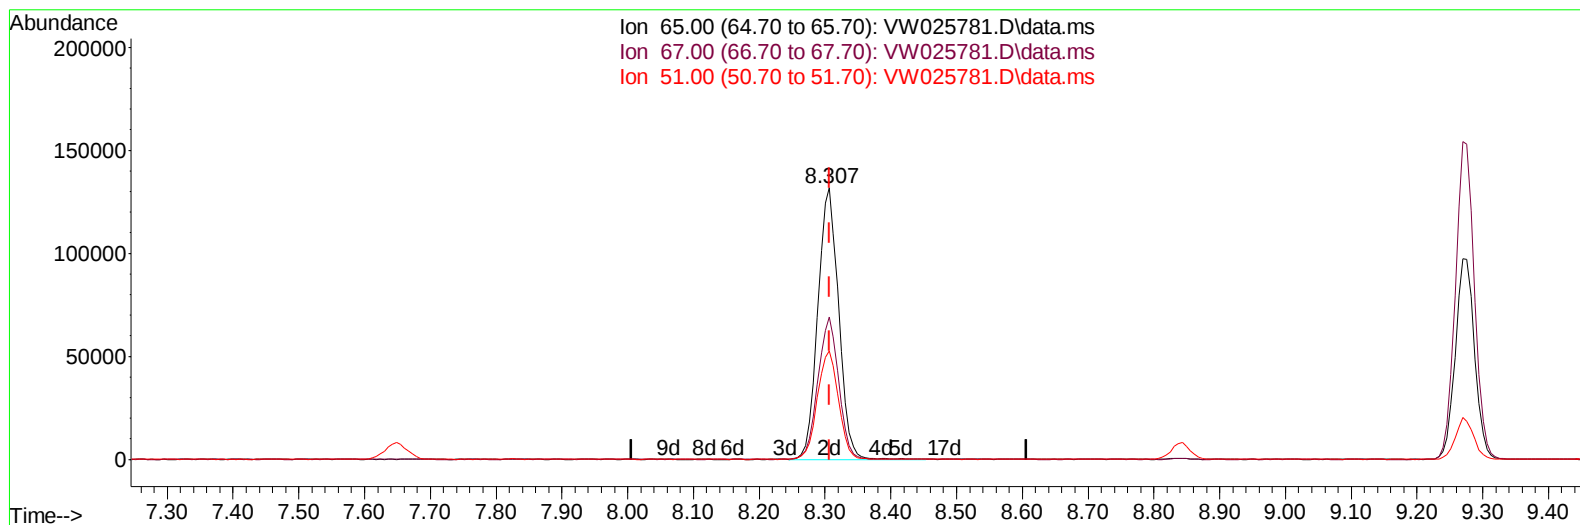

TIC: VW025781.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 25.48 ug/L m

response 290195

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.02#
51.00	112.30	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025781.D
 Acq On : 01 May 2023 16:29
 Operator : SY/MD
 Sample : 02526-16
 Misc : 5.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCG0

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		698518	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		638381	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		297368	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		245378	24.789	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	99.160%	
7) Chloroethane-d5	2.899	69		175722	23.945	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	95.800%	
11) 1,1-Dichloroethene-d2	4.027	65		112218	22.641	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	90.560%	
21) 2-Butanone-d5	7.075	46		215712	65.920	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	131.840%	
24) Chloroform-d	7.648	84		444972	22.092	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	88.360%	
26) 1,2-Dichloroethane-d4	8.307	65		290195m	25.479	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	101.920%	
32) Benzene-d6	8.270	84		946268	22.685	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	90.760%	
36) 1,2-Dichloropropane-d6	9.270	67		309342	23.178	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	92.720%	
41) Toluene-d8	10.325	98		836336	22.484	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	89.920%	
43) trans-1,3-Dichloroprop...	10.575	79		130499	24.122	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	96.480%	
47) 2-Hexanone-d5	10.922	63		152425	66.976	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	133.960%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		289164	28.426	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	113.720%	
66) 1,2-Dichlorobenzene-d4	13.848	152		264696	24.418	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	97.680%	
Target Compounds							
						Qvalue	
13) Acetone	4.118	43		361447	124.569	ug/L	100
22) 2-Butanone	7.179	43		34740	8.671	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
Data File : VW025781.D
Acq On : 01 May 2023 16:29
Operator : SY/MD
Sample : 02526-16
Misc : 5.88g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCG0

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 02 01:41:17 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
Supervised By :Mahesh Dadoda 05/02/2023

