




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025782.D
 Acq On : 01 May 2023 16:53
 Operator : SY/MD
 Sample : 02526-11
 Misc : 5.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCF5

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

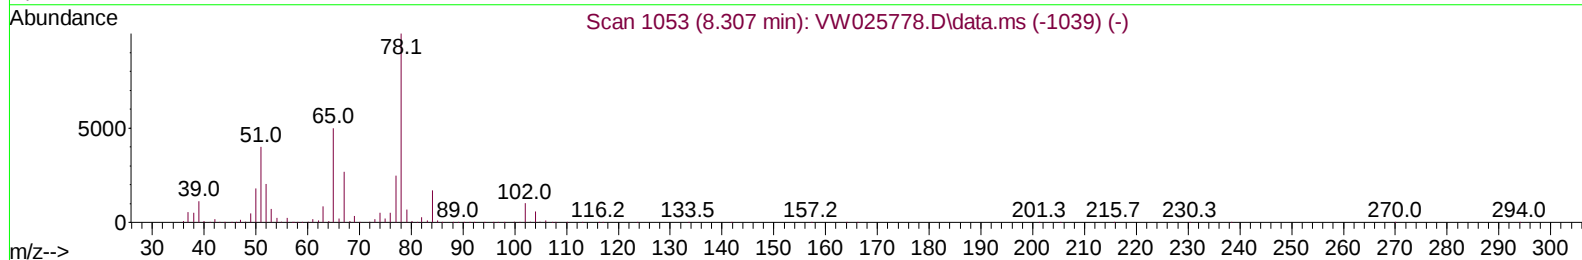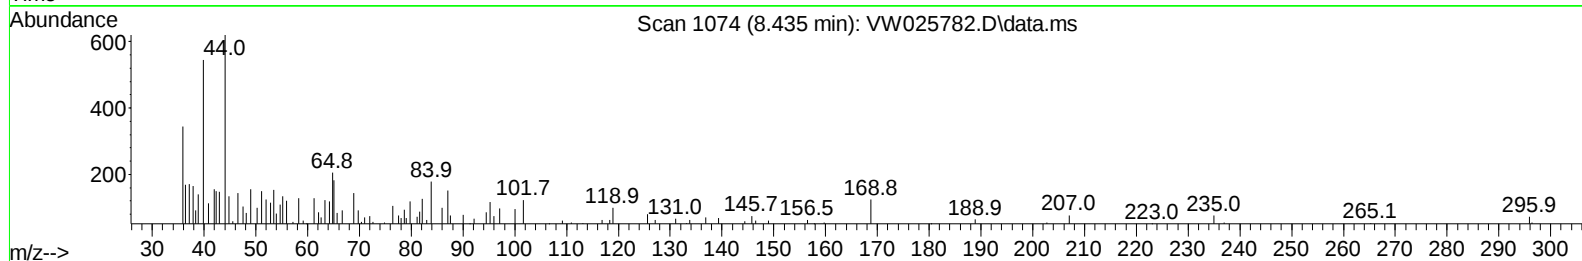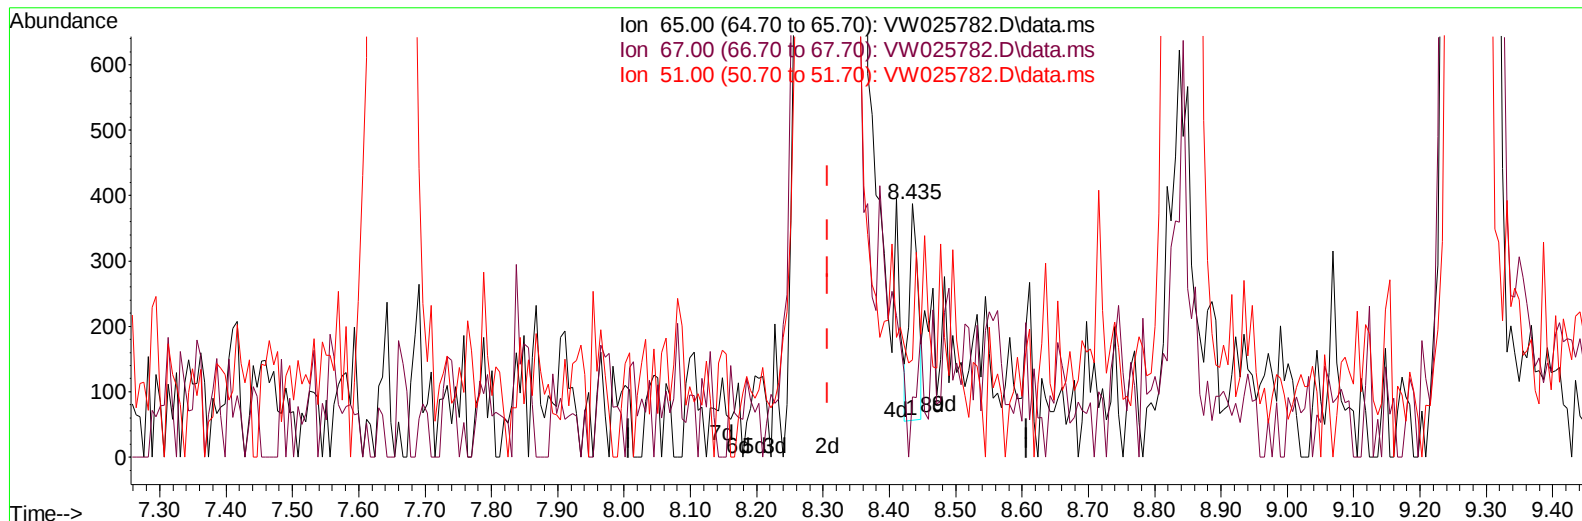

TIC: VW025782.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.435min (+ 0.128) 0.02 ug/L

response 309

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	59.22
51.00	112.30	92.88
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025782.D
 Acq On : 01 May 2023 16:53
 Operator : SY/MD
 Sample : 02526-11
 Misc : 5.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCF5

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

Quant Time: May 02 01:42:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

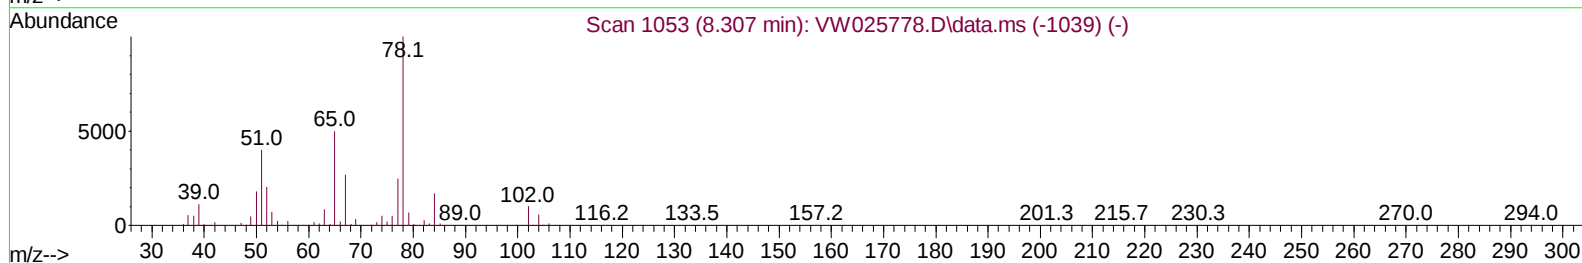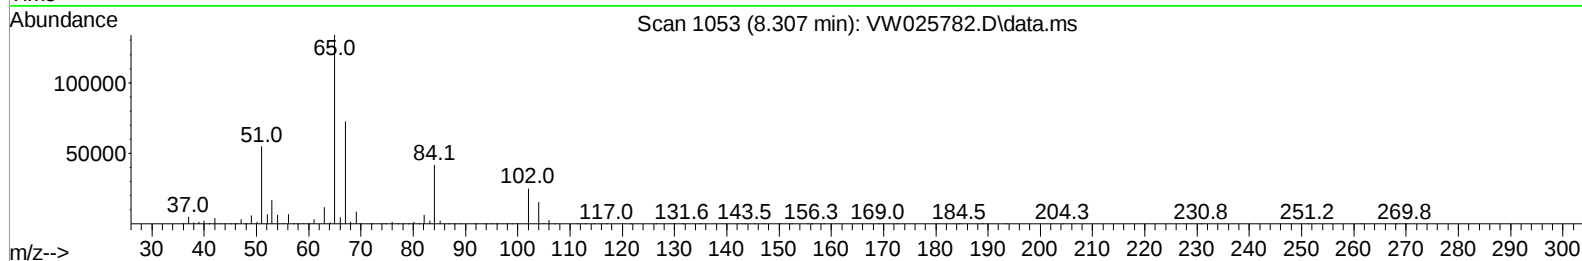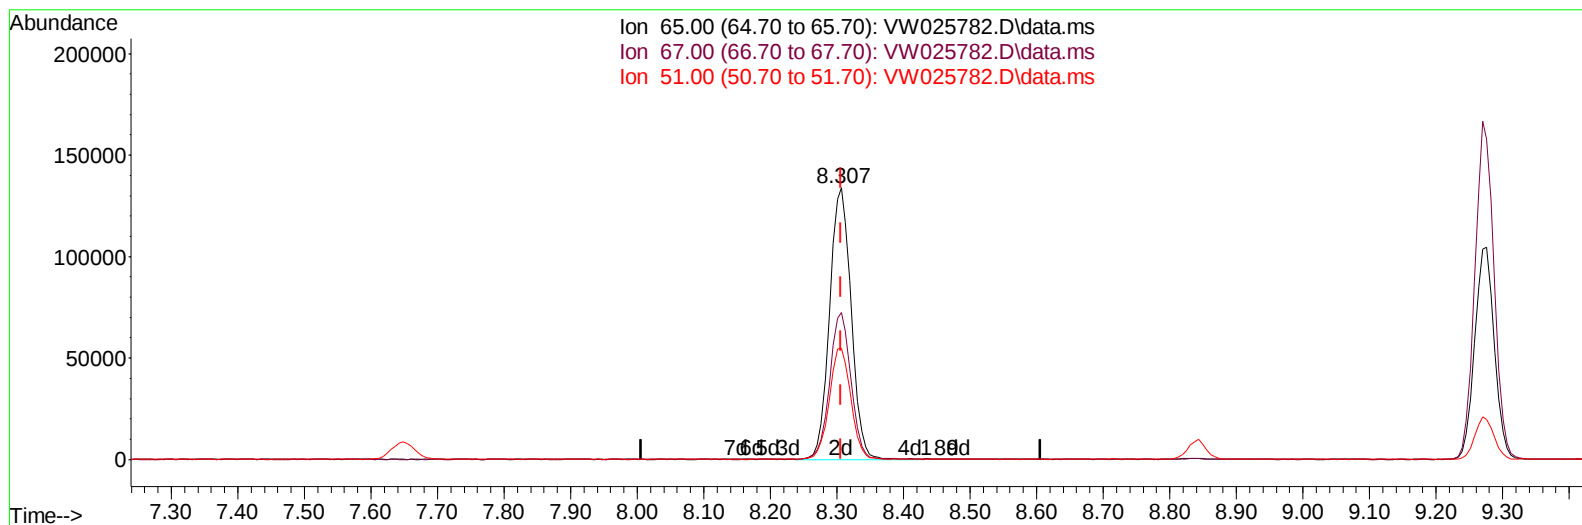

TIC: VW025782.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 23.80 ug/L m

response 300939

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.06#
51.00	112.30	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025782.D
 Acq On : 01 May 2023 16:53
 Operator : SY/MD
 Sample : 02526-11
 Misc : 5.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCF5

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		775491	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		699168	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		320373	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		259563	23.620	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	94.480%	
7) Chloroethane-d5	2.899	69		189406	23.248	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	93.000%	
11) 1,1-Dichloroethene-d2	4.027	65		121522	22.084	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	88.320%	
21) 2-Butanone-d5	7.075	46		201947	55.588	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	111.180%	
24) Chloroform-d	7.648	84		488653	21.853	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	87.400%	
26) 1,2-Dichloroethane-d4	8.307	65		300939m	23.799	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	95.200%	
32) Benzene-d6	8.276	84		1028533	22.514	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	90.040%	
36) 1,2-Dichloropropane-d6	9.270	67		331280	22.664	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	90.640%	
41) Toluene-d8	10.325	98		904974	22.214	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	88.840%	
43) trans-1,3-Dichloroprop...	10.575	79		135667	22.897	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	91.600%	
47) 2-Hexanone-d5	10.922	63		138568	55.594	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	111.180%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		281738	25.288	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	101.160%	
66) 1,2-Dichlorobenzene-d4	13.848	152		287398	24.608	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	98.440%	
Target Compounds							
						Qvalue	
13) Acetone	4.118	43		589195	182.905	ug/L	99
22) 2-Butanone	7.173	43		33963	7.636	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
Data File : VW025782.D
Acq On : 01 May 2023 16:53
Operator : SY/MD
Sample : 02526-11
Misc : 5.36g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCF5

Manual IntegrationsAPPROVED

Quant Time: May 02 01:42:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 02 01:41:17 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
Supervised By :Mahesh Dadoda 05/02/2023

