




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025783.D
 Acq On : 01 May 2023 17:17
 Operator : SY/MD
 Sample : VIBLK449
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK449

Manual IntegrationsAPPROVED

Quant Time: May 02 01:43:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

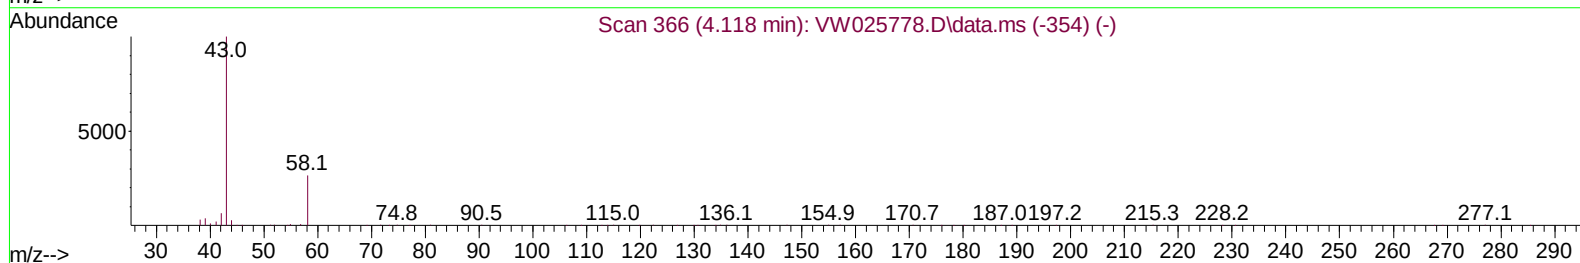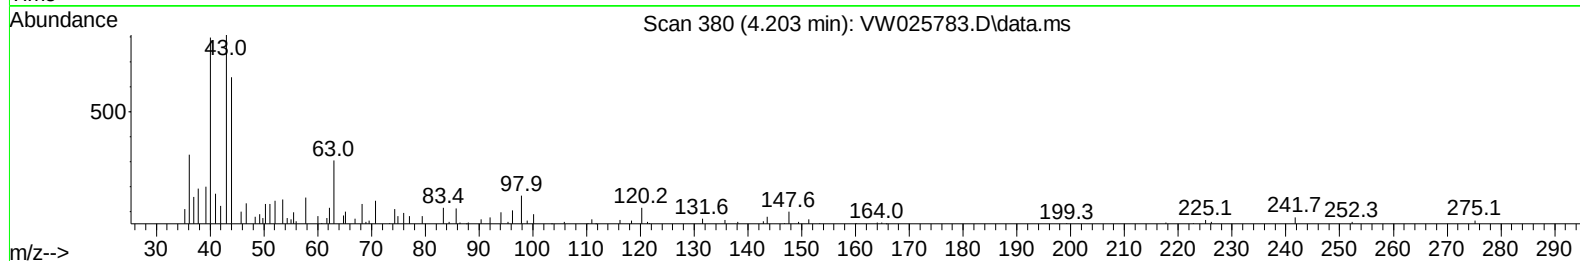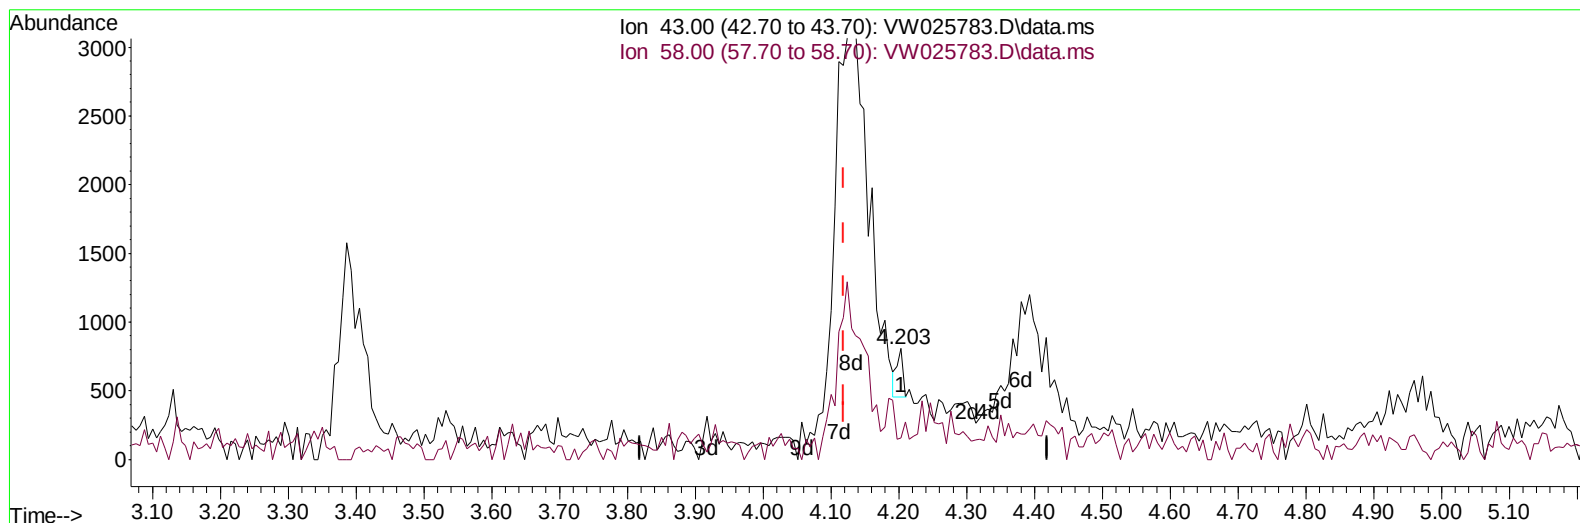

TIC: VW025783.D\data.ms

(13) Acetone (T)

4.203min (+ 0.085) 0.08 ug/L

response 209

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.10	45.45
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025783.D
 Acq On : 01 May 2023 17:17
 Operator : SY/MD
 Sample : VIBLK449
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK449

Manual IntegrationsAPPROVED

Quant Time: May 02 01:43:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

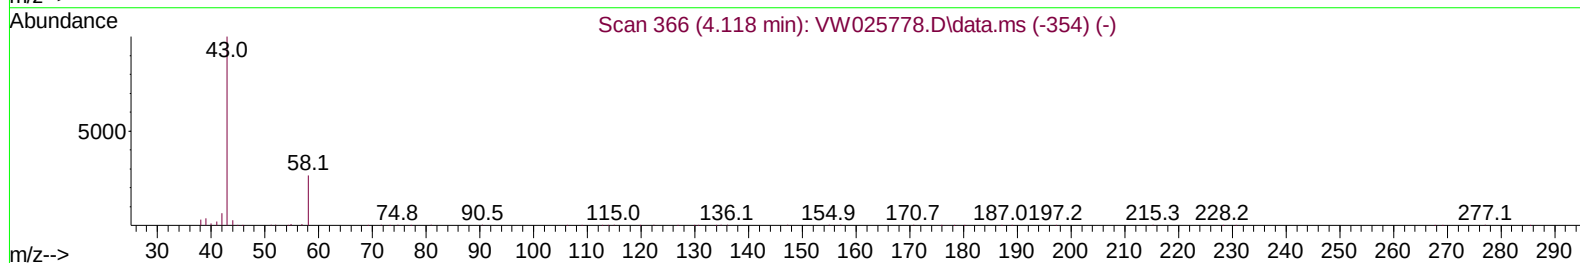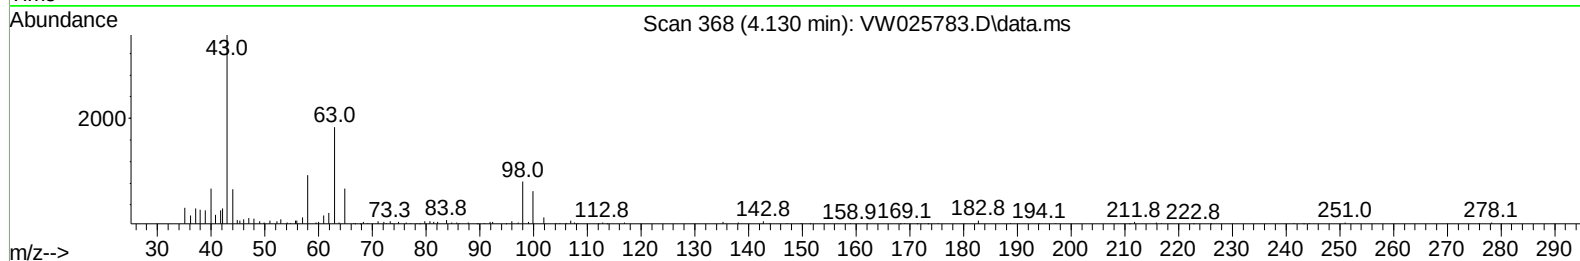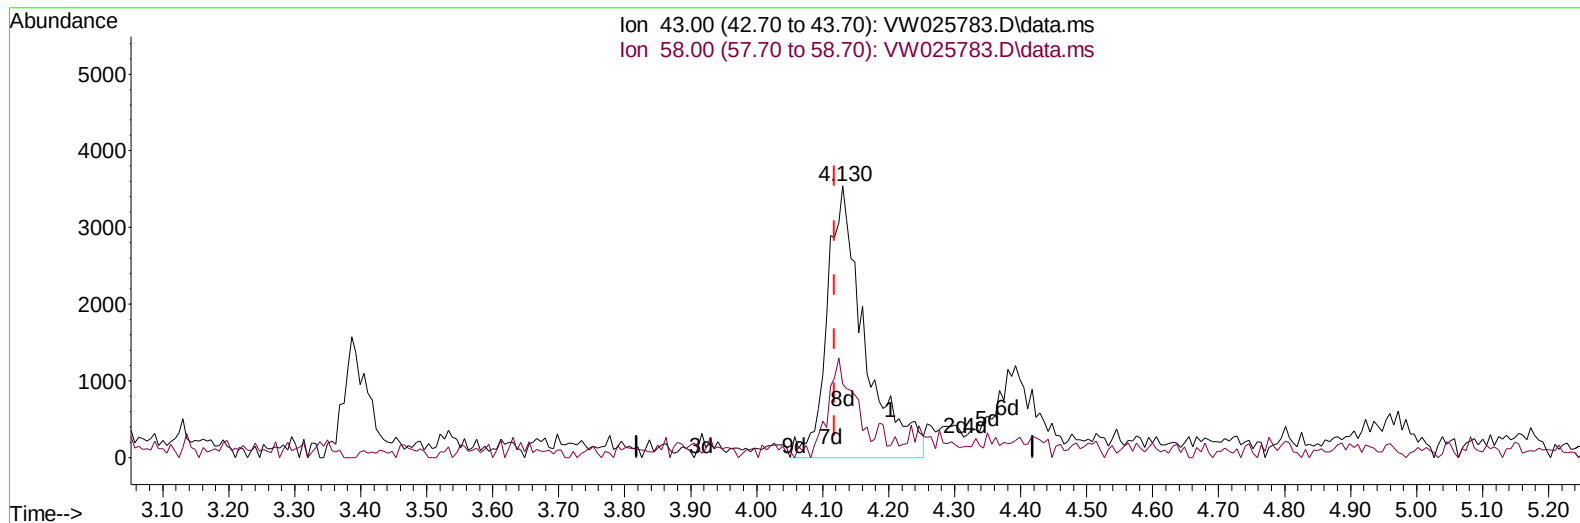

TIC: VW025783.D\data.ms

(13) Acetone (T)

4.130min (+ 0.012) 5.35 ug/L m

response 14050

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.10	0.68
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025783.D
 Acq On : 01 May 2023 17:17
 Operator : SY/MD
 Sample : VIBLK449
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK449

Manual IntegrationsAPPROVED

Quant Time: May 02 01:43:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		632559	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		570000	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152		259951	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.362	65		219729	24.513	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	98.040%	
7) Chloroethane-d5	2.899	69		156987	23.623	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	94.480%	
11) 1,1-Dichloroethene-d2	4.021	65		103934	23.156	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	92.640%	
21) 2-Butanone-d5	7.075	46		129272	43.624	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	87.240%	
24) Chloroform-d	7.648	84		408621	22.403	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	89.600%	
26) 1,2-Dichloroethane-d4	8.306	65		236236	22.904	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	91.600%	
32) Benzene-d6	8.276	84		860171	23.095	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	92.360%	
36) 1,2-Dichloropropane-d6	9.270	67		271408	22.775	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	91.120%	
41) Toluene-d8	10.324	98		760239	22.890	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	91.560%	
43) trans-1,3-Dichloroprop...	10.574	79		102848	21.292	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	85.160%	
47) 2-Hexanone-d5	10.922	63		86975	42.802	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	85.600%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		203411	22.395	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	89.600%	
66) 1,2-Dichlorobenzene-d4	13.854	152		233813	24.673	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	98.680%	
Target Compounds							
13) Acetone	4.130	43		14050m	5.347	ug/L	
16) Methylene chloride	4.923	84		36677	2.812	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
Data File : VW025783.D
Acq On : 01 May 2023 17:17
Operator : SY/MD
Sample : VIBLK449
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK449

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/02/2023
Supervised By :Mahesh Dadoda 05/02/2023

Quant Time: May 02 01:43:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 02 01:41:17 2023
Response via : Initial Calibration

