




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025785.D
 Acq On : 01 May 2023 18:05
 Operator : SY/MD
 Sample : 02526-07
 Misc : 4.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

Quant Time: May 02 01:43:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

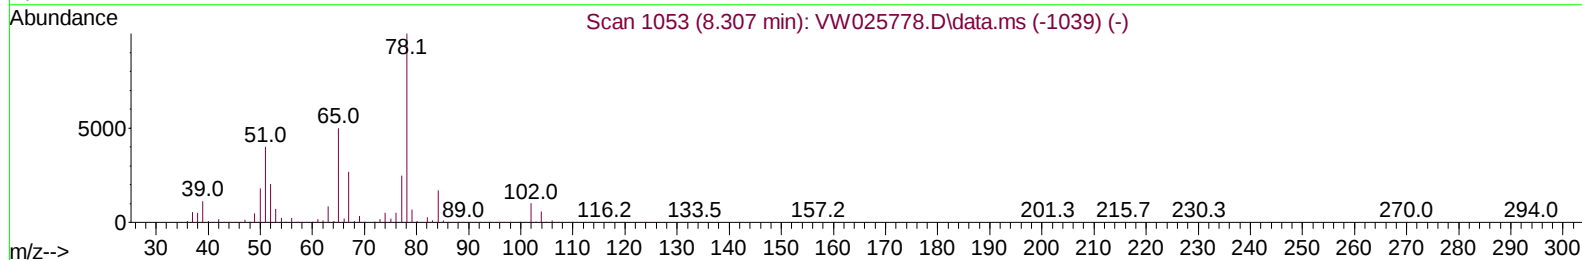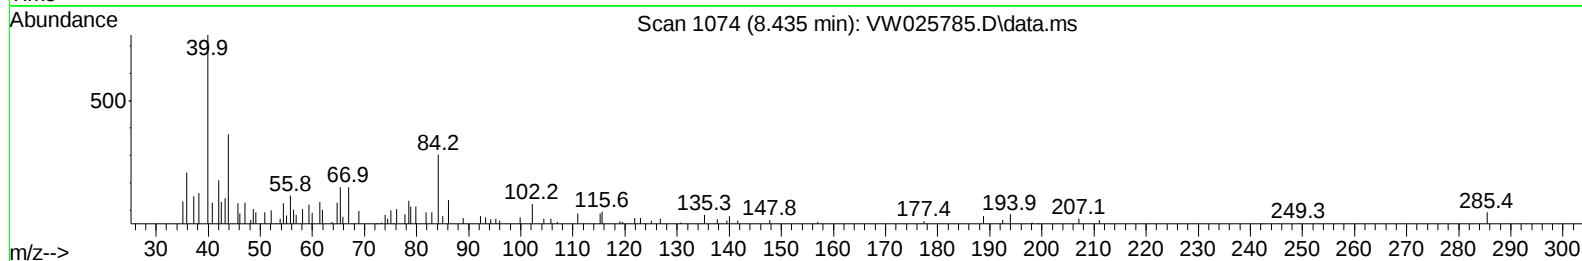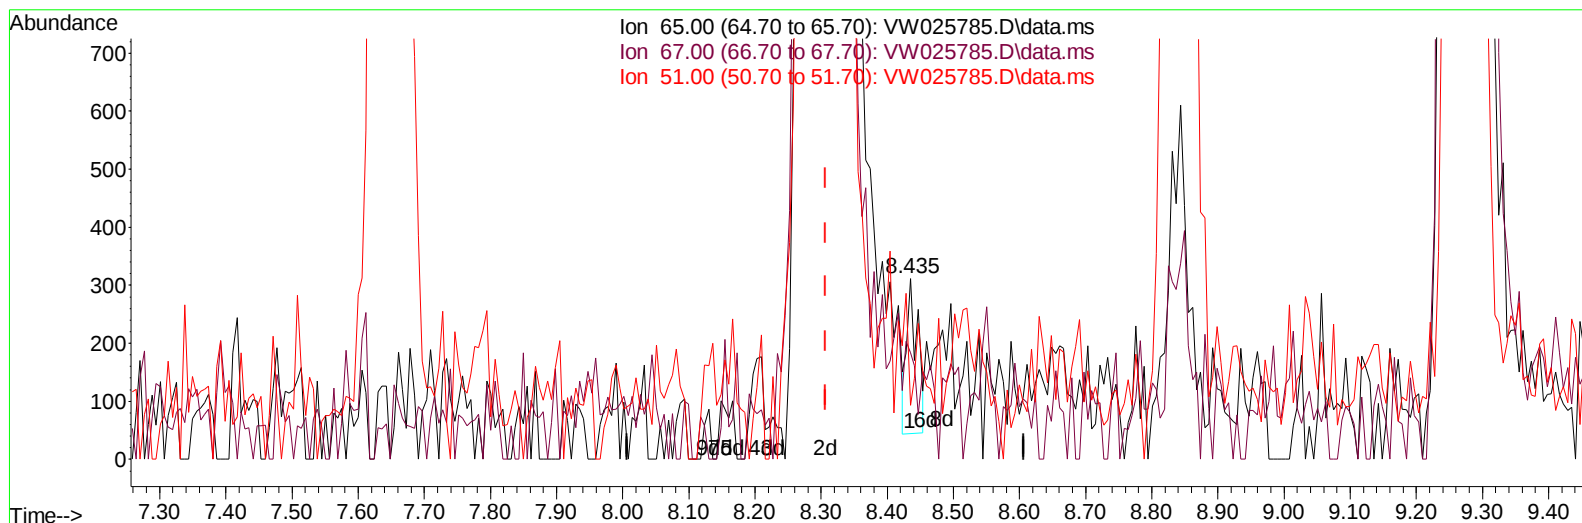

TIC: VW025785.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.435min (+ 0.128) 0.03 ug/L

response 299

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	39.13
51.00	112.30	91.30
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025785.D
 Acq On : 01 May 2023 18:05
 Operator : SY/MD
 Sample : 02526-07
 Misc : 4.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 02 01:43:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

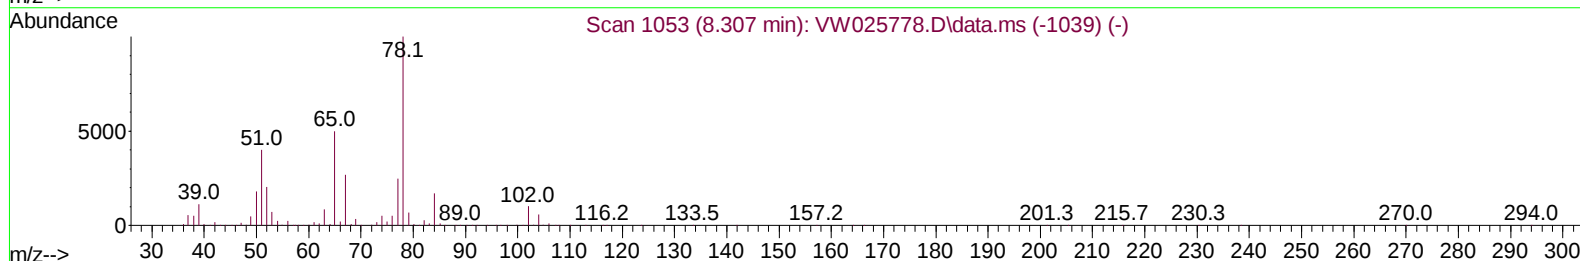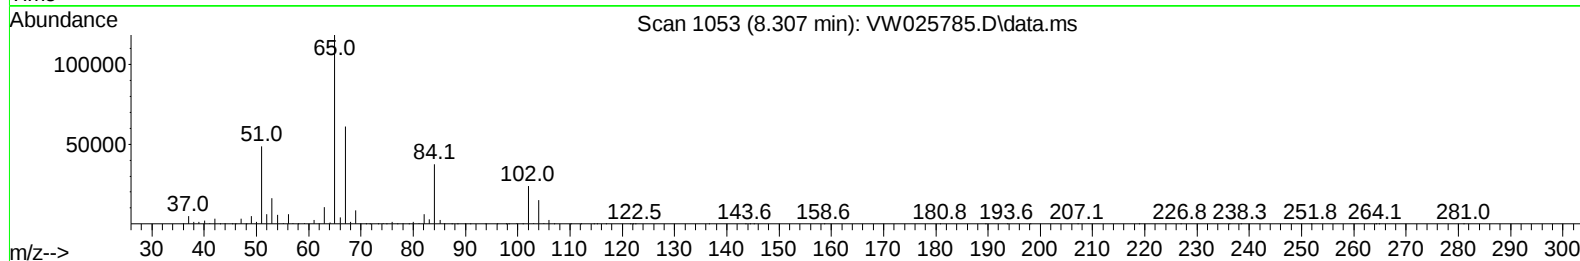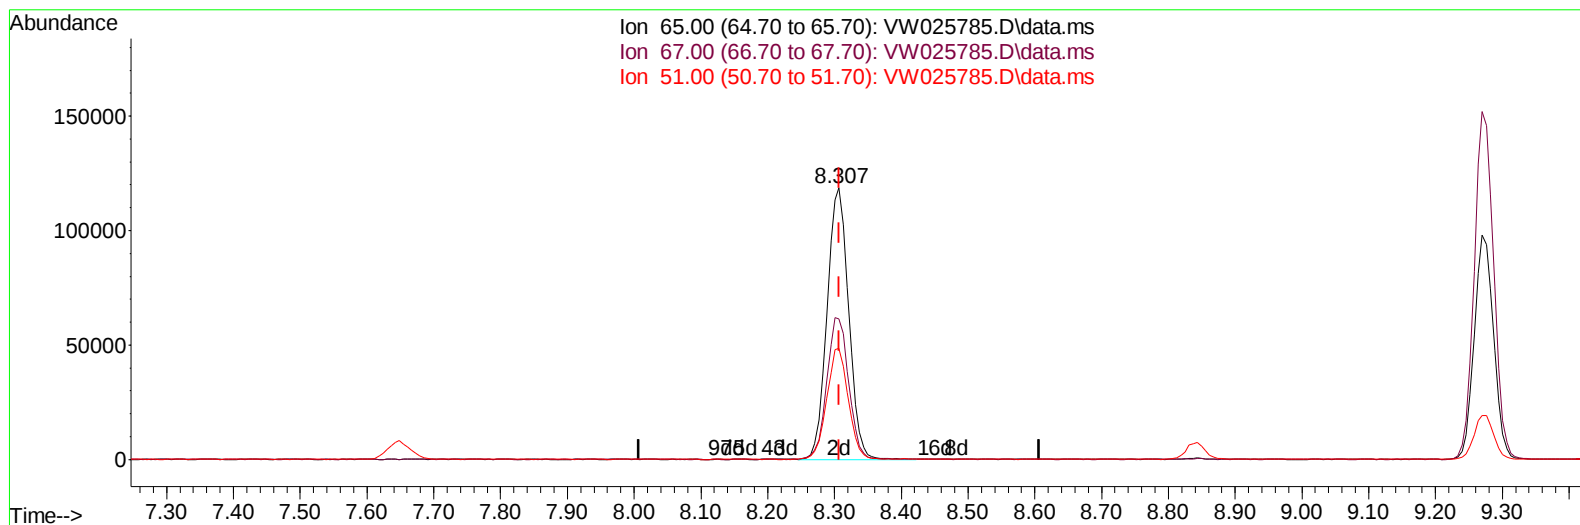

TIC: VW025785.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 25.49 ug/L m

response 266008

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.04#
51.00	112.30	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
 Data File : VW025785.D
 Acq On : 01 May 2023 18:05
 Operator : SY/MD
 Sample : 02526-07
 Misc : 4.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 02 01:43:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 01:41:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	640113	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	578269	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	264786	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	240231	26.484	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	105.920%	
7) Chloroethane-d5	2.899	69	176142	26.193	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	104.760%	
11) 1,1-Dichloroethene-d2	4.027	65	114339	25.173	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	100.680%	
21) 2-Butanone-d5	7.075	46	143651	47.904	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	95.800%	
24) Chloroform-d	7.648	84	457192	24.770	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	99.080%	
26) 1,2-Dichloroethane-d4	8.307	65	266008m	25.486	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	101.960%	
32) Benzene-d6	8.276	84	957900	25.351	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	101.400%	
36) 1,2-Dichloropropane-d6	9.270	67	306774	25.375	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	101.520%	
41) Toluene-d8	10.325	98	856151	25.410	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	101.640%	
43) trans-1,3-Dichloroprop...	10.575	79	116424	23.757	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	95.040%	
47) 2-Hexanone-d5	10.922	63	97469	47.280	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	94.560%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	226951	24.630	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	98.520%	
66) 1,2-Dichlorobenzene-d4	13.849	152	262459	27.191	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	108.760%	
Target Compounds						
16) Methylene chloride	4.917	84	50205	3.803	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050123\
Data File : VW025785.D
Acq On : 01 May 2023 18:05
Operator : SY/MD
Sample : 02526-07
Misc : 4.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/02/2023
Supervised By :Mahesh Dadoda 05/02/2023

Quant Time: May 02 01:43:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 02 01:41:17 2023
Response via : Initial Calibration

