

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050124\
 Data File : VW028558.D
 Acq On : 01 May 2024 12:04
 Operator : SY/MD
 Sample : P2321-08
 Misc : 5.07g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 02 02:21:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 02 02:18:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	234881	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	216580	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	103599	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	44204	11.739	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	46.960%
7) Chloroethane-d5	2.899	69	47330	16.584	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.320%
11) 1,1-Dichloroethene-d2	4.021	65	25743	16.144	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.560%
21) 2-Butanone-d5	7.081	46	46177	65.534	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	131.060%
24) Chloroform-d	7.648	84	118707	19.368	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.480%
26) 1,2-Dichloroethane-d4	8.215	65	45	0.014	ug/L	-0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.276	84	219890	18.585	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.320%
36) 1,2-Dichloropropane-d6	9.270	67	70490	20.043	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	80.160%
41) Toluene-d8	10.319	98	188776	17.546	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.200%
43) trans-1,3-Dichloroprop...	10.575	79	28280	20.223	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.880%
47) 2-Hexanone-d5	10.922	63	29765	61.100	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	69198	27.888	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.560%
66) 1,2-Dichlorobenzene-d4	13.848	152	66060	20.163	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.640%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	2344	0.453	ug/L #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050124\
Data File : VW028558.D
Acq On : 01 May 2024 12:04
Operator : SY/MD
Sample : P2321-08
Misc : 5.07g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 02 02:21:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 02 02:18:04 2024
Response via : Initial Calibration

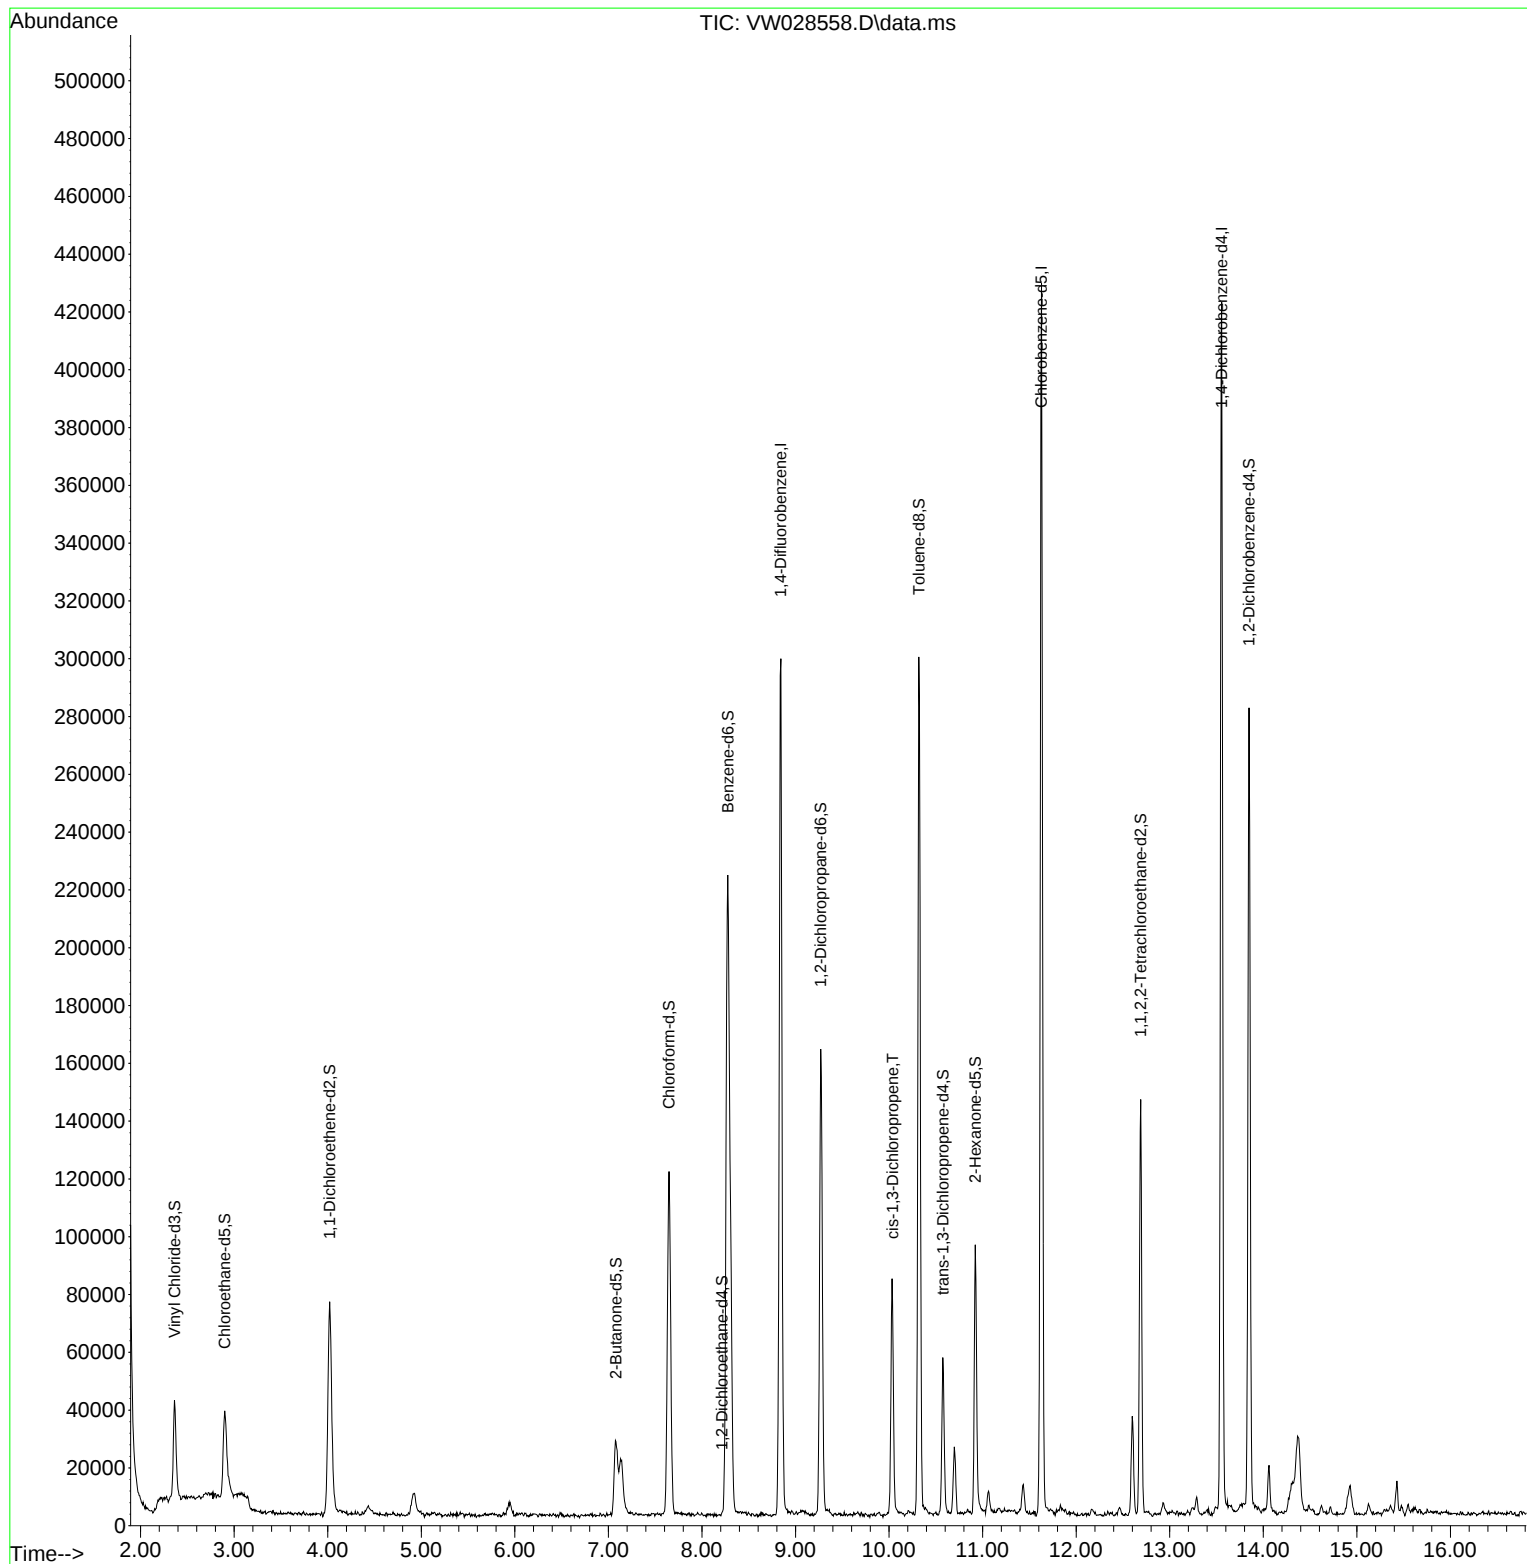

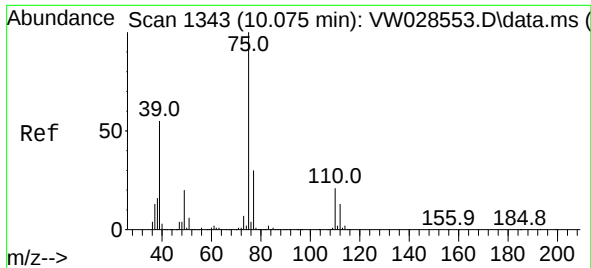

#39
 cis-1,3-Dichloropropene
 Concen: 0.453 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW028558.D
 Acq: 01 May 2024 12:04

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 2344
 Ion Ratio Lower Upper
 75 100
 77 46.9 21.3 39.5#

