

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022743.D
 Acq On : 02 May 2022 16:40
 Operator : SY/VA
 Sample : N2639-01
 Misc : 4.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 03 01:44:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	351728	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	320845	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	127499	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	152540	21.138	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.560%
7) Chloroethane-d5	2.891	69	106177	22.616	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.480%
11) 1,1-Dichloroethene-d2	4.019	63	149240	16.006	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.040%
21) 2-Butanone-d5	7.080	46	47338	34.502	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.000%
24) Chloroform-d	7.647	84	216756	21.034	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.120%
26) 1,2-Dichloroethane-d4	8.415	65	224	0.040	ug/L	0.11
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.160%#
32) Benzene-d6	8.275	84	428923	23.193	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.760%
36) 1,2-Dichloropropane-d6	9.274	67	124155	23.900	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.600%
41) Toluene-d8	10.323	98	398806	22.324	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.280%
43) trans-1,3-Dichloroprop...	10.579	79	45391	18.977	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.920%
47) 2-Hexanone-d5	10.921	63	35245	35.541	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.080%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	102117	21.090	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	100053	22.449	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.800%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4218	0.595	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022743.D
Acq On : 02 May 2022 16:40
Operator : SY/VA
Sample : N2639-01
Misc : 4.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 03 01:44:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

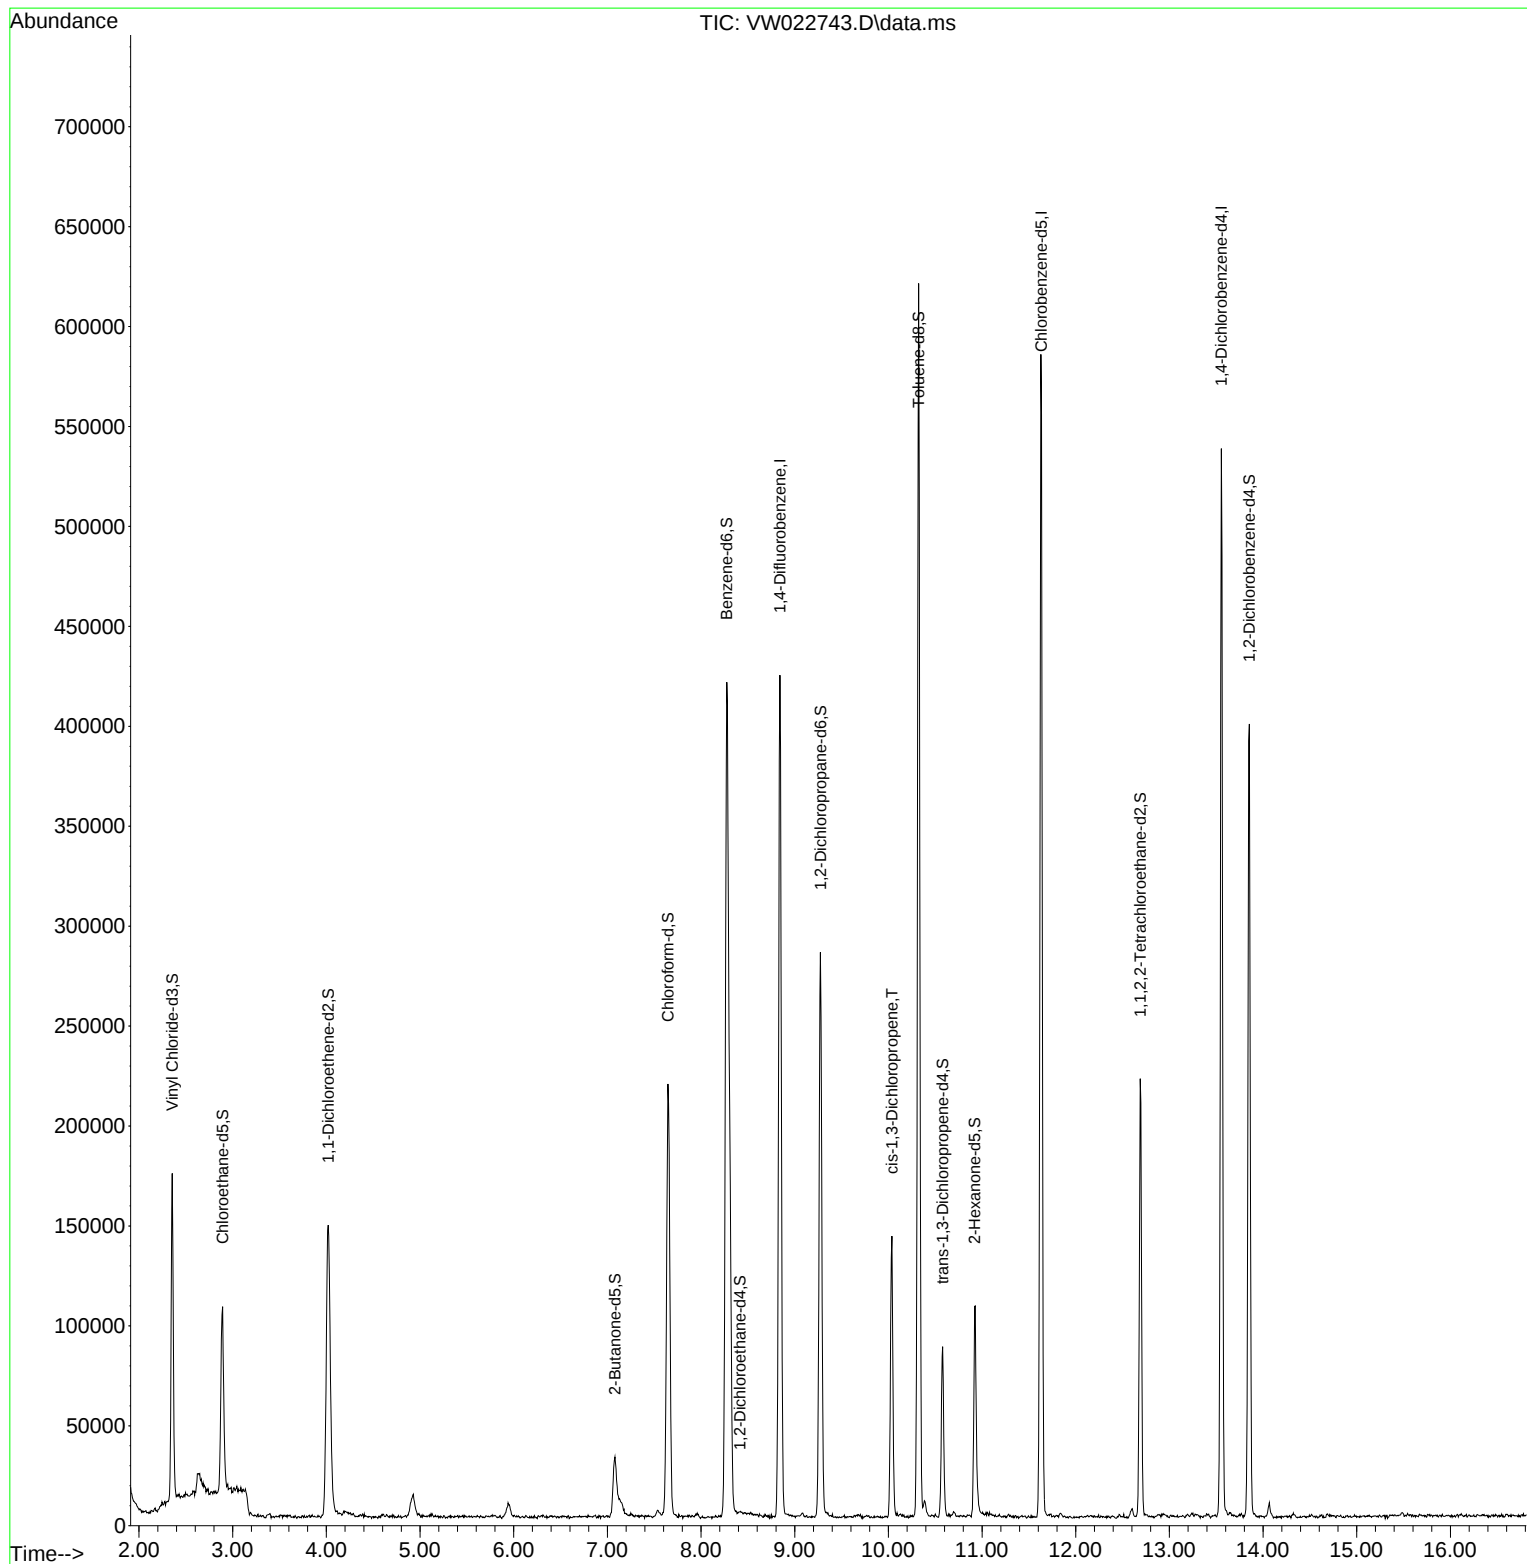

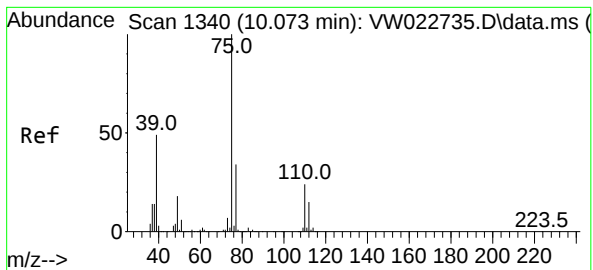

#39
 cis-1,3-Dichloropropene
 Concen: 0.595 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022743.D
 Acq: 02 May 2022 16:40

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4218
 Ion Ratio Lower Upper
 75 100
 77 39.0 22.1 41.1

