

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022746.D
 Acq On : 02 May 2022 17:52
 Operator : SY/VA
 Sample : N2639-04
 Misc : 5.16g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 03 01:44:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	343932	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	337137	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	163605	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	163775	23.210	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.840%
7) Chloroethane-d5	2.886	69	107668	23.454	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.800%
11) 1,1-Dichloroethene-d2	4.019	63	156571	17.173	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.680%
21) 2-Butanone-d5	7.080	46	62494	46.581	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.160%
24) Chloroform-d	7.647	84	236330	23.454	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.800%
26) 1,2-Dichloroethane-d4	8.305	65	138529	25.066	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.280%
32) Benzene-d6	8.275	84	470031	24.188	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.760%
36) 1,2-Dichloropropane-d6	9.275	67	136553	25.016	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.080%
41) Toluene-d8	10.323	98	449568	23.949	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.800%
43) trans-1,3-Dichloroprop...	10.579	79	57512	22.883	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.520%
47) 2-Hexanone-d5	10.921	63	49397	47.404	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.800%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	119002	23.390	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.560%
66) 1,2-Dichlorobenzene-d4	13.847	152	140410	24.551	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.200%
Target Compounds						
46) Tetrachloroethene	10.860	164	9994	2.435	ug/L	Qvalue 92
49) Dibromochloromethane	10.866	129	9816	2.030	ug/L	# 11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022746.D
Acq On : 02 May 2022 17:52
Operator : SY/VA
Sample : N2639-04
Misc : 5.16g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 03 01:44:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

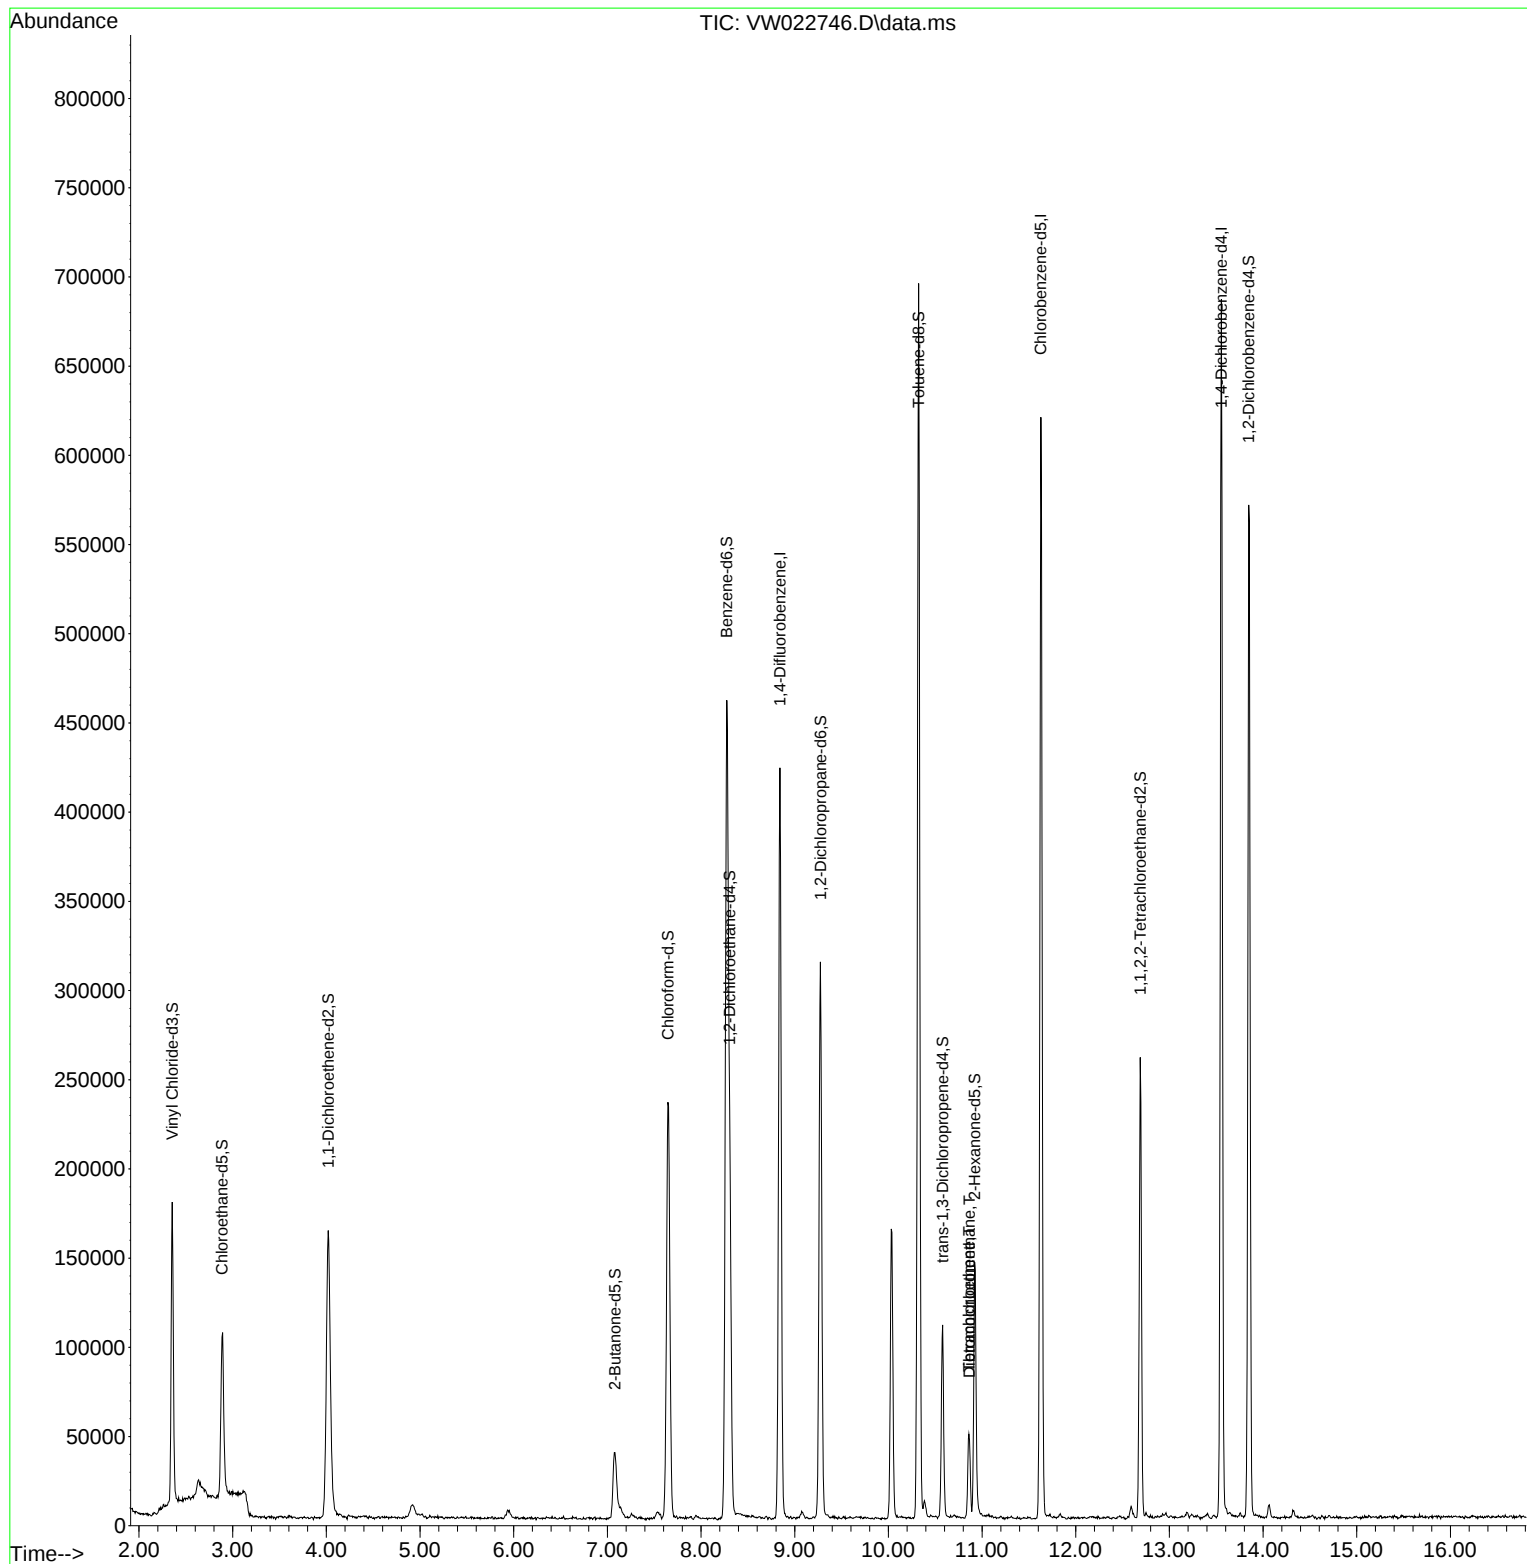



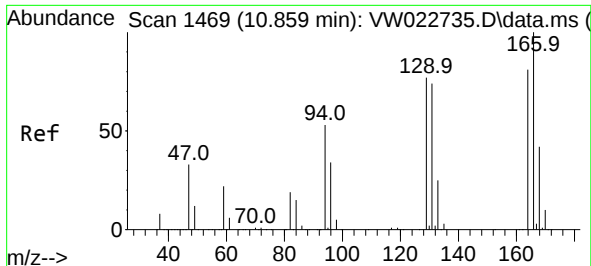


#46
Tetrachloroethene
Concen: 2.435 ug/L
RT: 10.860 min Scan# 1469
Delta R.T. 0.000 min
Lab File: VW022746.D
Acq: 02 May 2022 17:52


Instrument :
MSVOA_W
ClientSampleId :

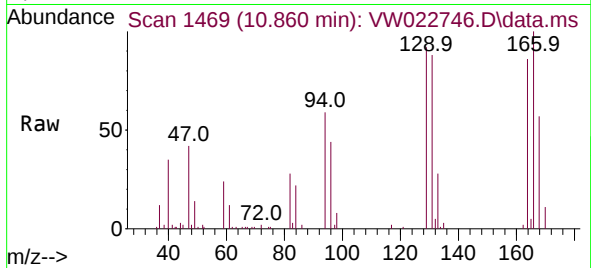

Tgt Ion:	164	Resp:	9994
Ion	Ratio	Lower	Upper
164	100		
129	107.8	76.9	142.7
131	103.2	75.1	139.5
166	116.8	96.0	178.2

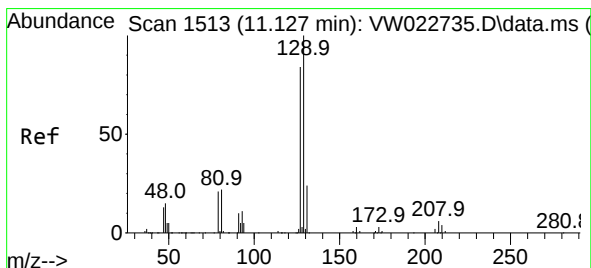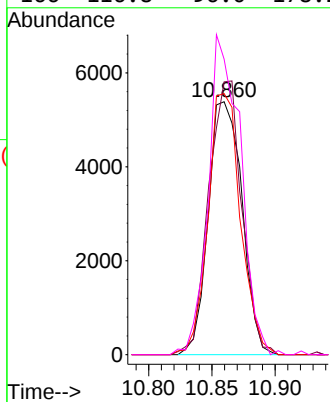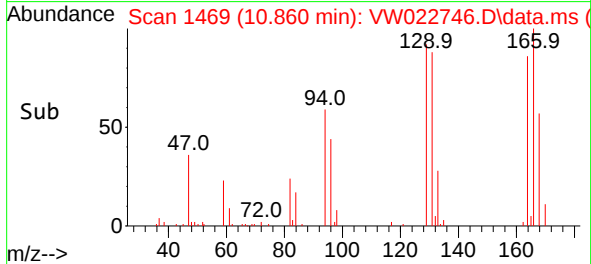

#49
Dibromochloromethane
Concen: 2.030 ug/L
RT: 10.866 min Scan# 1470
Delta R.T. -0.262 min
Lab File: VW022746.D
Acq: 02 May 2022 17:52

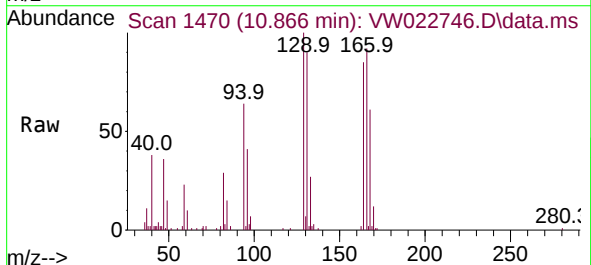

Tgt Ion:	129	Resp:	9816
Ion	Ratio	Lower	Upper
129	100		
127	0.0	53.8	100.0#

