

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022747.D
 Acq On : 02 May 2022 18:16
 Operator : SY/VA
 Sample : N2639-06
 Misc : 5.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 03 01:44:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	350143	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	336170	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	159887	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	160814	22.386	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.560%
7) Chloroethane-d5	2.885	69	102445	21.920	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.680%
11) 1,1-Dichloroethene-d2	4.019	63	153538	16.541	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.160%
21) 2-Butanone-d5	7.080	46	65259	47.779	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.560%
24) Chloroform-d	7.647	84	233559	22.768	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.080%
26) 1,2-Dichloroethane-d4	8.396	65	273	0.049	ug/L	0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.200%#
32) Benzene-d6	8.275	84	467871	24.146	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.600%
36) 1,2-Dichloropropane-d6	9.274	67	132070	24.264	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.040%
41) Toluene-d8	10.323	98	437190	23.357	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.440%
43) trans-1,3-Dichloroprop...	10.579	79	55987	22.340	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.360%
47) 2-Hexanone-d5	10.920	63	53108	51.112	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.220%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	122100	24.068	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.280%
66) 1,2-Dichlorobenzene-d4	13.853	152	135454	24.235	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.960%
Target Compounds						
39) cis-1,3-Dichloropropene	10.030	75	4882	0.657	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022747.D
Acq On : 02 May 2022 18:16
Operator : SY/VA
Sample : N2639-06
Misc : 5.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 03 01:44:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

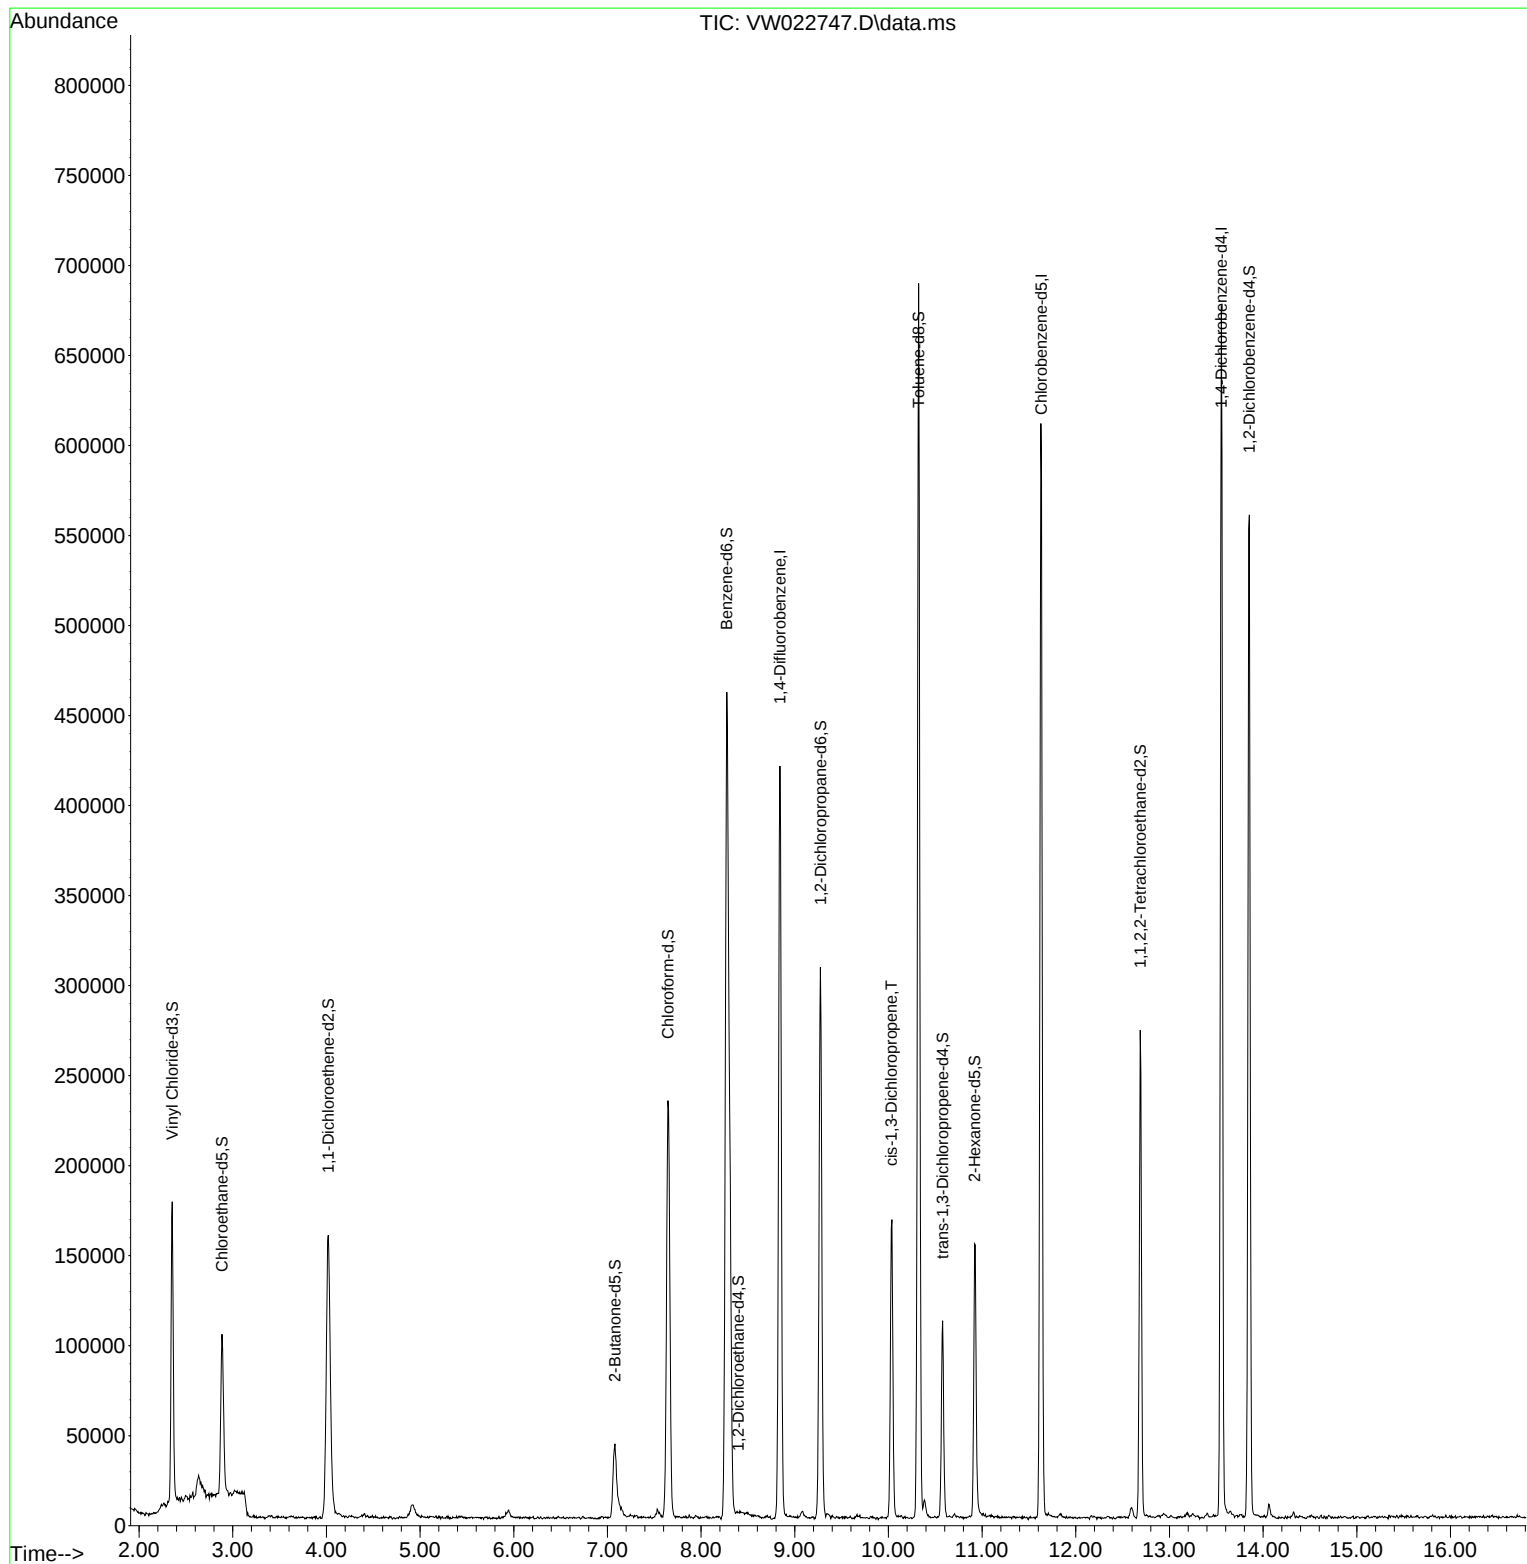

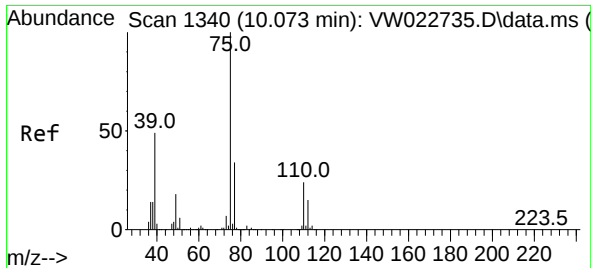

#39
 cis-1,3-Dichloropropene
 Concen: 0.657 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VW022747.D
 Acq: 02 May 2022 18:16

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4882
 Ion Ratio Lower Upper
 75 100
 77 41.1 22.1 41.1

