

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022750.D
 Acq On : 02 May 2022 19:28
 Operator : SY/VA
 Sample : N2639-16
 Misc : 5.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 03 01:45:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	329566	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	326726	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	156237	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	170707	25.247	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.000%
7) Chloroethane-d5	2.885	69	113063	25.702	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.800%
11) 1,1-Dichloroethene-d2	4.019	63	159317	18.235	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.960%
21) 2-Butanone-d5	7.080	46	64540	50.203	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.400%
24) Chloroform-d	7.647	84	247950	25.680	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.720%
26) 1,2-Dichloroethane-d4	8.421	65	209	0.039	ug/L	0.12
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.160%#
32) Benzene-d6	8.275	84	498450	26.468	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.880%
36) 1,2-Dichloropropane-d6	9.268	67	144789	27.370	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.480%
41) Toluene-d8	10.323	98	469163	25.789	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.160%
43) trans-1,3-Dichloroprop...	10.579	79	59357	24.369	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.480%
47) 2-Hexanone-d5	10.920	63	51110	50.611	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.220%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	122720	24.889	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.560%
66) 1,2-Dichlorobenzene-d4	13.847	152	147525	27.012	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.040%
Target Compounds						Qvalue
46) Tetrachloroethene	10.859	164	3395	0.853	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022750.D
Acq On : 02 May 2022 19:28
Operator : SY/VA
Sample : N2639-16
Misc : 5.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 03 01:45:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

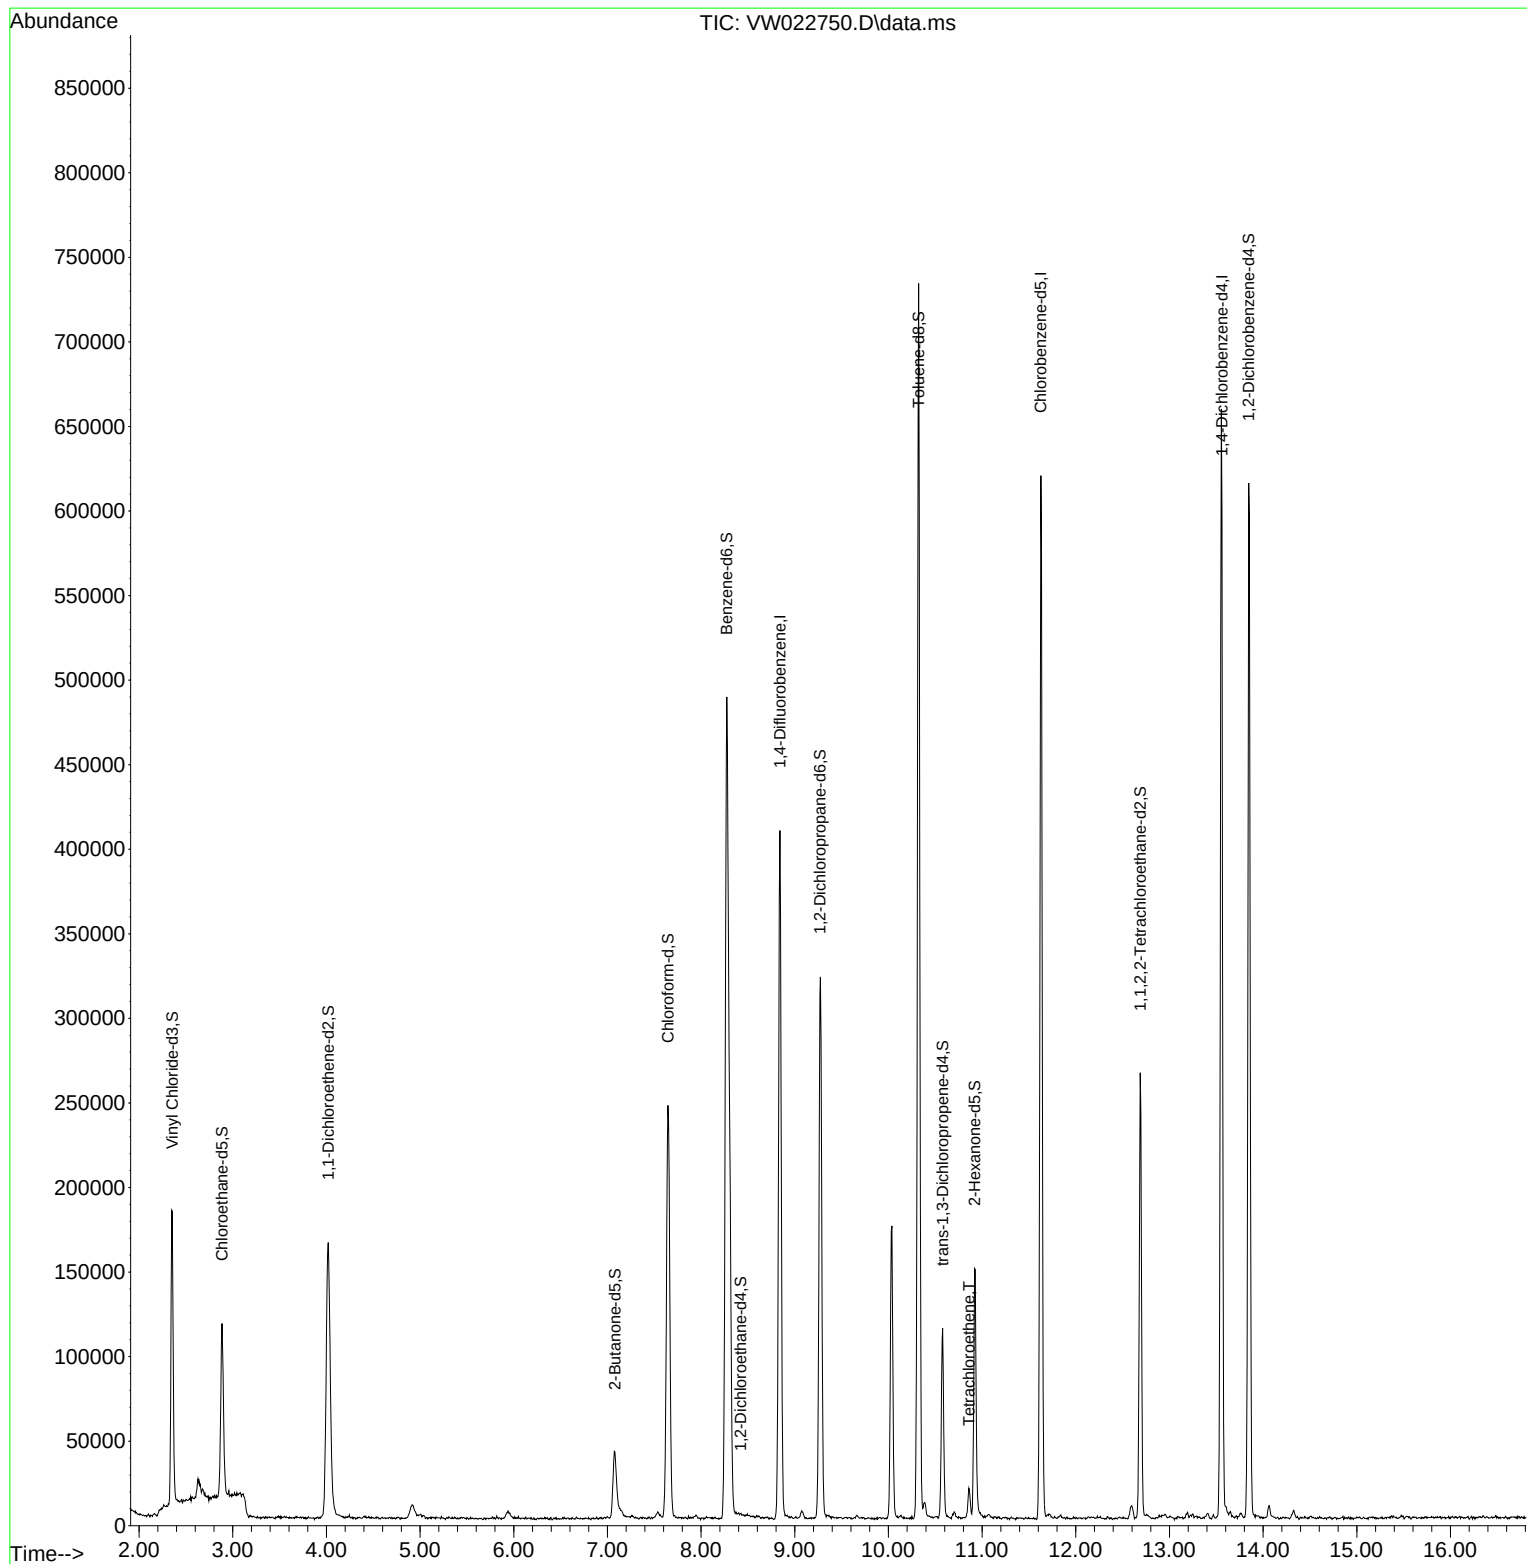

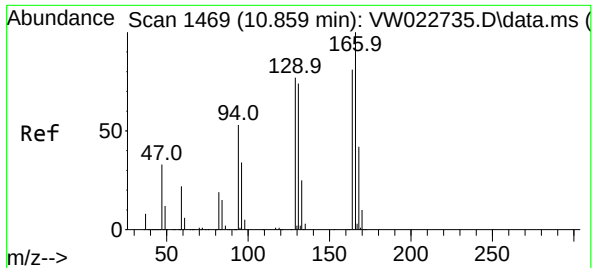

#46
 Tetrachloroethene
 Concen: 0.853 ug/L
 RT: 10.859 min Scan# 1469
 Delta R.T. 0.000 min
 Lab File: VW022750.D
 Acq: 02 May 2022 19:28

Instrument :
 MSVOA_W
 ClientSampleId :

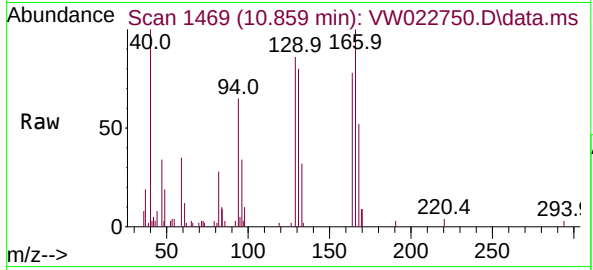

Tgt Ion:	164	Resp:	3395
Ion	Ratio	Lower	Upper
164	100		
129	109.9	76.9	142.7
131	103.0	75.1	139.5
166	127.4	96.0	178.2

