

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022755.D
 Acq On : 02 May 2022 21:29
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 03 01:46:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	289834	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	292710	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	147258	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	143157	24.075	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.280%
7) Chloroethane-d5	2.885	69	96418	24.923	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.680%
11) 1,1-Dichloroethene-d2	4.019	63	131368	17.098	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.400%
21) 2-Butanone-d5	7.080	46	58236	51.509	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.020%
24) Chloroform-d	7.647	84	203971	24.021	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.080%
26) 1,2-Dichloroethane-d4	8.305	65	123281	26.471	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.880%
32) Benzene-d6	8.275	84	409520	24.273	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.080%
36) 1,2-Dichloropropane-d6	9.274	67	117511	24.795	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.200%
41) Toluene-d8	10.323	98	388177	23.817	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.280%
43) trans-1,3-Dichloroprop...	10.579	79	49173	22.534	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.120%
47) 2-Hexanone-d5	10.927	63	45060	49.805	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.620%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	109387	24.763	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	127476	24.764	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.040%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4188	0.647	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022755.D
Acq On : 02 May 2022 21:29
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 03 01:46:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

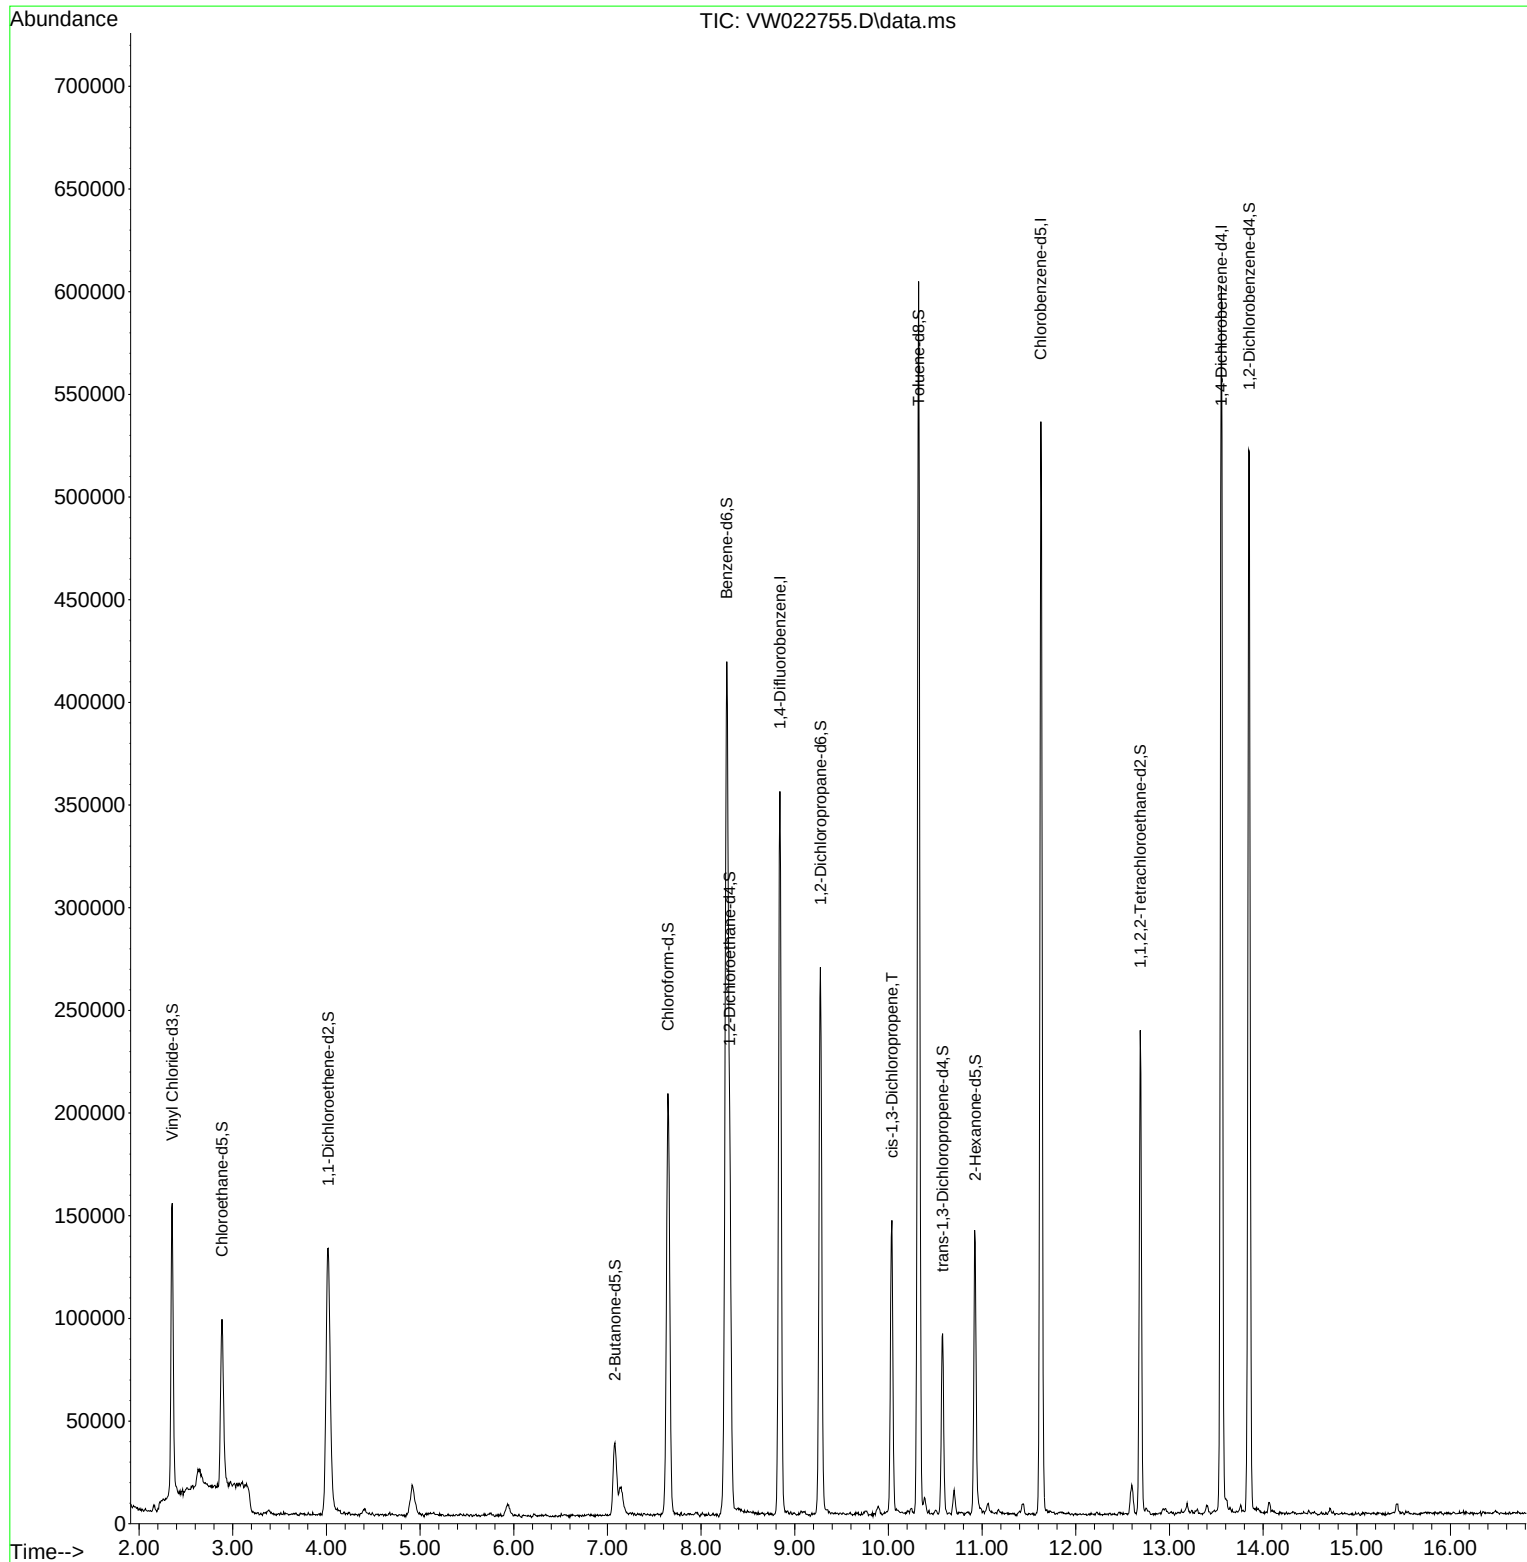

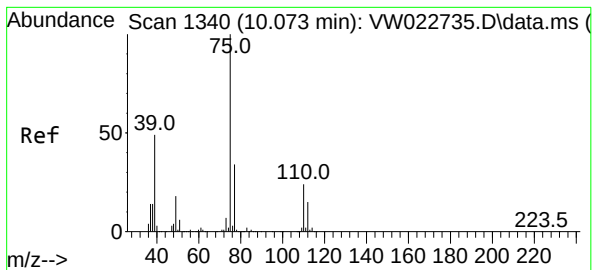

#39
 cis-1,3-Dichloropropene
 Concen: 0.647 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022755.D
 Acq: 02 May 2022 21:29

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4188
 Ion Ratio Lower Upper
 75 100
 77 40.5 22.1 41.1

