




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

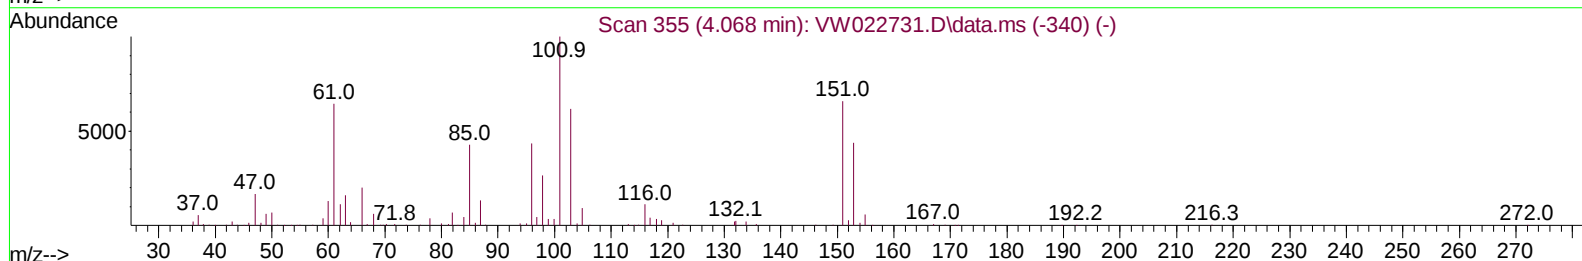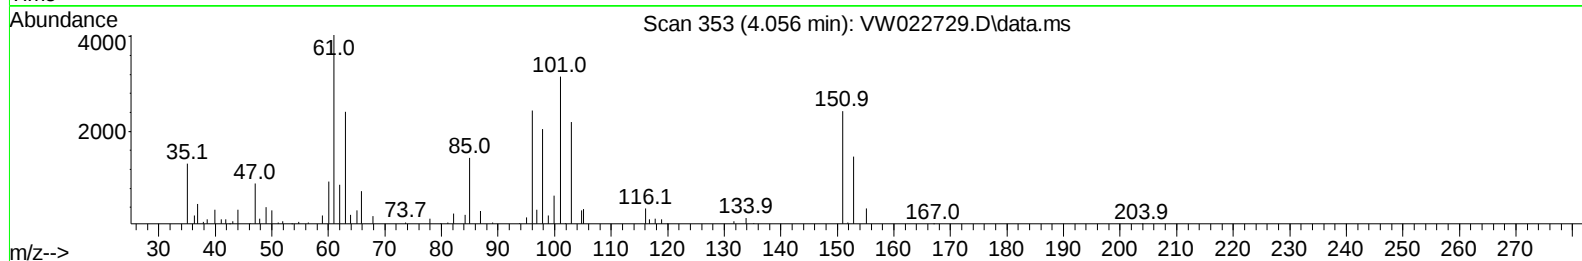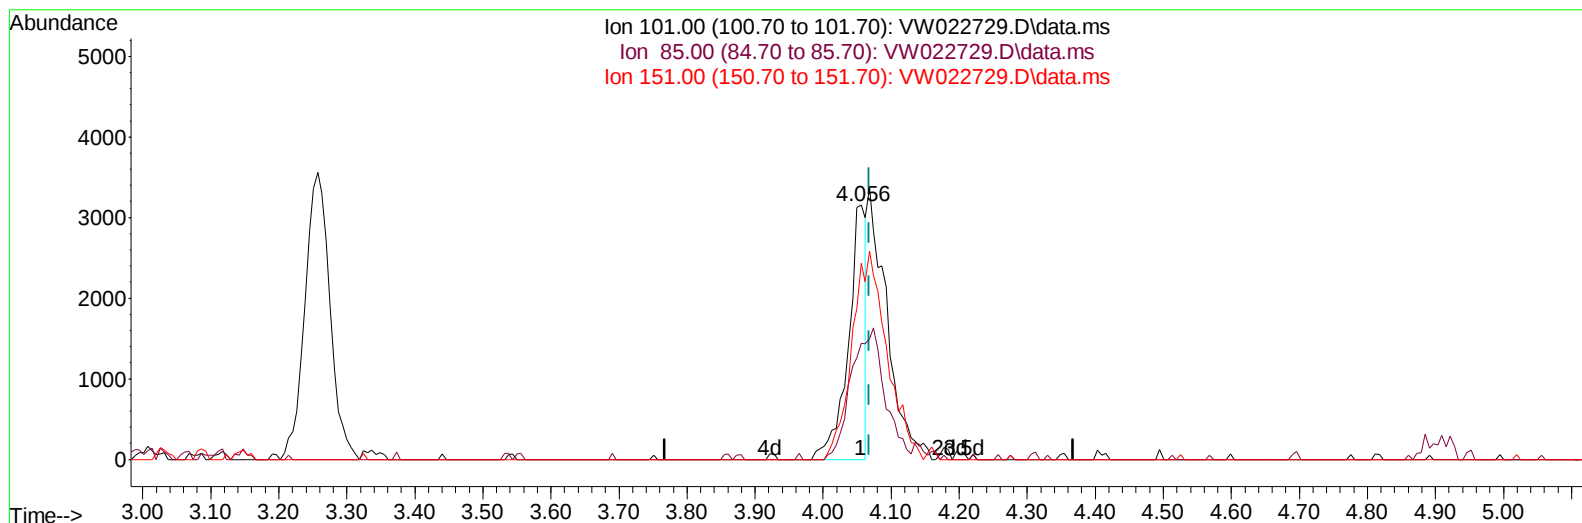

TIC: VW022729.D\data.ms

(10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.056min (-0.012) 1.25 ug/L

response 5749

Ion	Exp%	Act%
101.00	100.00	100.00
85.00	42.90	97.06#
151.00	67.70	159.09#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

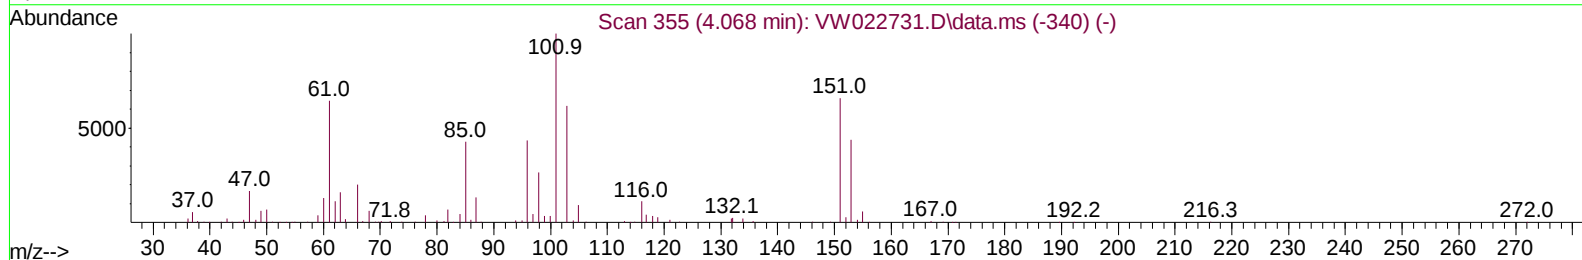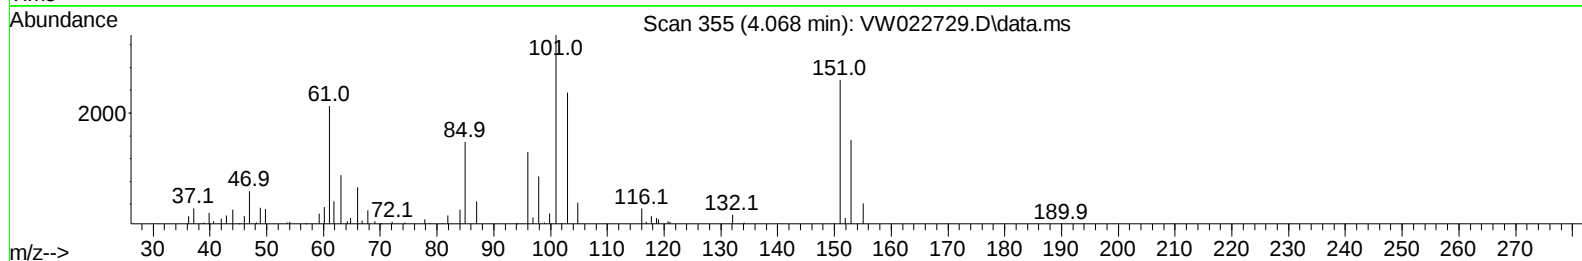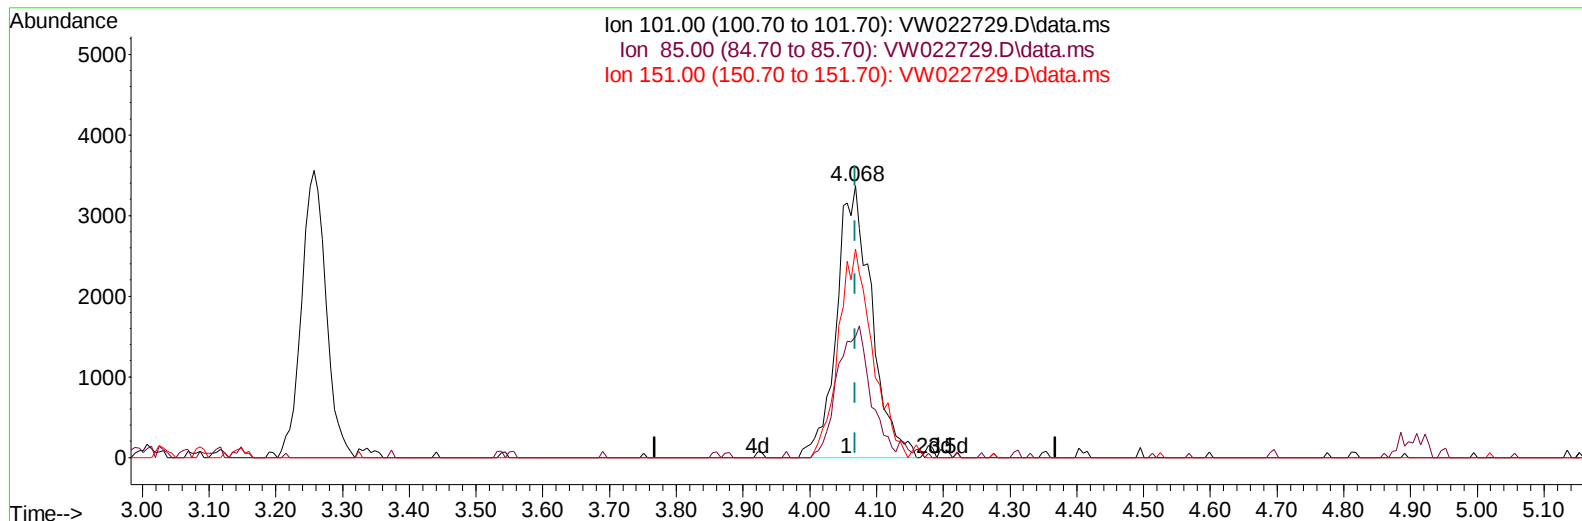

TIC: VW022729.D\data.ms

(10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.068min (-0.000) 2.67 ug/L m

response 12318

Ion	Exp%	Act%
101.00	100.00	100.00
85.00	42.90	45.30
151.00	67.70	74.25
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022729.D
Acq On : 02 May 2022 09:57
Operator : SY/VA
Sample : VSTD2.501
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 02 23:58:08 2022
Response via : Initial Calibration

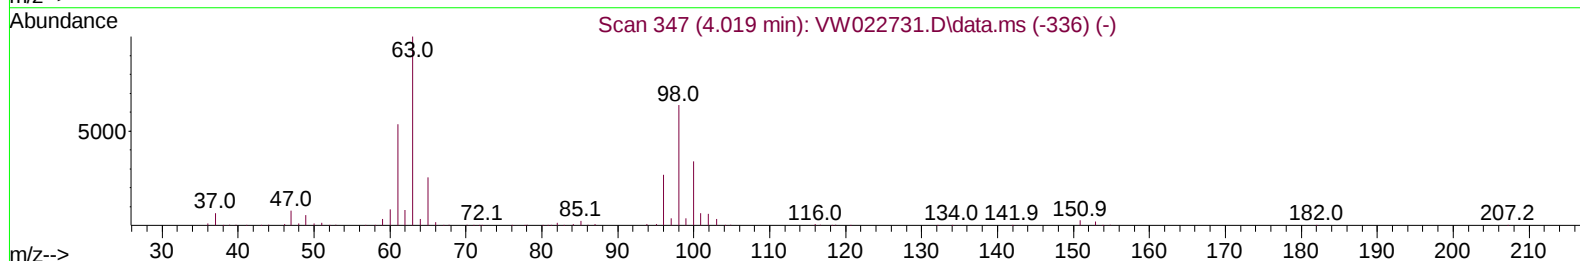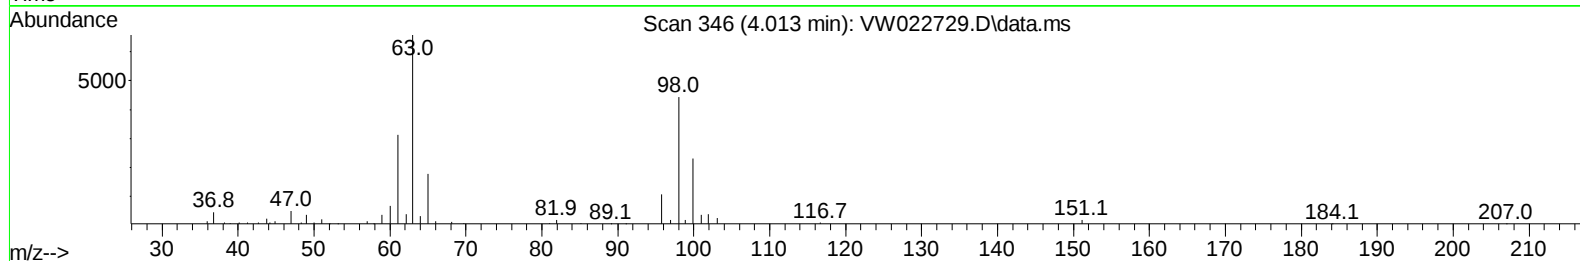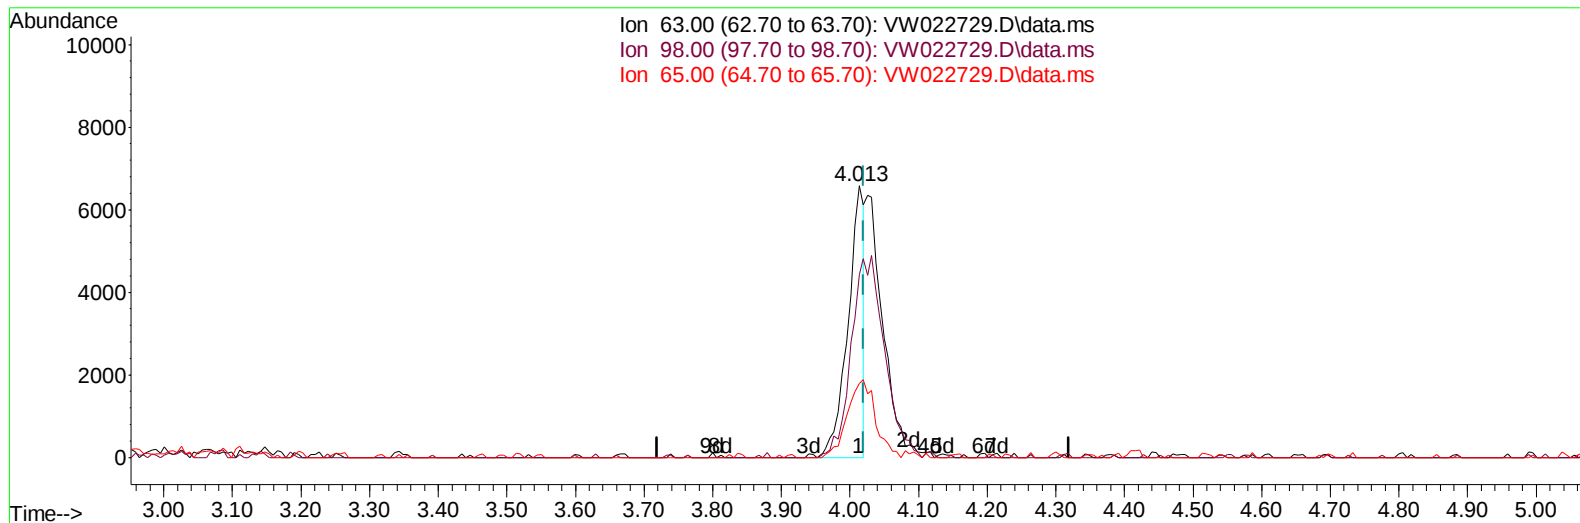

TIC: VW022729.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 1.27 ug/L

response 10816

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	79.72
65.00	23.30	49.19#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

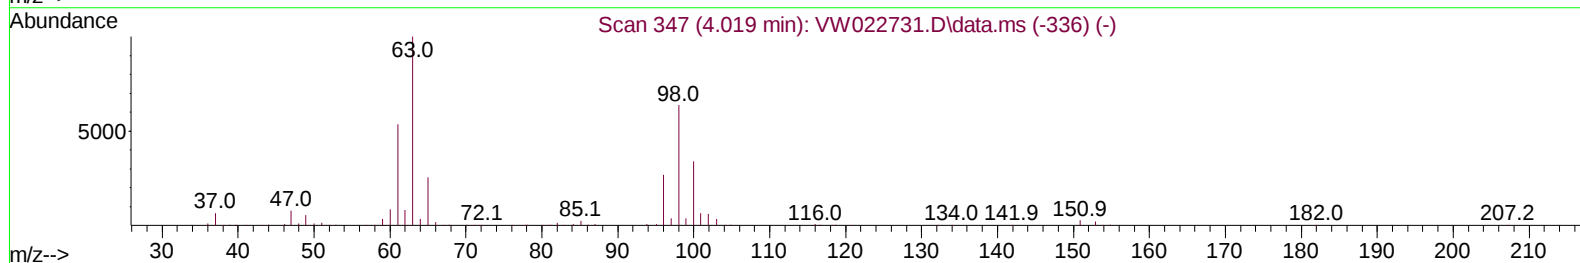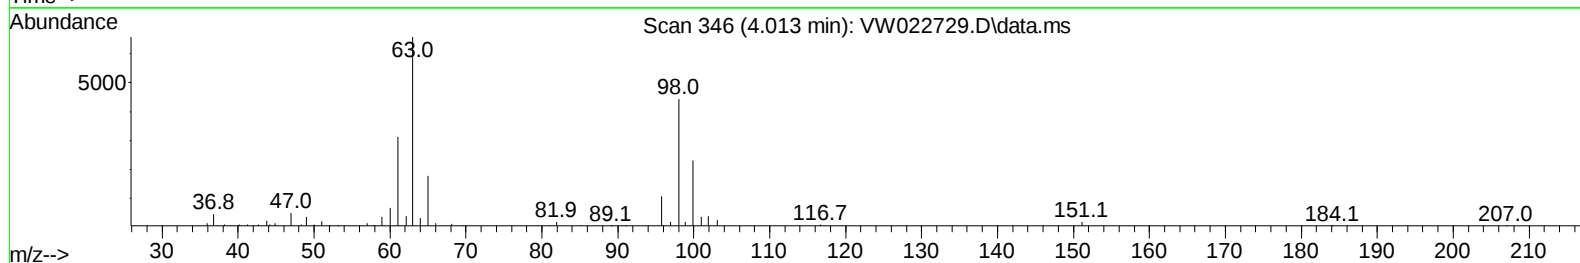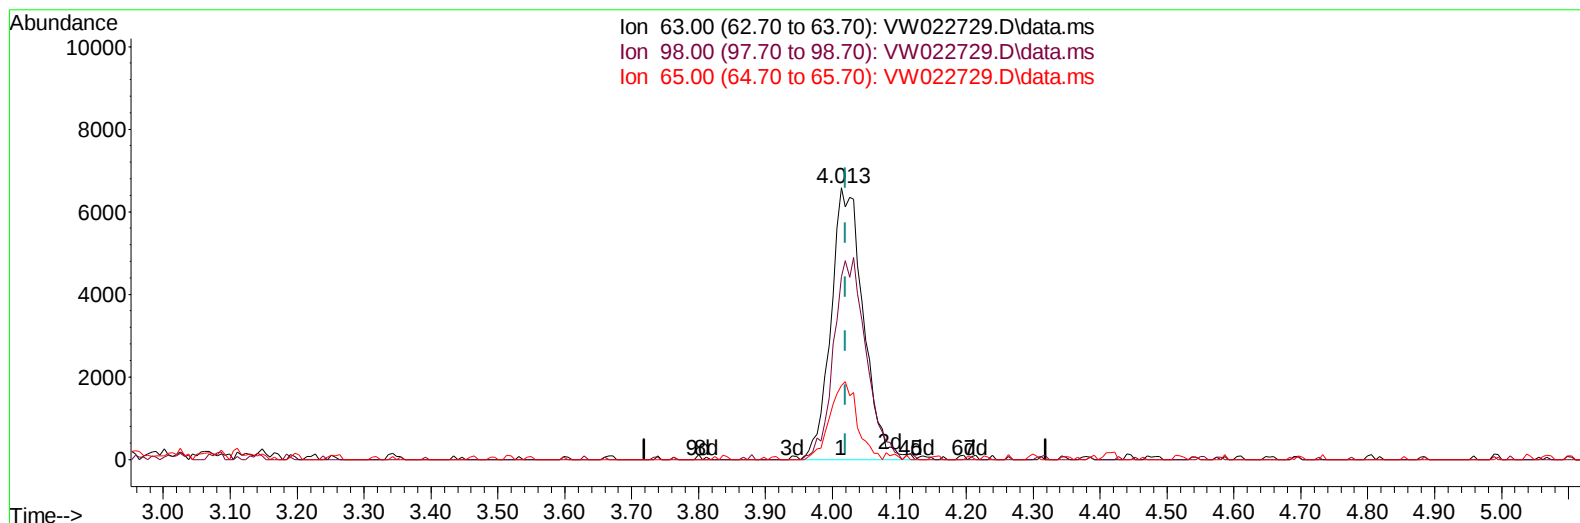

TIC: VW022729.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 2.60 ug/L m

response 22077

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	39.06#
65.00	23.30	24.10
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

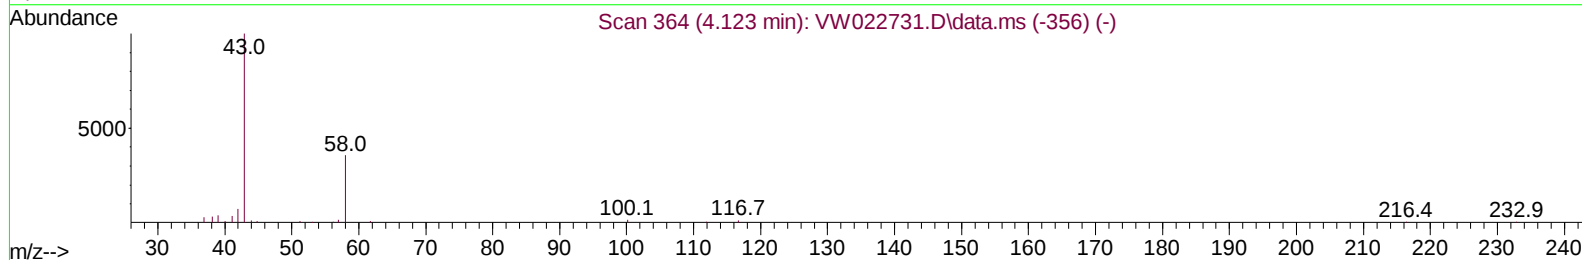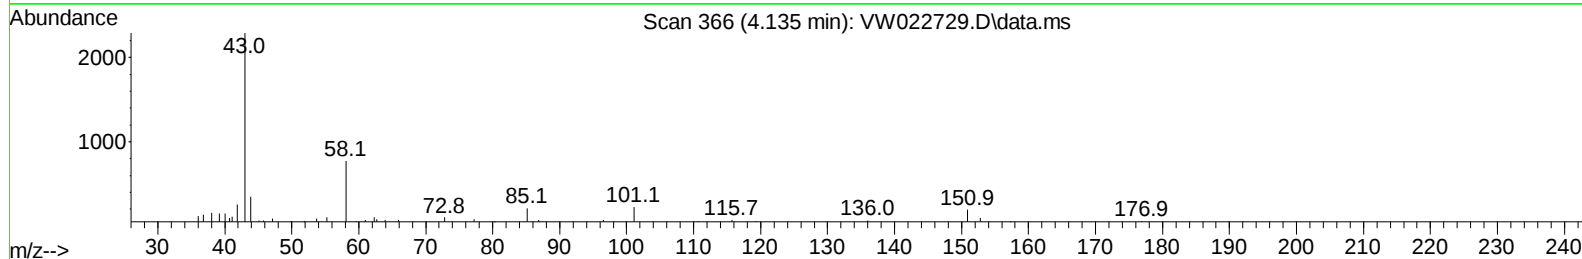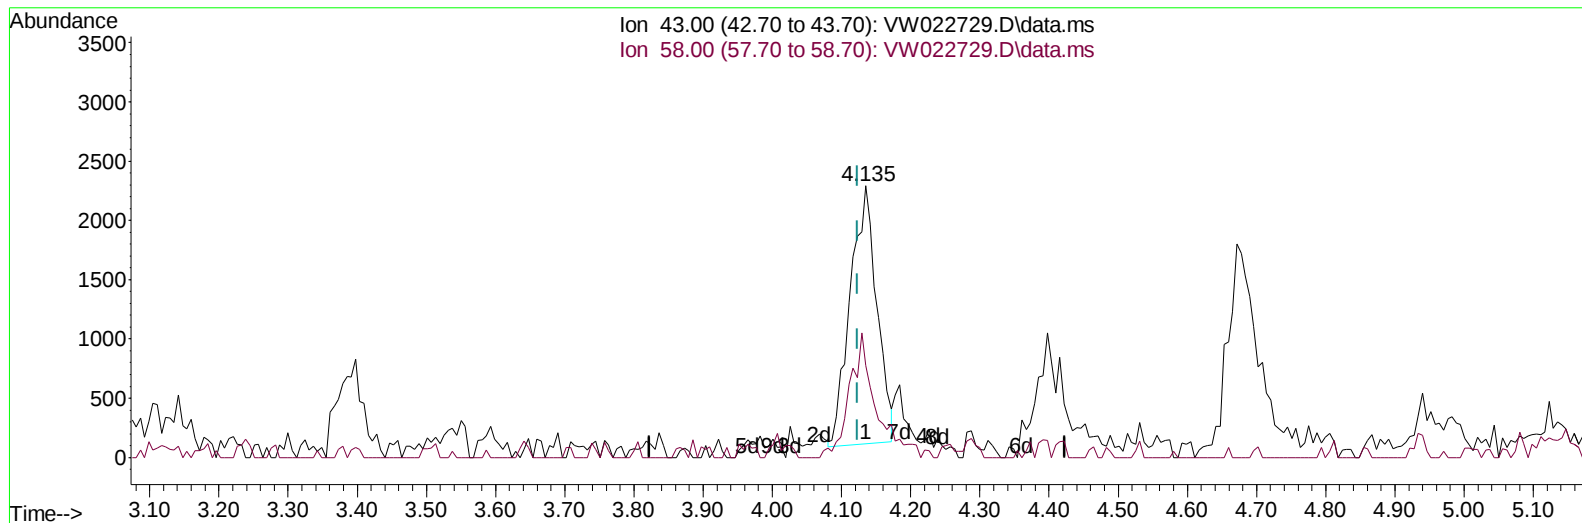

TIC: VW022729.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 6.83 ug/L

response 5788

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	13.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

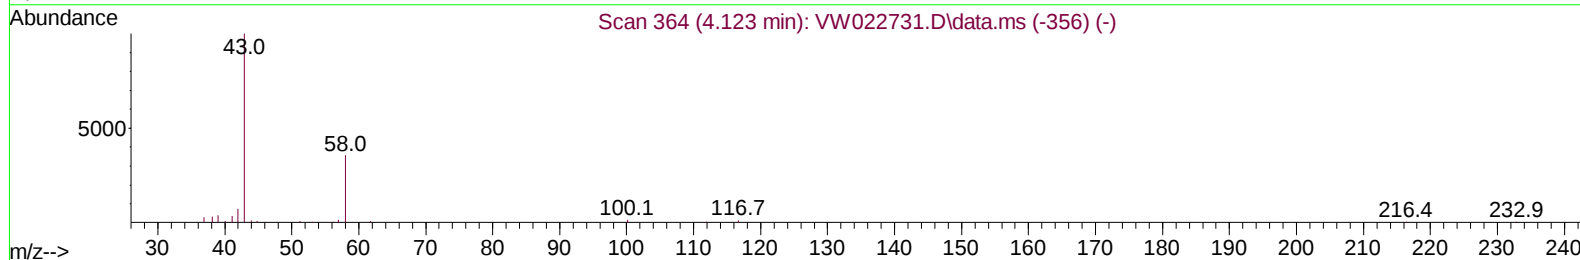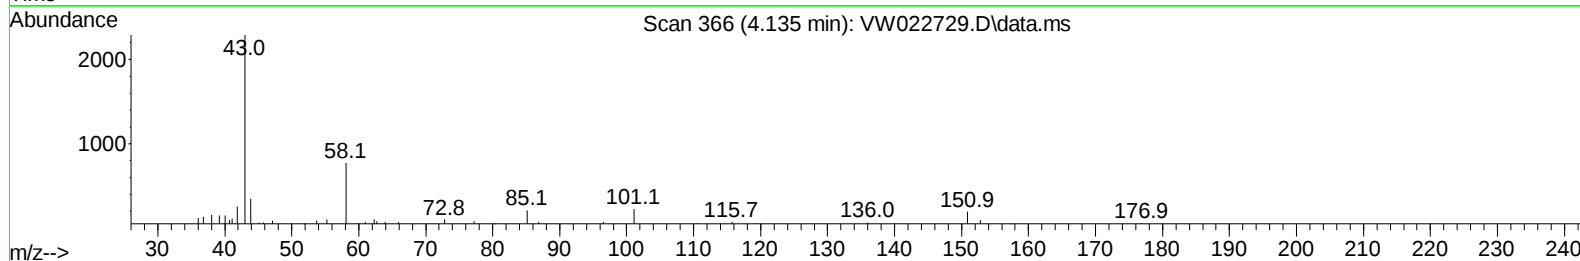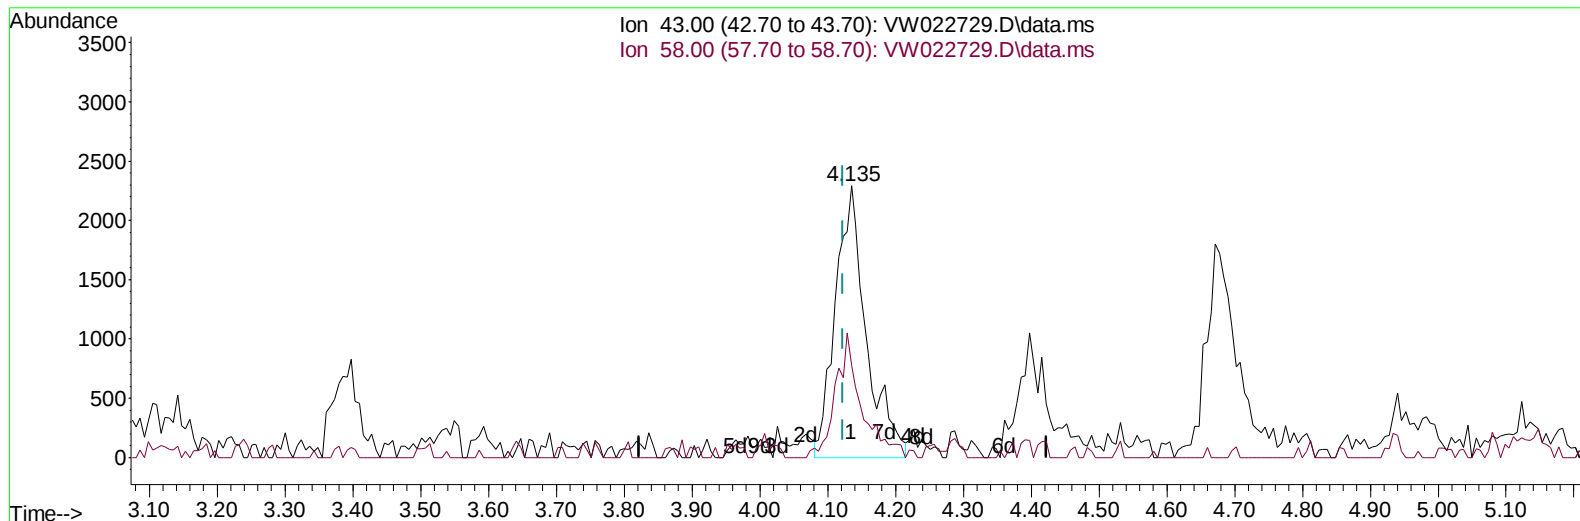

TIC: VW022729.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 8.52 ug/L m

response 7217

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	11.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022729.D
Acq On : 02 May 2022 09:57
Operator : SY/VA
Sample : VSTD2.501
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 02 23:58:08 2022
Response via : Initial Calibration

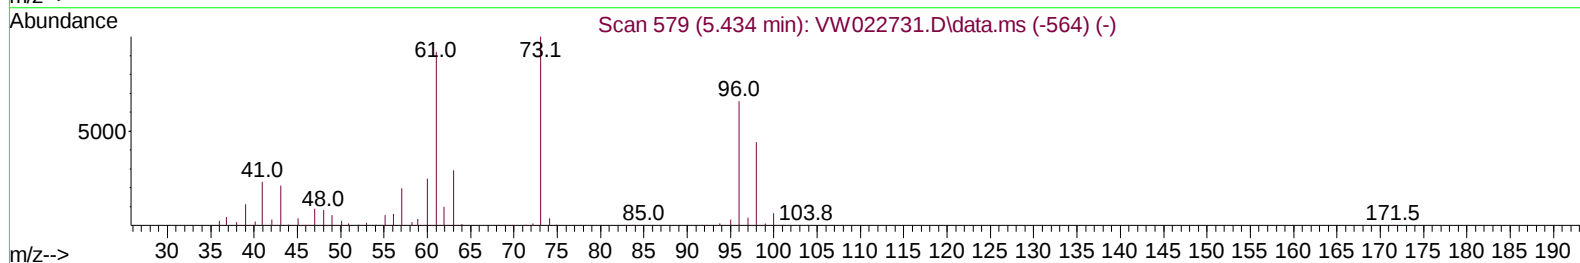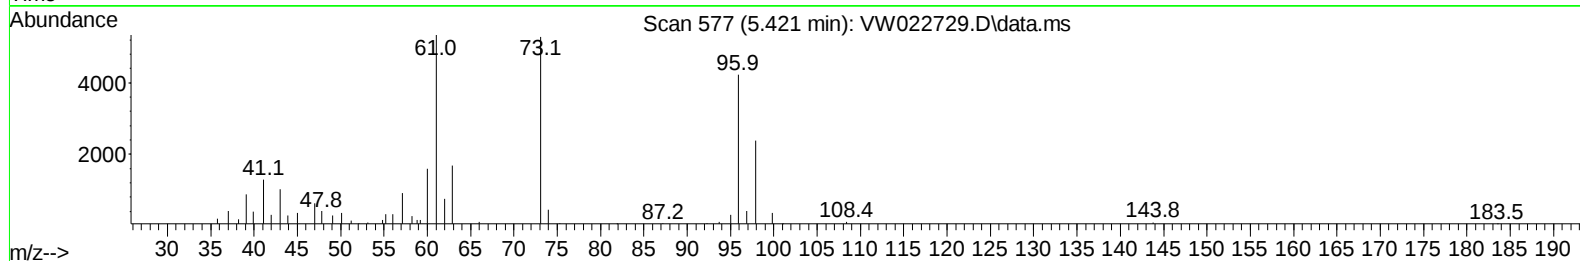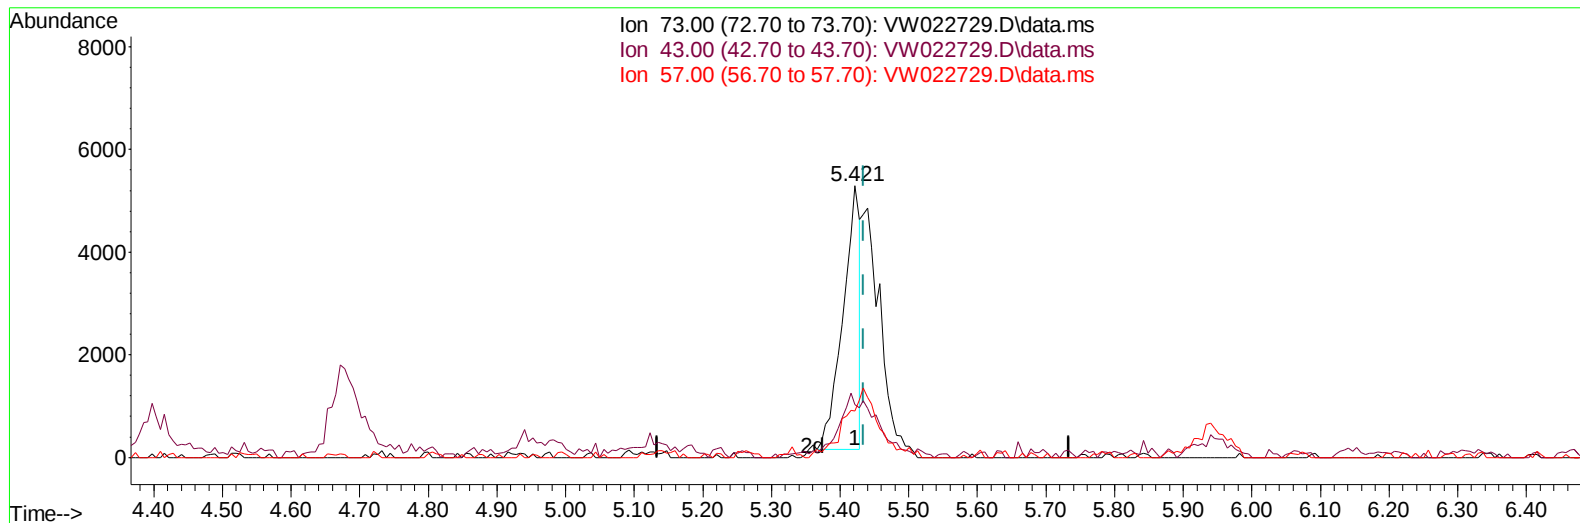

TIC: VW022729.D\data.ms

(18) Methyl tert-butyl Ether (T)

5.421min (-0.012) 1.24 ug/L

response 8753

Ion	Exp%	Act%
73.00	100.00	100.00
43.00	19.90	24.96#
57.00	20.60	46.46#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022729.D
Acq On : 02 May 2022 09:57
Operator : SY/VA
Sample : VSTD2.501
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 02 23:58:08 2022
Response via : Initial Calibration

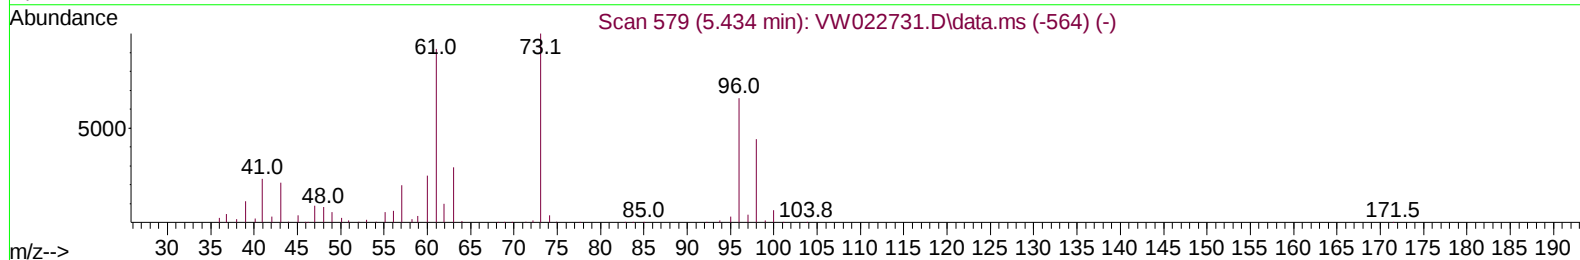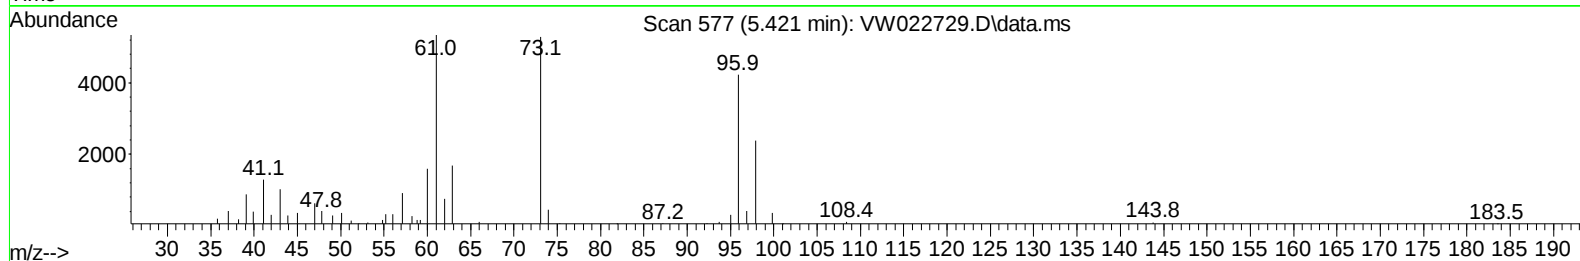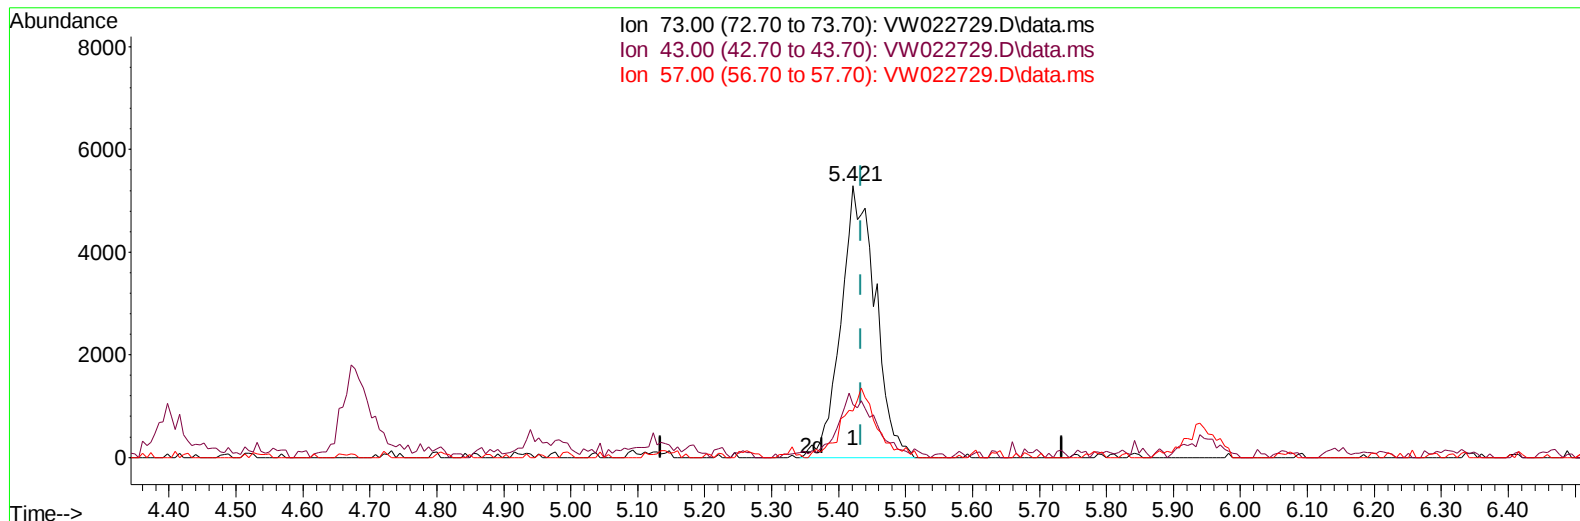

TIC: VW022729.D\data.ms

(18) Methyl tert-butyl Ether (T)

5.421min (-0.012) 2.66 ug/L m

response 18746

Ion	Exp%	Act%
73.00	100.00	100.00
43.00	19.90	11.66#
57.00	20.60	21.70
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022729.D
Acq On : 02 May 2022 09:57
Operator : SY/VA
Sample : VSTD2.501
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 02 23:58:08 2022
Response via : Initial Calibration

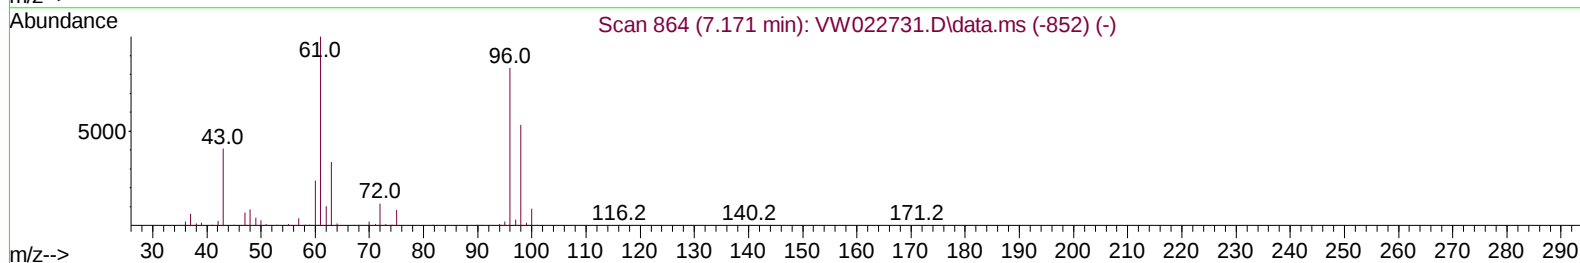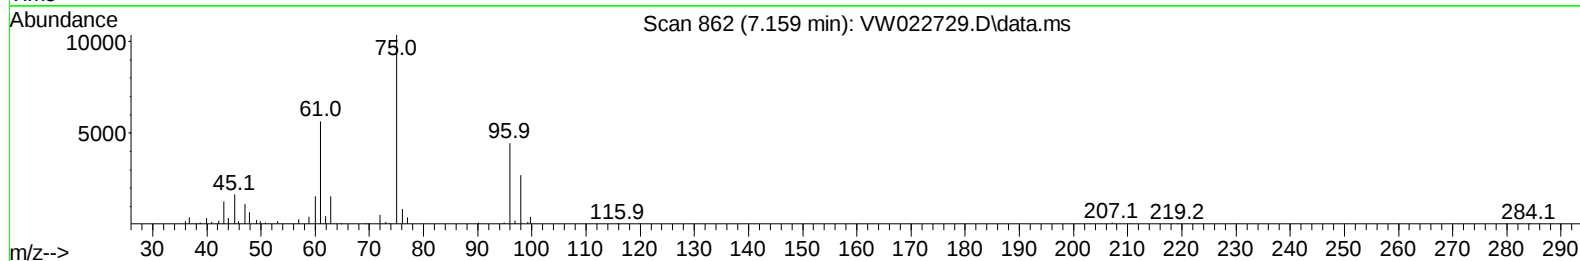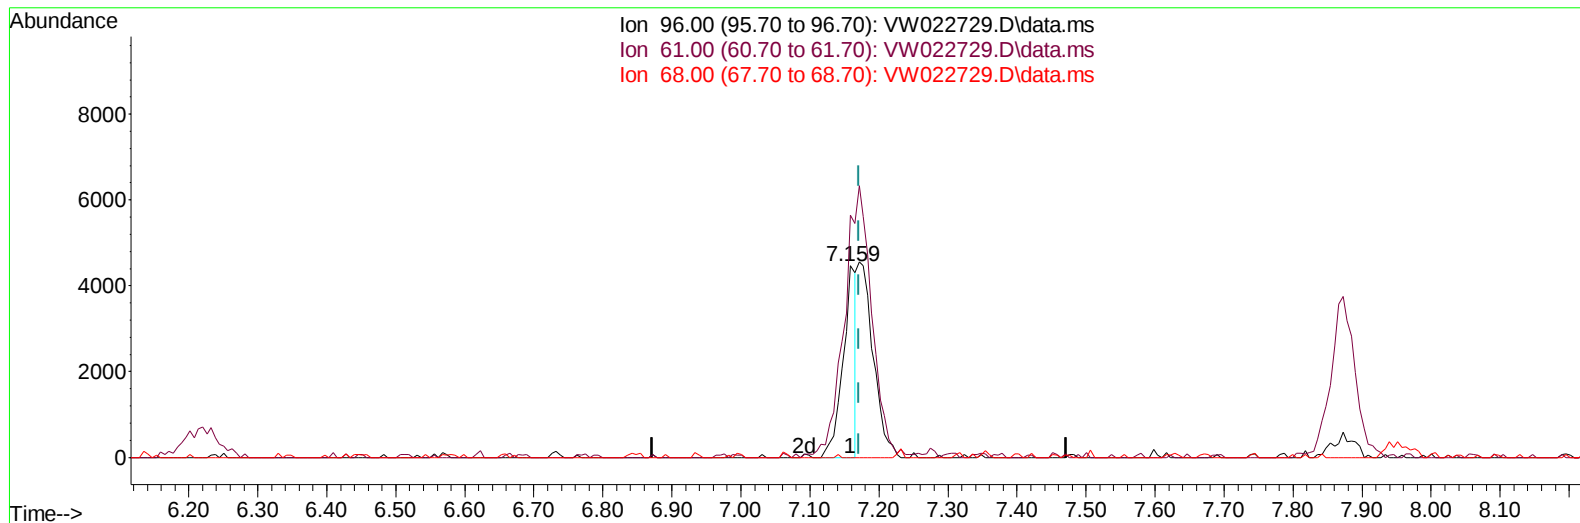

TIC: VW022729.D\data.ms

(20) cis-1,2-Dichloroethene (T)

7.159min (-0.012) 1.18 ug/L

response 5879

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	120.30	126.58
68.00	0.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022729.D
Acq On : 02 May 2022 09:57
Operator : SY/VA
Sample : VSTD2.501
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 02 23:58:08 2022
Response via : Initial Calibration

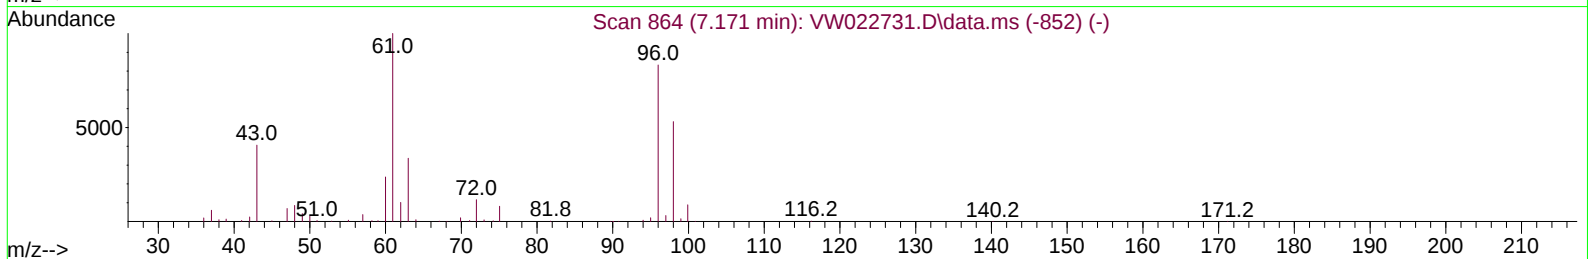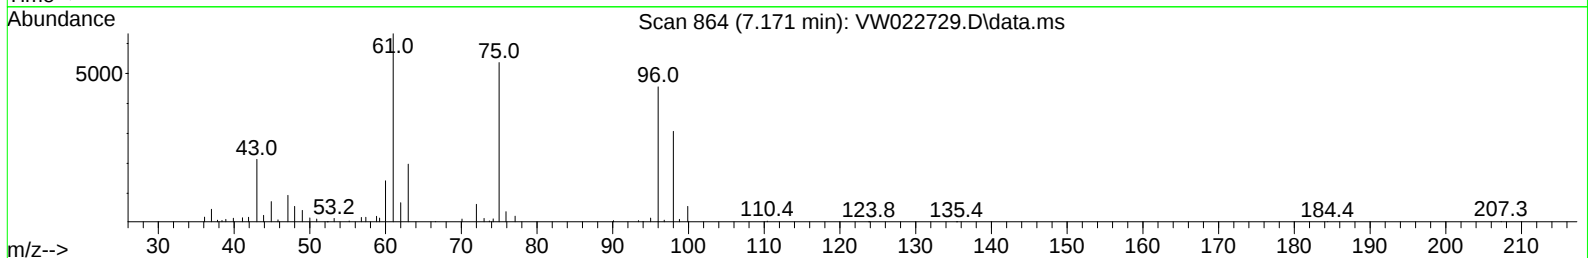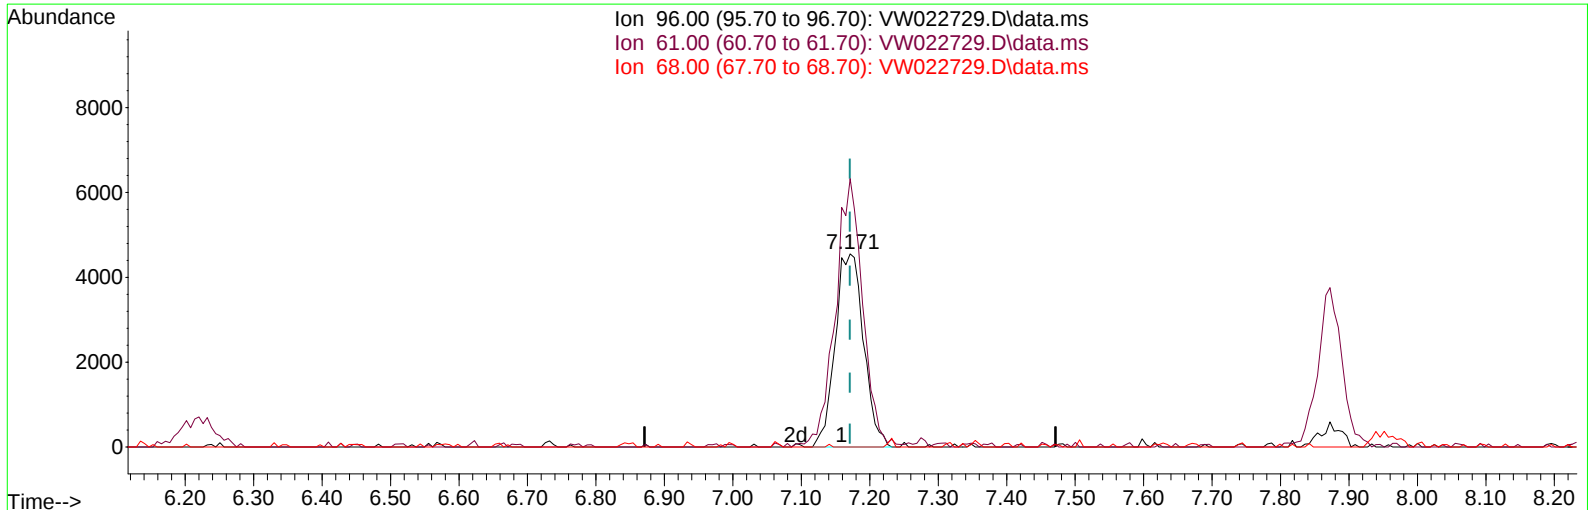

TIC: VW022729.D\data.ms

(20) cis-1,2-Dichloroethene (T)

7.171min (-0.000) 2.64 ug/L m

response 13091

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	120.30	138.99
68.00	0.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022729.D
Acq On : 02 May 2022 09:57
Operator : SY/VA
Sample : VSTD2.501
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 02 23:58:08 2022
Response via : Initial Calibration

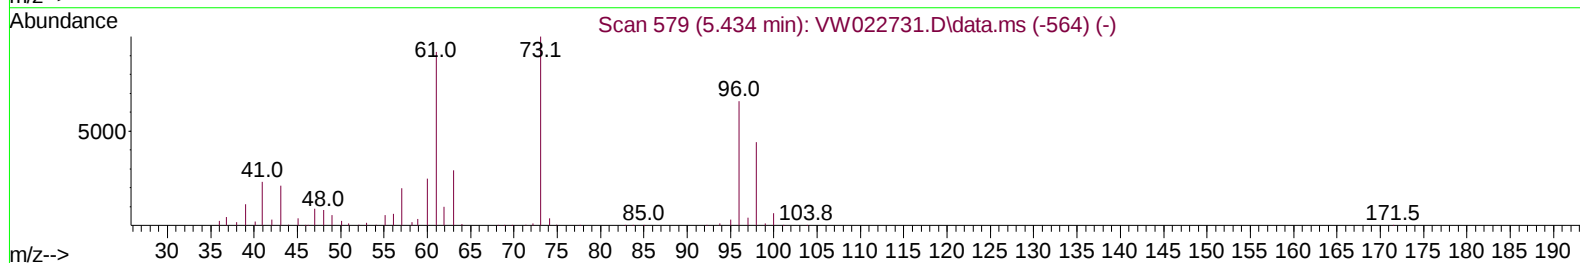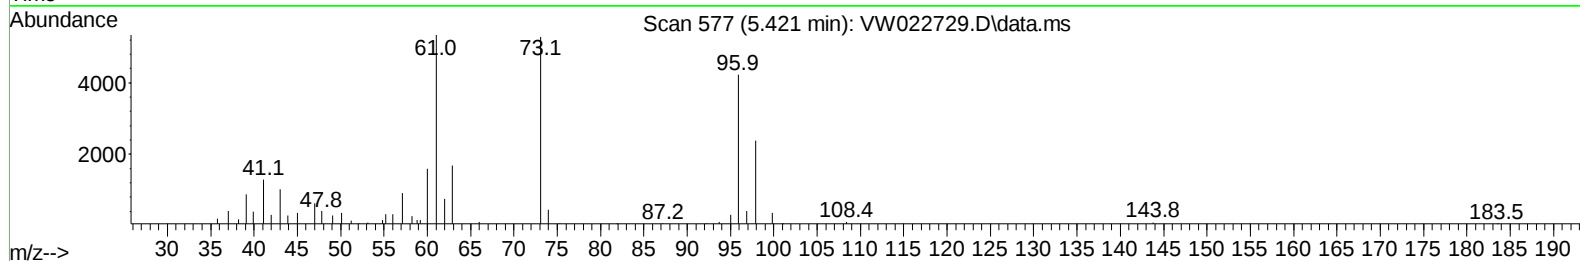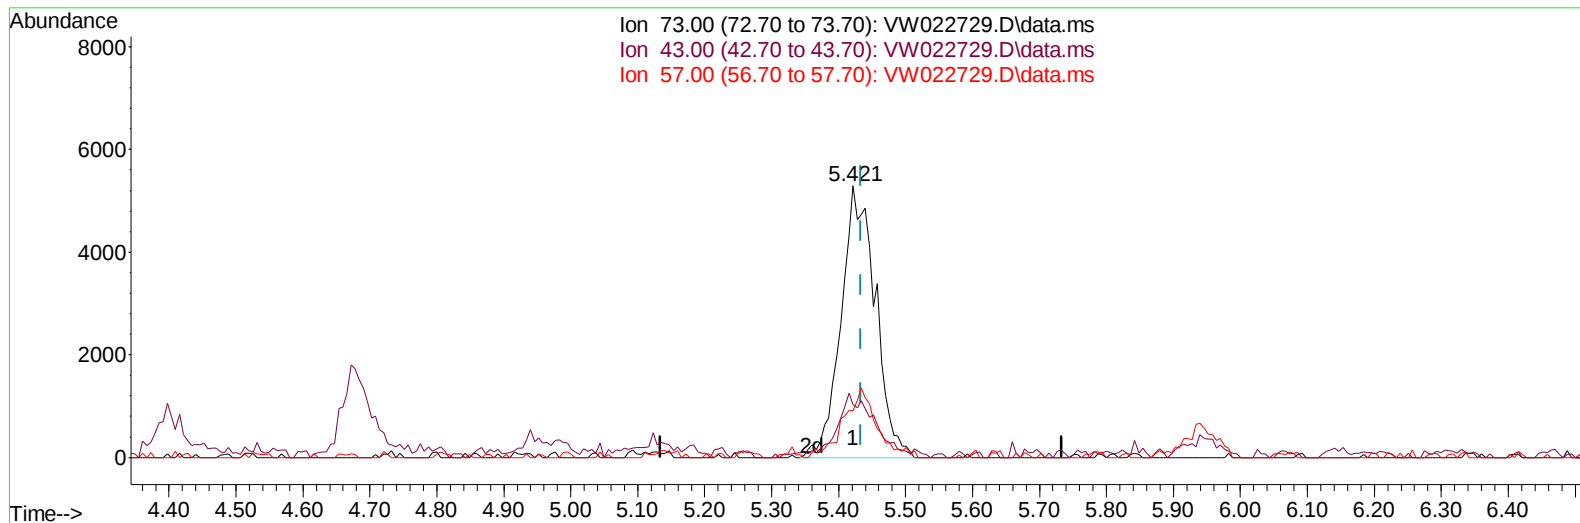

TIC: VW022729.D\data.ms

(18) Methyl tert-butyl Ether (T)

5.421min (-0.012) 2.66 ug/L m

response 18746

Ion	Exp%	Act%
73.00	100.00	100.00
43.00	19.90	11.66#
57.00	20.60	21.70
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022729.D
Acq On : 02 May 2022 09:57
Operator : SY/VA
Sample : VSTD2.501
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 02 23:58:08 2022
Response via : Initial Calibration

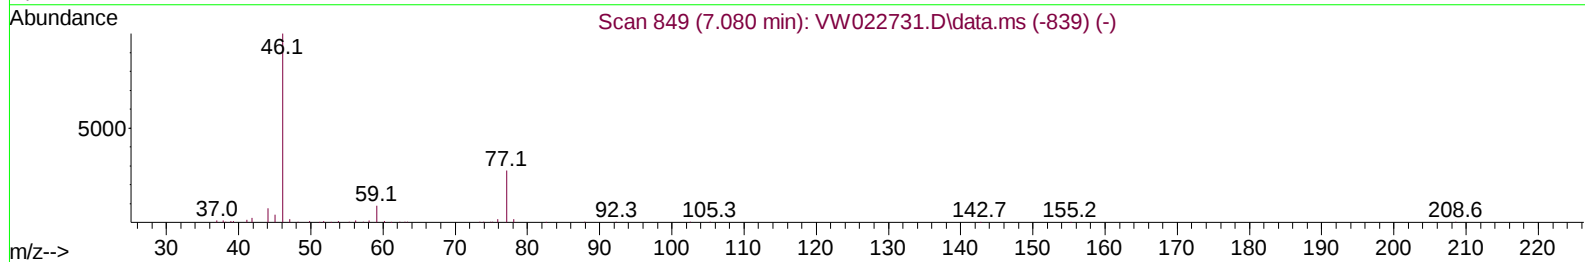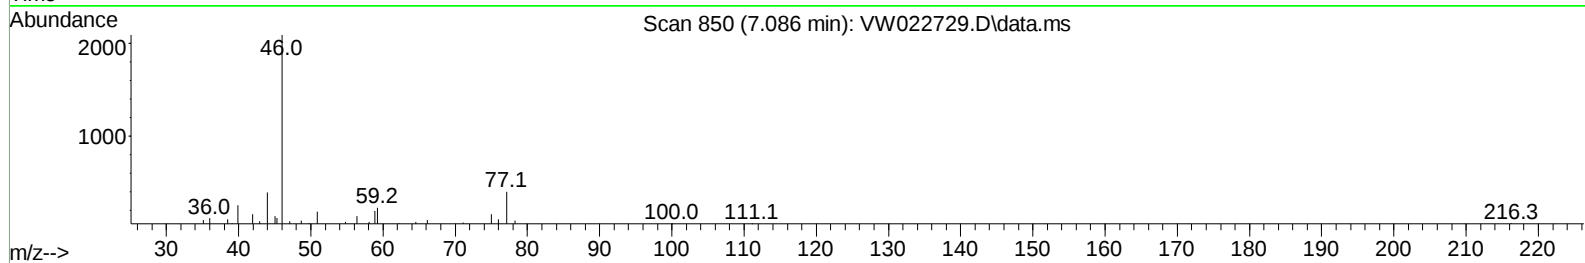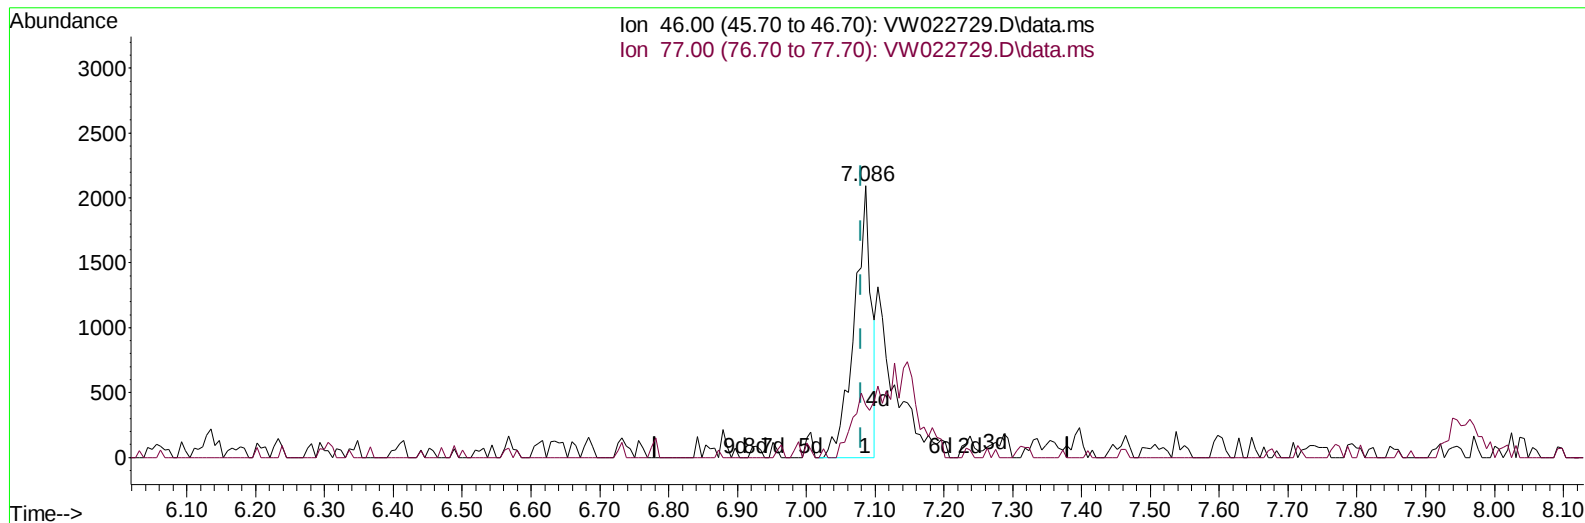

TIC: VW022729.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 2.89 ug/L

response 3584

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	23.88
0.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

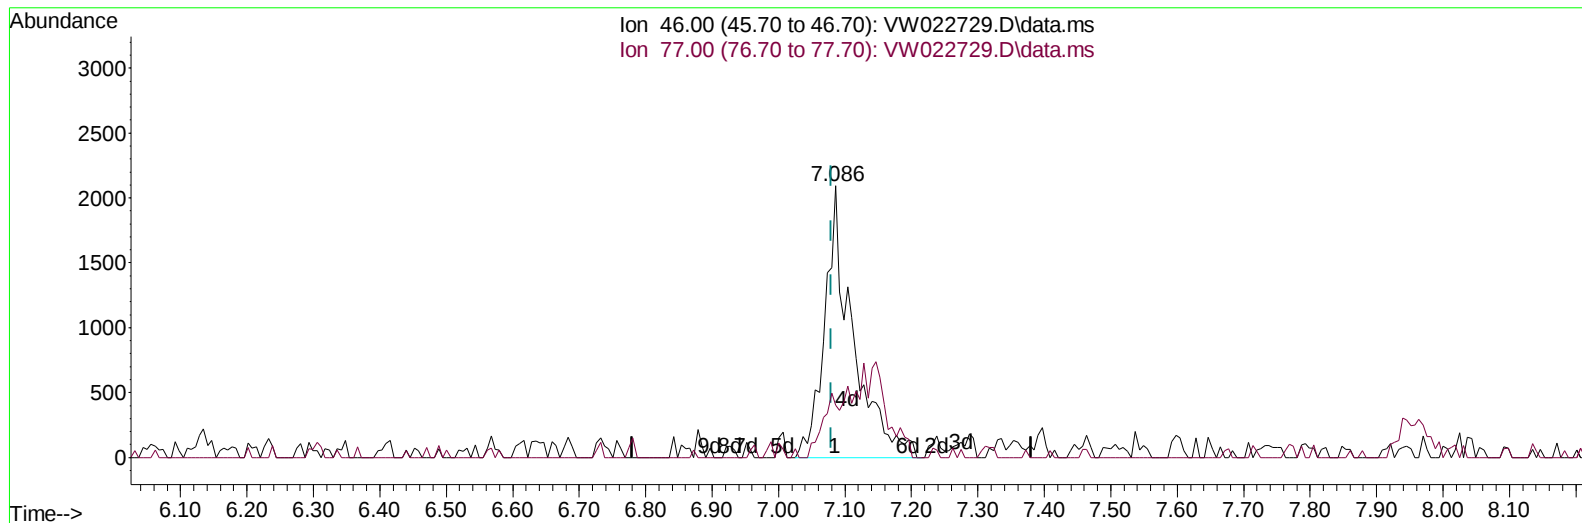




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

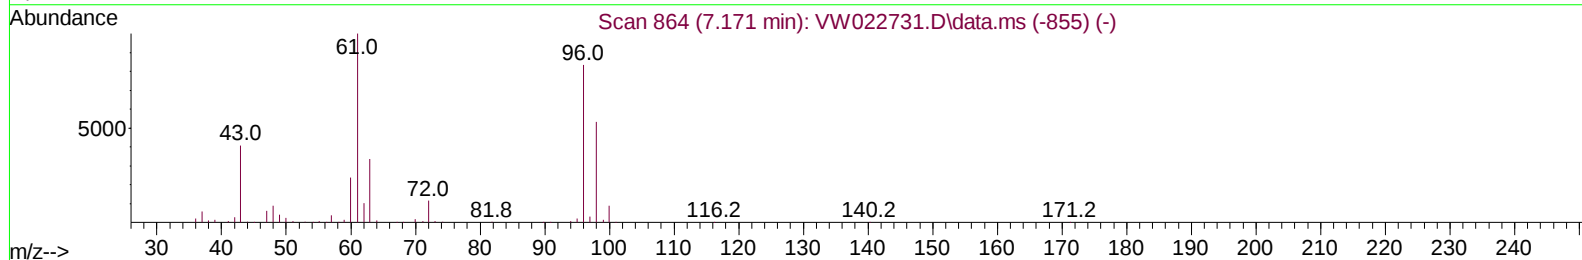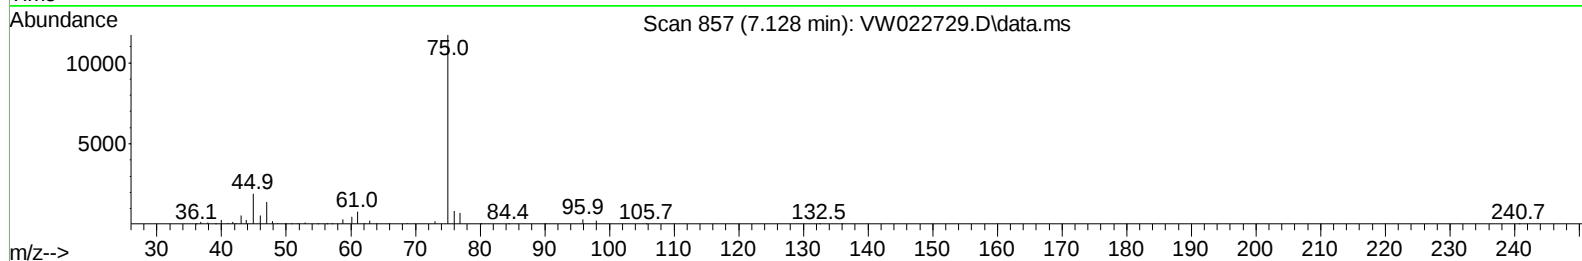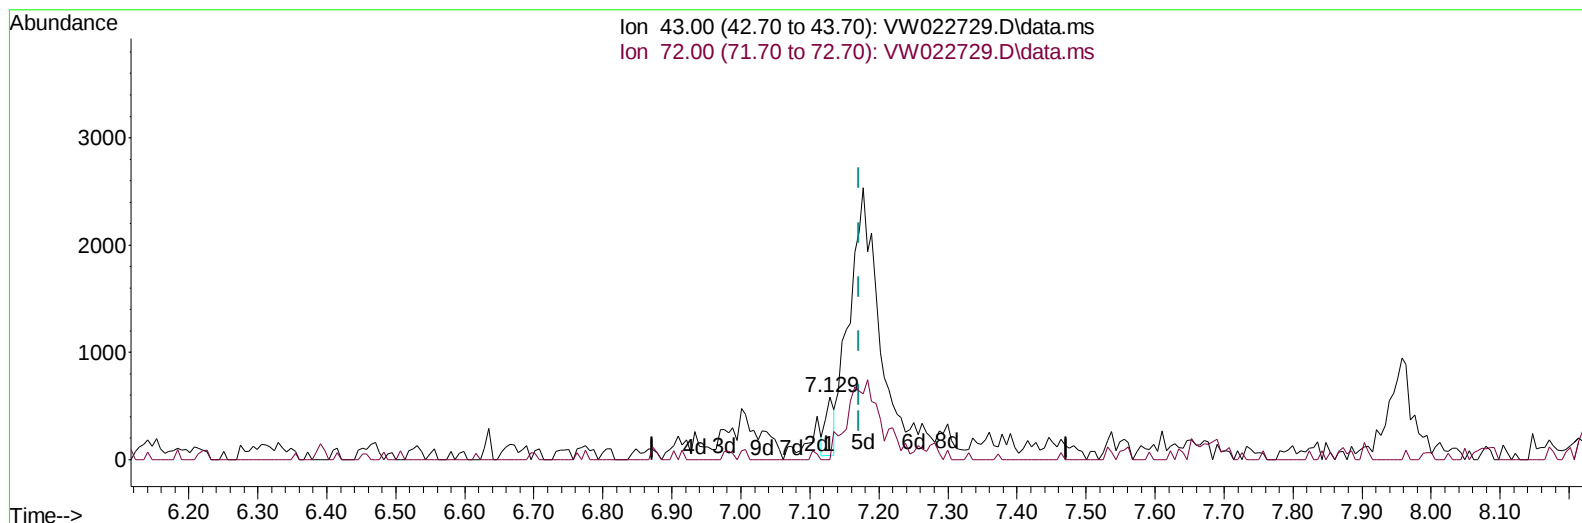

TIC: VW022729.D\data.ms

(22) 2-Butanone (T)

7.128min (-0.043) 0.37 ug/L

response 480

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.20	36.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

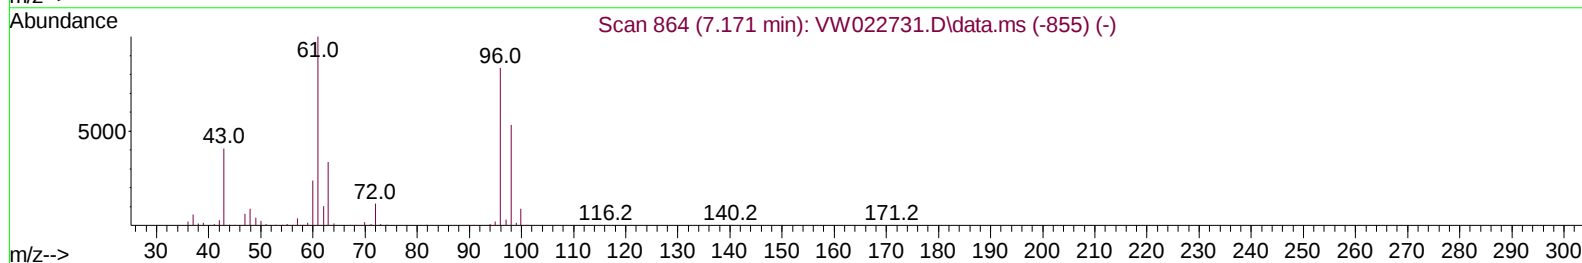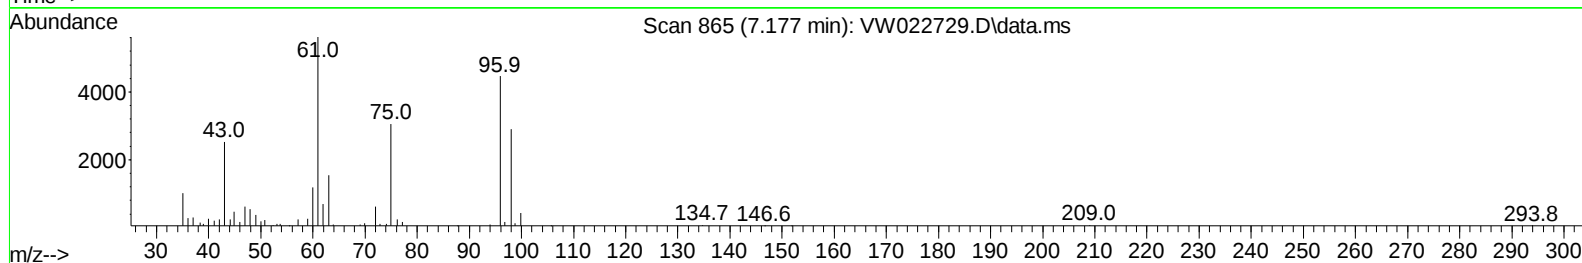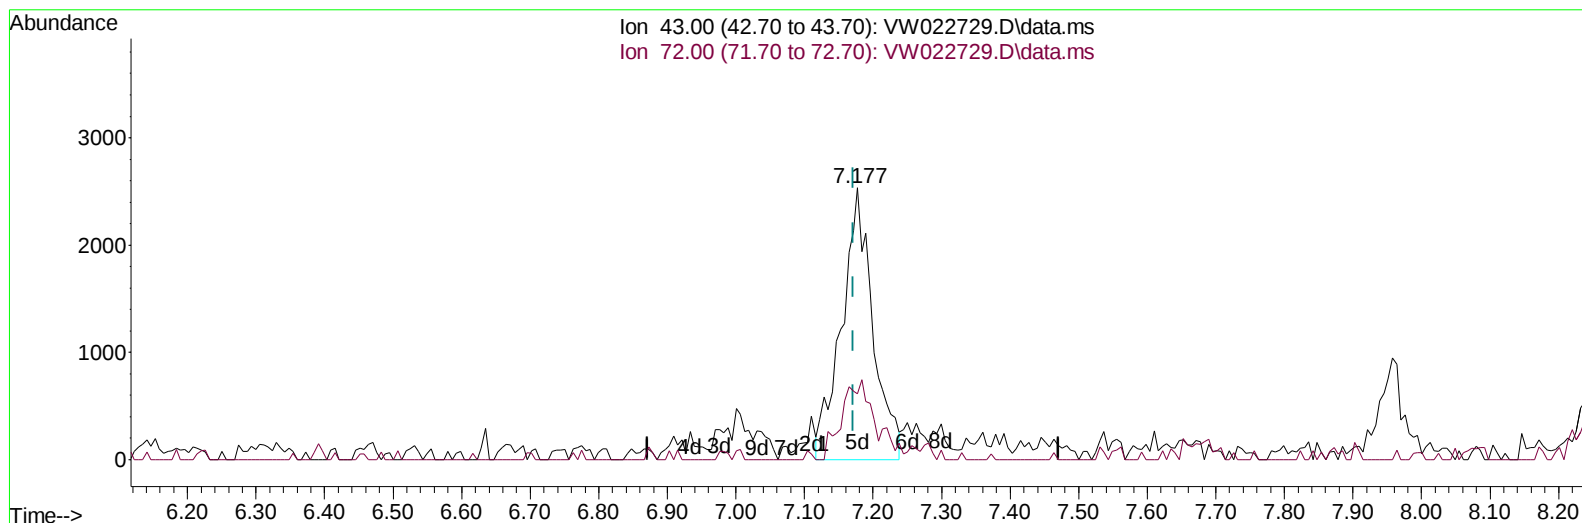

TIC: VW022729.D\data.ms

(22) 2-Butanone (T)

7.177min (+ 0.006) 6.11 ug/L m

response 7990

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.20	2.19#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	320624	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	299888	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	160353	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	17096	2.599	ug/L	0.00
7) Chloroethane-d5	2.879	69	10027	2.343	ug/L	0.00
11) 1,1-Dichloroethene-d2	4.013	63	22077m	2.600	ug/L	0.00
21) 2-Butanone-d5	7.086	46	6133m	4.945	ug/L	0.00
24) Chloroform-d	7.653	84	22004	2.342	ug/L	0.00
26) 1,2-Dichloroethane-d4	8.311	65	12304	2.388	ug/L	0.00
32) Benzene-d6	8.275	84	40837	2.363	ug/L	0.00
36) 1,2-Dichloropropane-d6	9.274	67	11416	2.351	ug/L	0.00
41) Toluene-d8	10.323	98	38917	2.331	ug/L	0.00
43) trans-1,3-Dichloroprop...	10.573	79	4721	2.112	ug/L	0.00
47) 2-Hexanone-d5	10.927	63	3754	4.050	ug/L	0.00
56) 1,1,2,2-Tetrachloroeth...	12.695	84	10524	2.325	ug/L	0.00
66) 1,2-Dichlorobenzene-d4	13.847	152	12489	2.228	ug/L	0.00
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.007	85	3647	2.108	ug/L #	72
3) Chloromethane	2.215	50	9348	2.768	ug/L	100
5) Vinyl chloride	2.361	62	18954	2.796	ug/L	100
6) Bromomethane	2.776	94	12687	2.915	ug/L	91
8) Chloroethane	2.916	64	8528	2.609	ug/L	96
9) Trichlorofluoromethane	3.257	101	9070	2.928	ug/L	91
10) 1,1,2-Trichloro-1,2,2-...	4.068	101	12318m	2.671	ug/L	
12) 1,1-Dichloroethene	4.044	96	11009	2.681	ug/L	83
13) Acetone	4.135	43	7217m	8.518	ug/L	
14) Carbon disulfide	4.391	76	31106	2.763	ug/L	96
15) Methyl Acetate	4.672	43	4674	2.401	ug/L #	81
16) Methylene chloride	4.915	84	14872	3.170	ug/L	99
17) trans-1,2-Dichloroethene	5.421	96	12881	2.787	ug/L	95
18) Methyl tert-butyl Ether	5.421	73	18746m	2.663	ug/L	
19) 1,1-Dichloroethane	6.220	63	20837	2.660	ug/L	96
20) cis-1,2-Dichloroethene	7.171	96	13091m	2.637	ug/L	
22) 2-Butanone	7.177	43	7990m	6.111	ug/L	
23) Bromochloromethane	7.519	128	6401	2.754	ug/L	91
25) Chloroform	7.677	83	22969	2.652	ug/L	99
27) 1,2-Dichloroethane	8.403	62	15688	2.717	ug/L #	94
29) Cyclohexane	7.958	56	17314	2.670	ug/L	98
30) 1,1,1-Trichloroethane	7.872	97	18988	2.679	ug/L	96
31) Carbon tetrachloride	8.073	117	18321	2.764	ug/L	99
33) Benzene	8.323	78	50228	2.843	ug/L	100
34) Trichloroethene	9.092	95	13365	2.751	ug/L	95
35) Methylcyclohexane	9.335	83	21379	2.679	ug/L	96
37) 1,2-Dichloropropane	9.366	63	12234	2.862	ug/L	100
38) Bromodichloromethane	9.640	83	16245	2.675	ug/L #	98
39) cis-1,3-Dichloropropene	10.073	75	15745	2.375	ug/L	100
40) 4-Methyl-2-pentanone	10.207	43	14682	5.449	ug/L	98
42) Toluene	10.390	91	52499	2.652	ug/L	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) trans-1,3-Dichloropropene	10.610	75	14048	2.374	ug/L	91
45) 1,1,2-Trichloroethane	10.786	97	9797	2.741	ug/L	92
46) Tetrachloroethene	10.866	164	9773	2.677	ug/L	96
48) 2-Hexanone	10.969	43	9373	5.206	ug/L #	90
49) Dibromochloromethane	11.128	129	10716	2.491	ug/L	98
50) 1,2-Dibromoethane	11.231	107	9640	2.686	ug/L #	93
51) Chlorobenzene	11.652	112	34784	2.665	ug/L	95
52) Ethylbenzene	11.731	91	57574	2.614	ug/L	100
53) m,p-Xylene	11.835	106	21729	2.504	ug/L	86
54) o-Xylene	12.164	106	20731	2.489	ug/L	94
55) Styrene	12.176	104	33222	2.348	ug/L	98
57) 1,1,2,2-Tetrachloroethane	12.707	83	12057	2.701	ug/L #	98
59) Bromoform	12.353	173	5384	2.369	ug/L	98
60) Isopropylbenzene	12.463	105	55474	2.525	ug/L	98
61) 1,2,3-Trichloropropane	12.768	75	9272	2.894	ug/L	97
62) 1,3,5-Trimethylbenzene	12.938	105	31564	2.583	ug/L	98
63) 1,2,4-Trimethylbenzene	13.249	105	45645	2.487	ug/L	94
64) 1,3-Dichlorobenzene	13.493	146	26084	2.659	ug/L	95
65) 1,4-Dichlorobenzene	13.572	146	27659	2.730	ug/L	93
67) 1,2-Dichlorobenzene	13.871	146	23620	2.632	ug/L	98
68) 1,2-Dibromo-3-chloropr...	14.487	75	2007	2.866	ug/L #	78
69) 1,3,5-Trichlorobenzene	14.621	180	16867	2.591	ug/L	98
70) 1,2,4-trichlorobenzene	15.127	180	12946	2.472	ug/L	94
71) Naphthalene	15.359	128	25536	2.243	ug/L #	95
72) 1,2,3-Trichlorobenzene	15.554	180	11849	2.553	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022729.D
 Acq On : 02 May 2022 09:57
 Operator : SY/VA
 Sample : VSTD2.501
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.5401

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 02 23:59:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 02 23:58:08 2022
 Response via : Initial Calibration

