




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022738.D
 Acq On : 02 May 2022 14:39
 Operator : SY/VA
 Sample : N2603-15RE
 Misc : 6.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW495RE

Manual IntegrationsAPPROVED

Quant Time: May 03 01:43:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

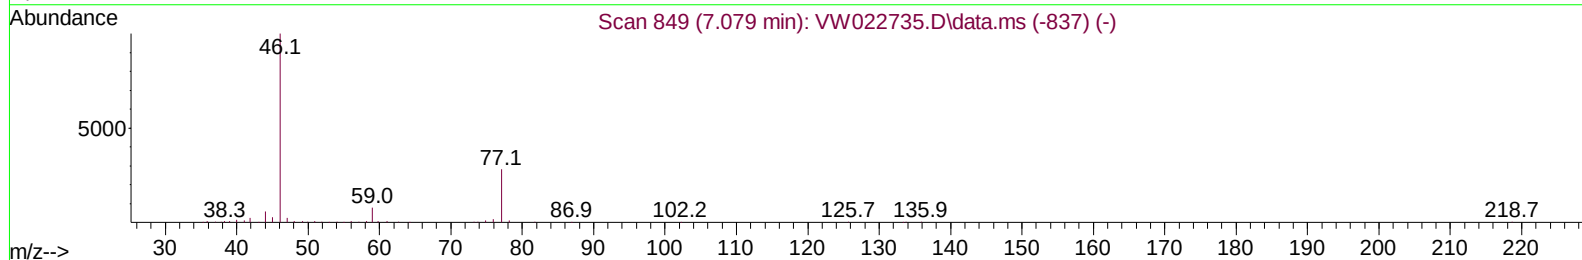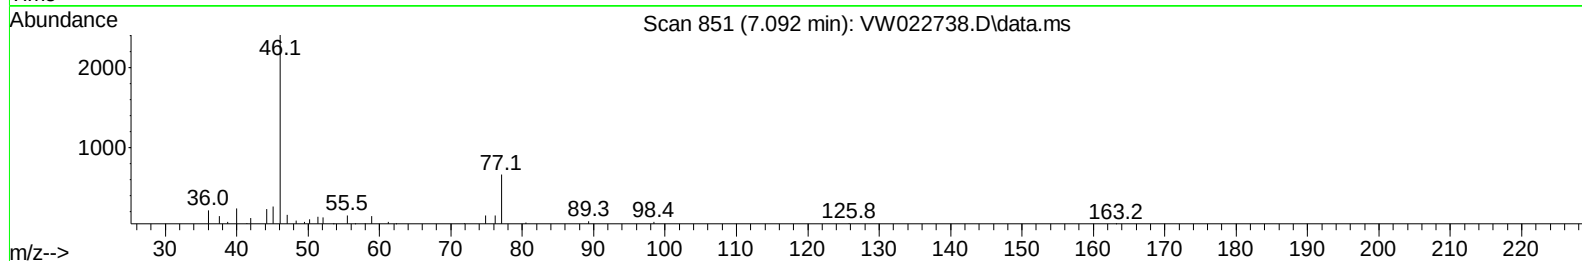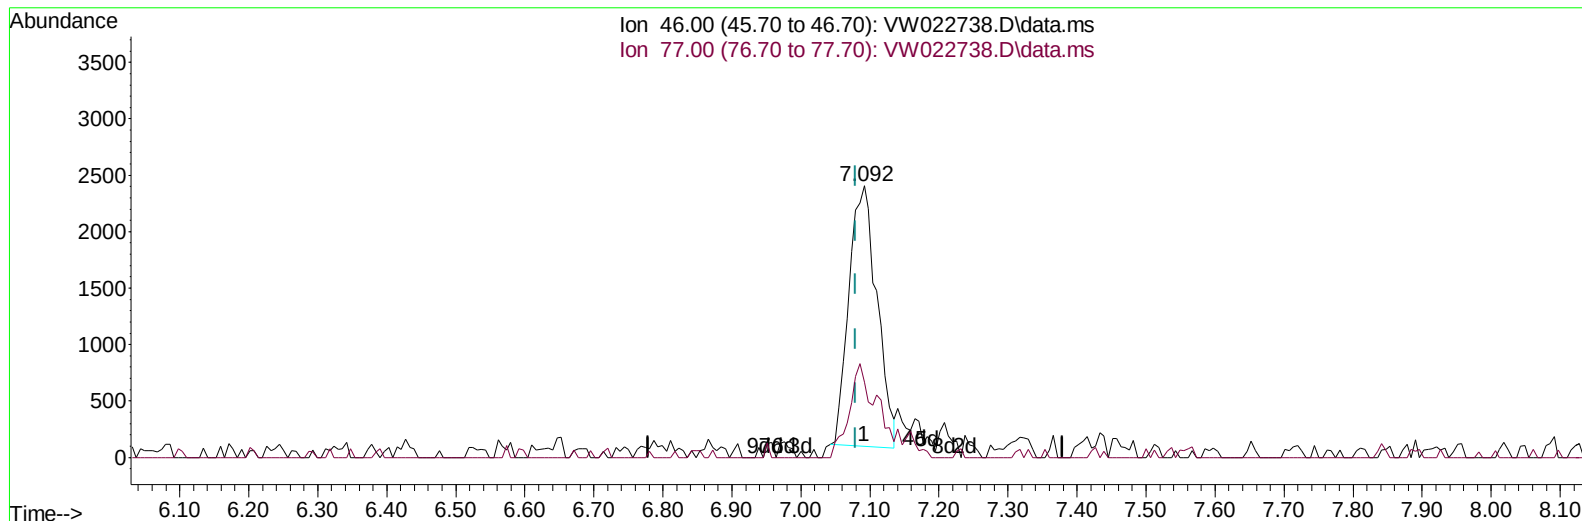

TIC: VW022738.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.012) 28.46 ug/L

response 6480

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	25.26
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022738.D
 Acq On : 02 May 2022 14:39
 Operator : SY/VA
 Sample : N2603-15RE
 Misc : 6.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW495RE

Manual IntegrationsAPPROVED

Quant Time: May 03 01:43:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

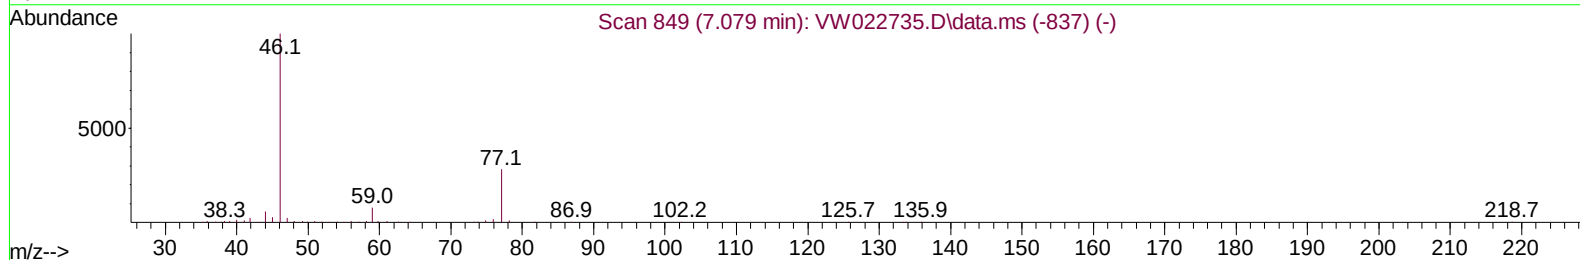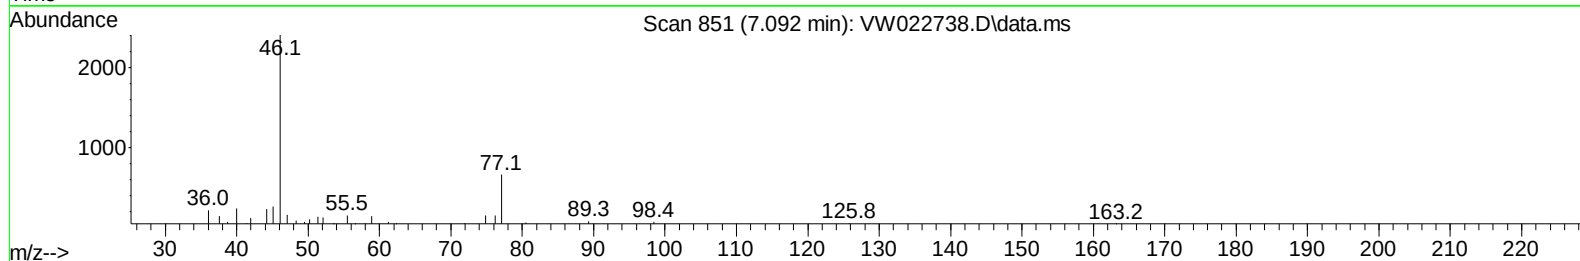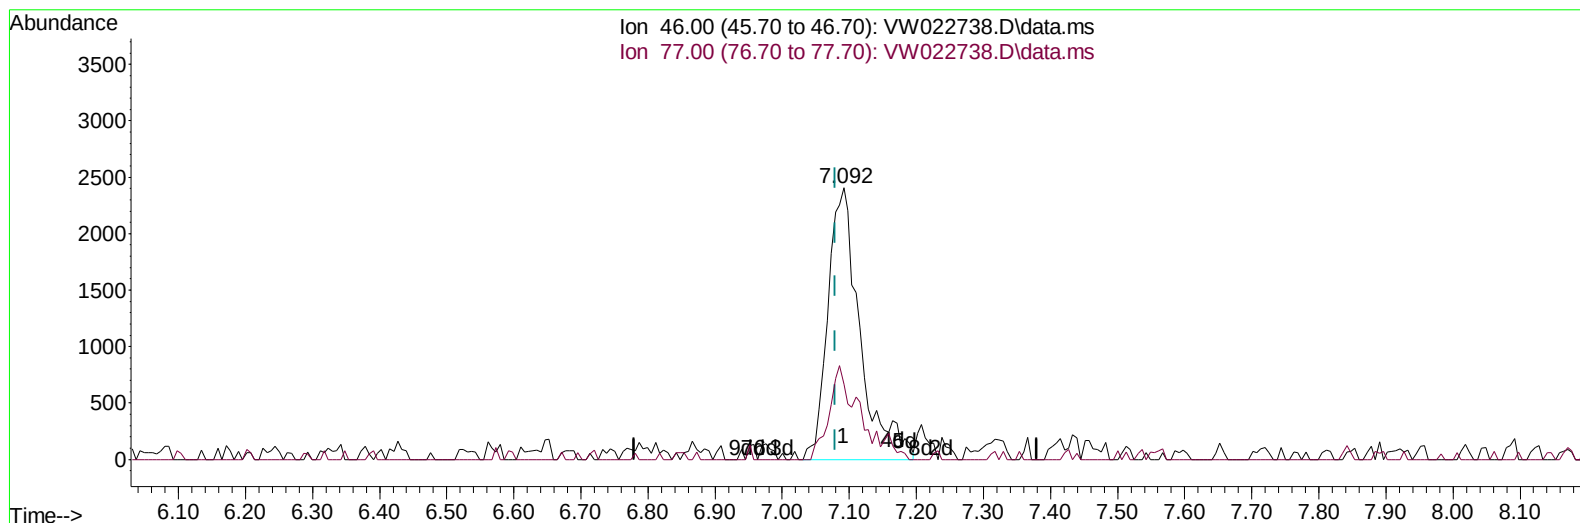

TIC: VW022738.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.012) 35.13 ug/L m

response 7998

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	20.47
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022738.D
 Acq On : 02 May 2022 14:39
 Operator : SY/VA
 Sample : N2603-15RE
 Misc : 6.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW495RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 03 01:43:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	58372	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	46338	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	14297	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	30703	25.637	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 102.560%			
7) Chloroethane-d5	2.885	69	30031	38.544	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 154.160%#			
11) 1,1-Dichloroethene-d2	4.019	63	32235	20.831	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 83.320%			
21) 2-Butanone-d5	7.092	46	7998m	35.125	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery = 70.260%			
24) Chloroform-d	7.646	84	41739	24.406	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 97.640%			
26) 1,2-Dichloroethane-d4	8.311	65	24558	26.182	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 104.720%			
32) Benzene-d6	8.280	84	84544	31.654	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 126.600%			
36) 1,2-Dichloropropane-d6	9.274	67	23823	31.753	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 127.000%#			
41) Toluene-d8	10.323	98	71436	27.687	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 110.760%			
43) trans-1,3-Dichloroprop...	10.579	79	7659	22.171	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 88.680%			
47) 2-Hexanone-d5	10.926	63	3776	26.364	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 52.720%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	17846	25.520	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 102.080%			
66) 1,2-Dichlorobenzene-d4	13.853	152	12918	25.848	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 103.400%			

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022738.D
Acq On : 02 May 2022 14:39
Operator : SY/VA
Sample : N2603-15RE
Misc : 6.94g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW495RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 03 01:43:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

