




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022747.D
 Acq On : 02 May 2022 18:16
 Operator : SY/VA
 Sample : N2639-06
 Misc : 5.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL15

Manual IntegrationsAPPROVED

Quant Time: May 03 01:44:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

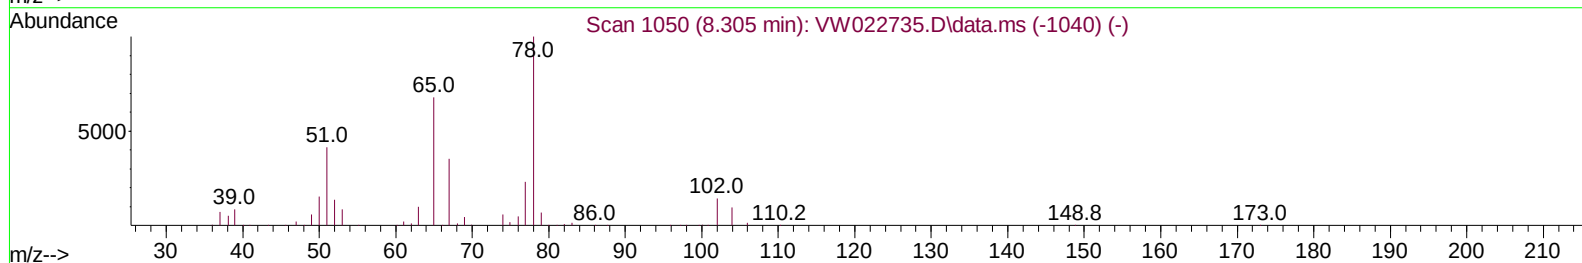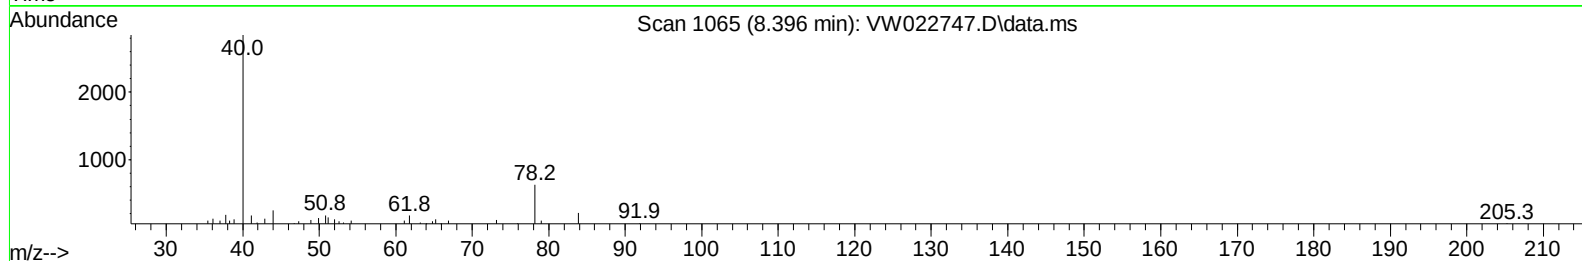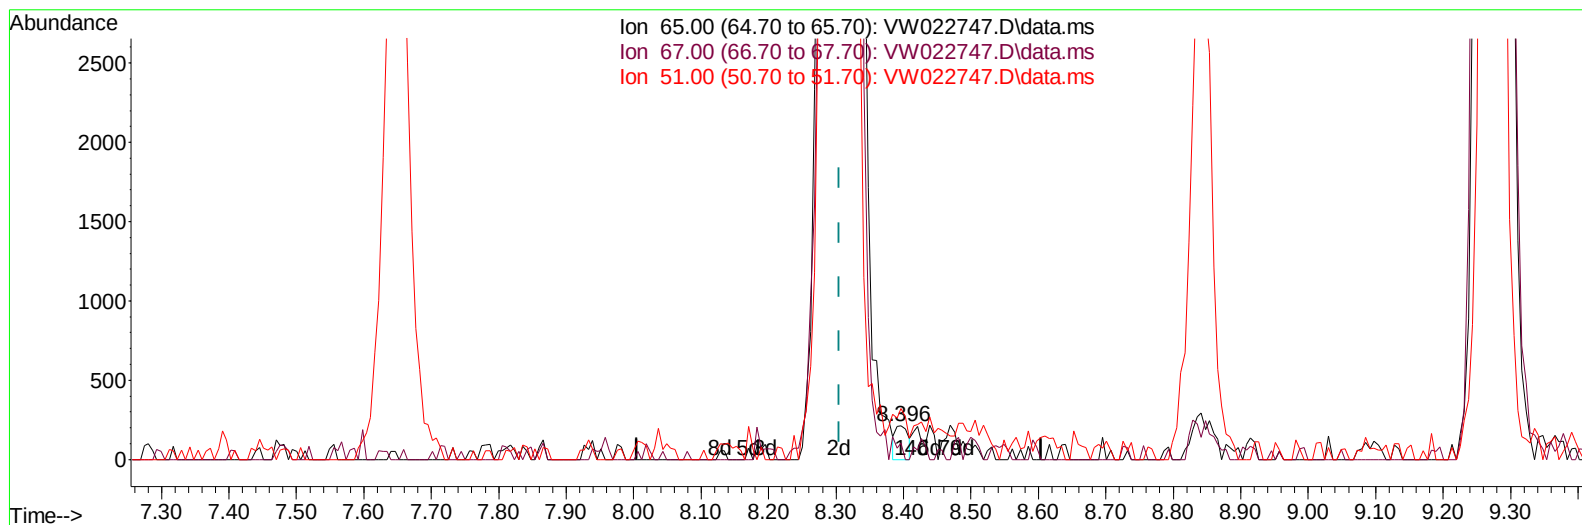

TIC: VW022747.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.396min (+ 0.092) 0.05 ug/L

response 273

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	42.49
51.00	92.30	91.58
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022747.D
 Acq On : 02 May 2022 18:16
 Operator : SY/VA
 Sample : N2639-06
 Misc : 5.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL15

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 03 01:44:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

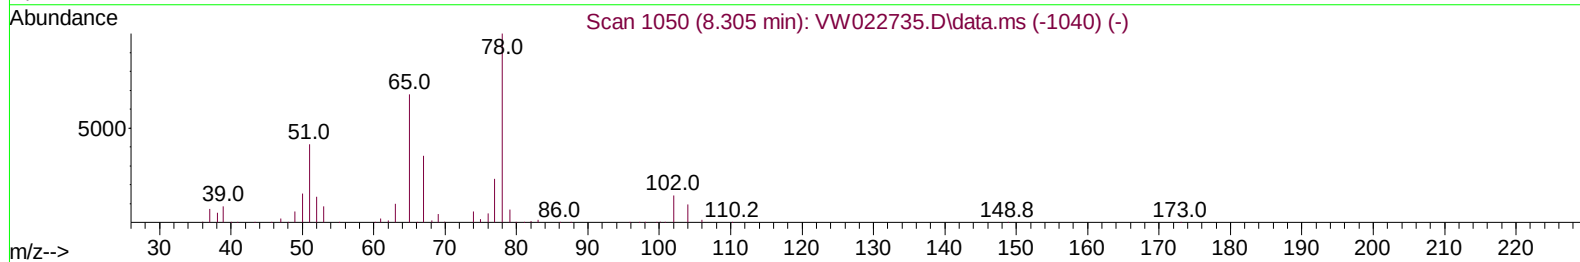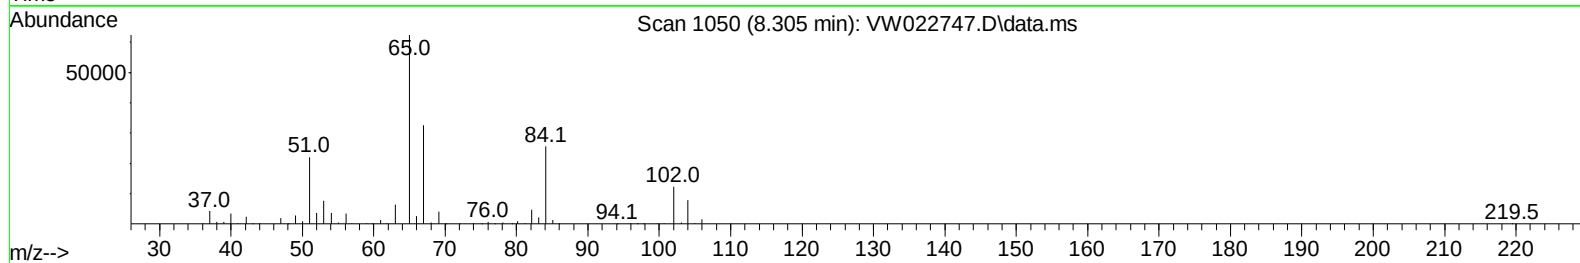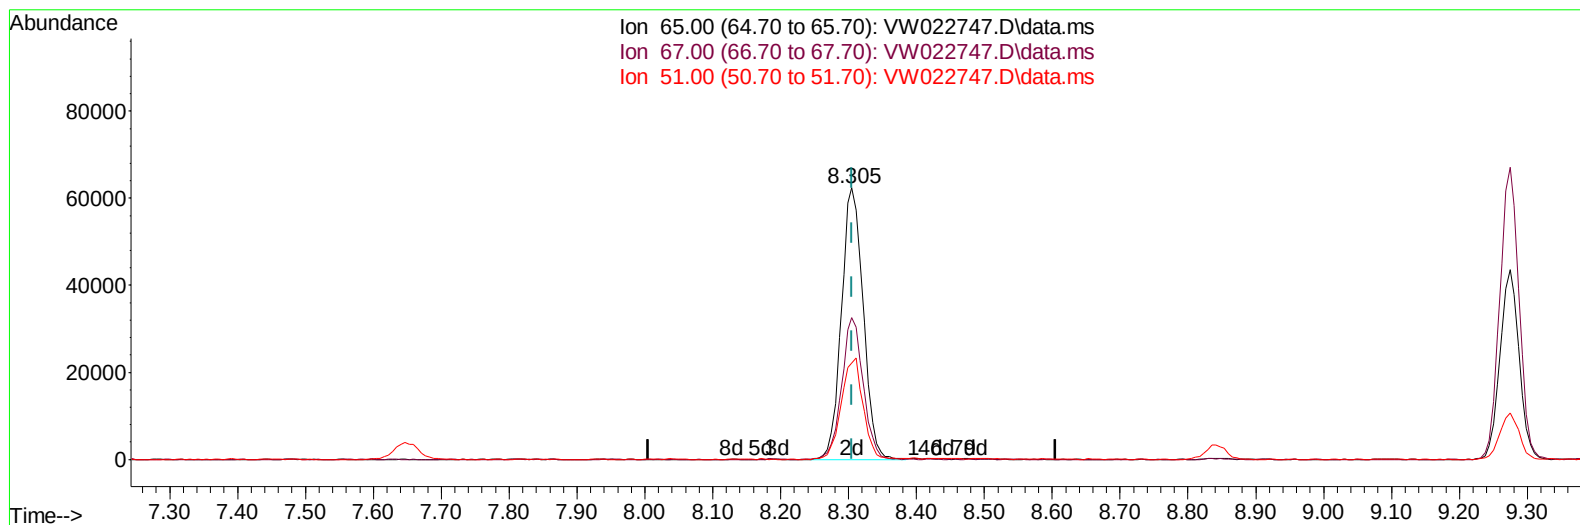

TIC: VW022747.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 24.84 ug/L m

response 139756

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.08#
51.00	92.30	0.18#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022747.D
 Acq On : 02 May 2022 18:16
 Operator : SY/VA
 Sample : N2639-06
 Misc : 5.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL15

Manual IntegrationsAPPROVED

Quant Time: May 03 01:44:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		350143	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		336170	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		159887	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		160814	22.386	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	89.560%	
7) Chloroethane-d5	2.885	69		102445	21.920	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	87.680%	
11) 1,1-Dichloroethene-d2	4.019	63		153538	16.541	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	66.160%	
21) 2-Butanone-d5	7.080	46		65259	47.779	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	95.560%	
24) Chloroform-d	7.647	84		233559	22.768	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	91.080%	
26) 1,2-Dichloroethane-d4	8.305	65		139756m	24.840	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	99.360%	
32) Benzene-d6	8.275	84		467871	24.146	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	96.600%	
36) 1,2-Dichloropropane-d6	9.274	67		132070	24.264	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	97.040%	
41) Toluene-d8	10.323	98		437190	23.357	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	93.440%	
43) trans-1,3-Dichloroprop...	10.579	79		55987	22.340	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	89.360%	
47) 2-Hexanone-d5	10.920	63		53108	51.112	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	102.220%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		122100	24.068	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	96.280%	
66) 1,2-Dichlorobenzene-d4	13.853	152		135454	24.235	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	96.960%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022747.D
Acq On : 02 May 2022 18:16
Operator : SY/VA
Sample : N2639-06
Misc : 5.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL15

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 03 01:44:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

