




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022752.D
Acq On : 02 May 2022 20:16
Operator : SY/VA
Sample : N2639-05
Misc : 5.65g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL14

Manual IntegrationsAPPROVED

Quant Time: May 03 01:45:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

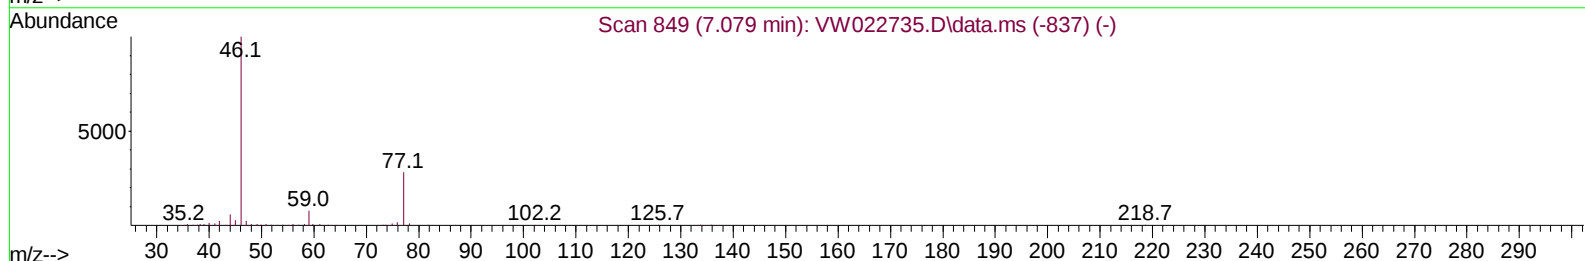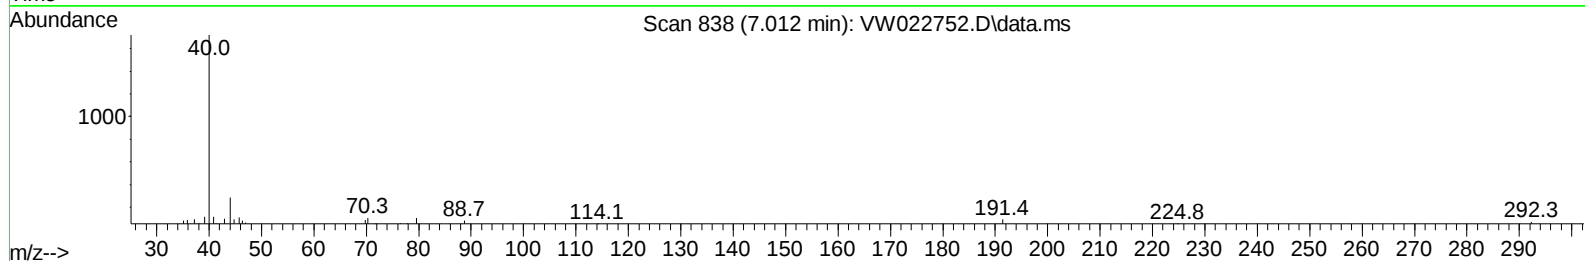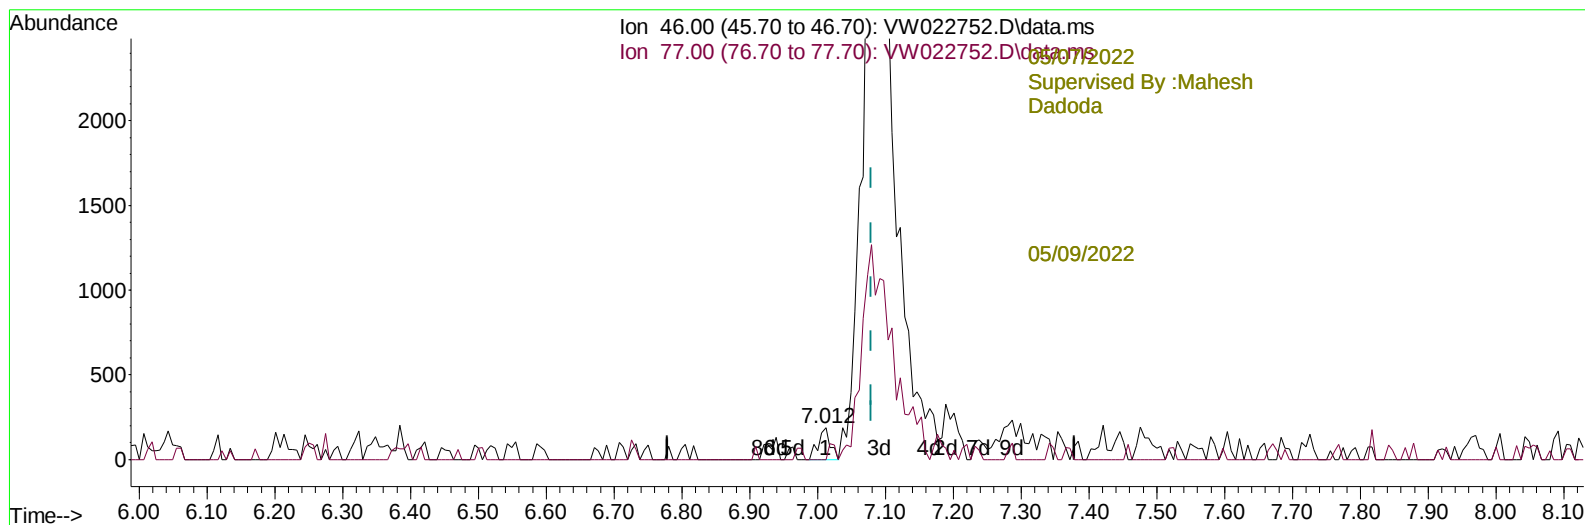

TIC: VW022752.D\data.ms

(21) 2-Butanone-d5 (S)

7.012min (-0.067) 0.78 ug/L

response 228

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	28.51
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022752.D
Acq On : 02 May 2022 20:16
Operator : SY/VA
Sample : N2639-05
Misc : 5.65g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL14

Manual IntegrationsAPPROVED

Quant Time: May 03 01:45:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

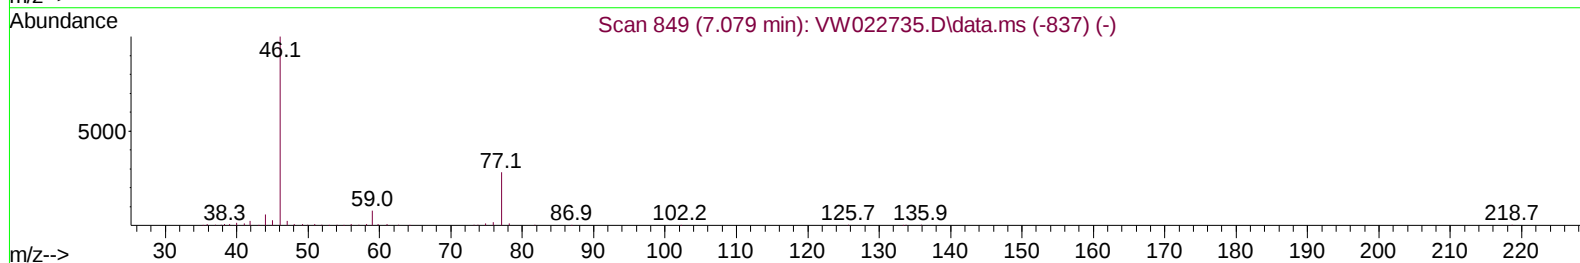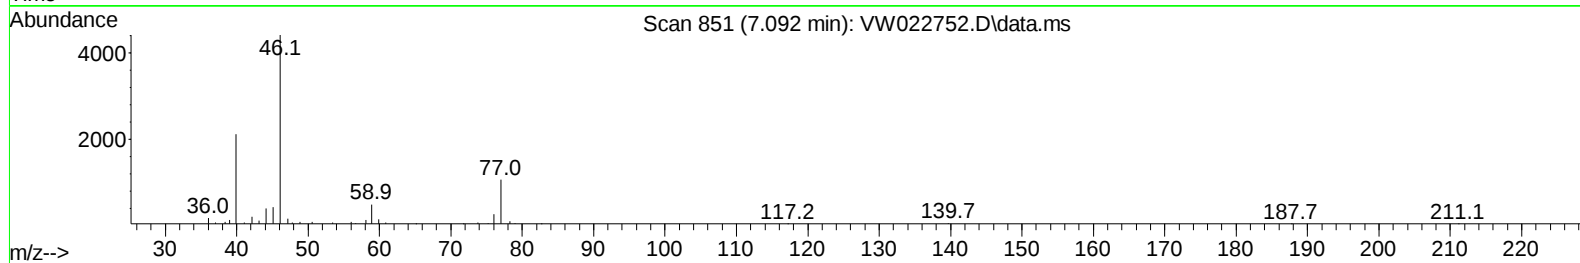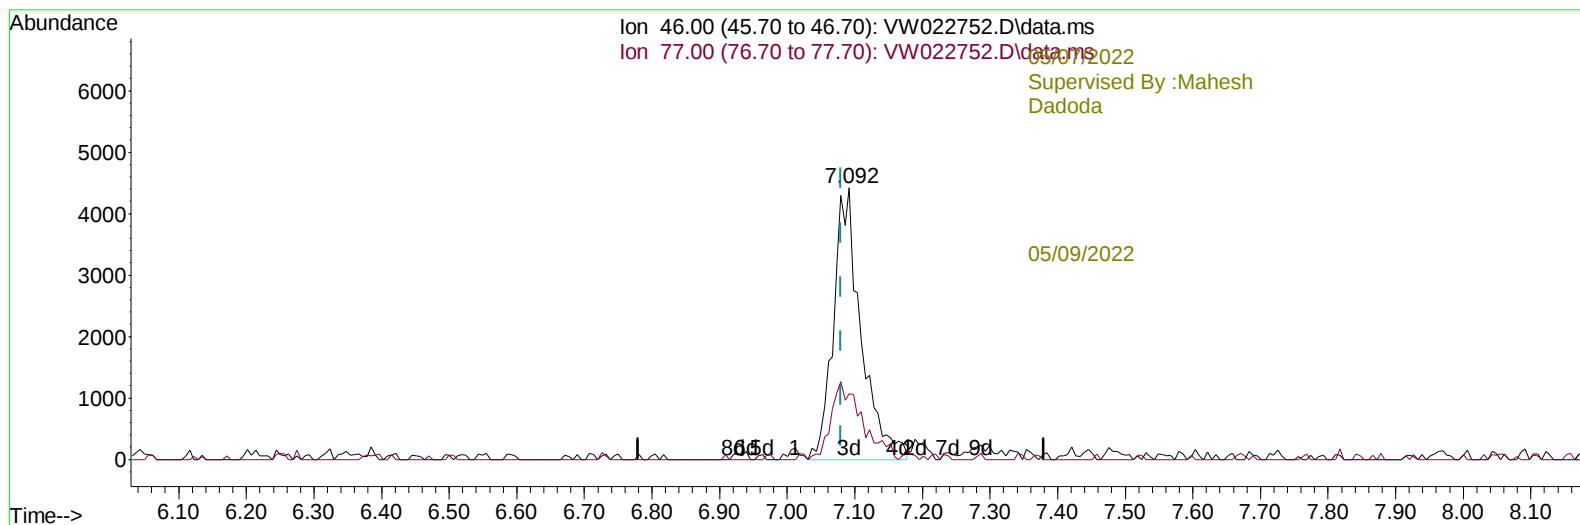

TIC: VW022752.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.012) 42.87 ug/L m

response 12543

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.52#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022752.D
 Acq On : 02 May 2022 20:16
 Operator : SY/VA
 Sample : N2639-05
 Misc : 5.65g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL14

Manual IntegrationsAPPROVED

Quant Time: May 03 01:45:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----05/07/2022							
Supervised By :Mahesh							
Dadoda							
Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		75011	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117		58758	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		15164	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		45225	29.387	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150		Recovery	=	117.560%	
7) Chloroethane-d5	2.885	69		37312	37.267	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150		Recovery	=	149.080%	
11) 1,1-Dichloroethene-d2	4.013	63		43571	21.911	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110		Recovery	=	87.640%	
21) 2-Butanone-d5	7.092	46		12543m	42.867	ug/L	0.01
Spiked Amount	50.000	Range 20 - 135		Recovery	=	85.740%	
24) Chloroform-d	7.652	84		57025	25.948	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150		Recovery	=	103.800%	
26) 1,2-Dichloroethane-d4	8.305	65		33232	27.571	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130		Recovery	=	110.280%	
32) Benzene-d6	8.274	84		107353	31.698	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135		Recovery	=	126.800%	
36) 1,2-Dichloropropane-d6	9.274	67		31591	33.206	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120		Recovery	=	132.840%#	
41) Toluene-d8	10.323	98		87157	26.640	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130		Recovery	=	106.560%	
43) trans-1,3-Dichloroprop...	10.579	79		9657	22.046	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135		Recovery	=	88.200%	
47) 2-Hexanone-d5	10.920	63		7419	40.851	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135		Recovery	=	81.700%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		23553	26.562	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120		Recovery	=	106.240%	
66) 1,2-Dichlorobenzene-d4	13.853	152		13786	26.007	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120		Recovery	=	104.040%	
Target Compounds							
						Qvalue	
13) Acetone	4.135	43		2751	12.558	ug/L	83
46) Tetrachloroethene	10.859	164		1058	1.479	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022752.D
Acq On : 02 May 2022 20:16
Operator : SY/VA
Sample : N2639-05
Misc : 5.65g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL14

Manual IntegrationsAPPROVED

Quant Time: May 03 01:45:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

