




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022756.D
 Acq On : 02 May 2022 21:53
 Operator : SY/VA
 Sample : N2638-09
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL04

Manual IntegrationsAPPROVED

Quant Time: May 03 01:46:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/17/2022
 Supervised By :Semsettin Yesilyurt 05/17/2022

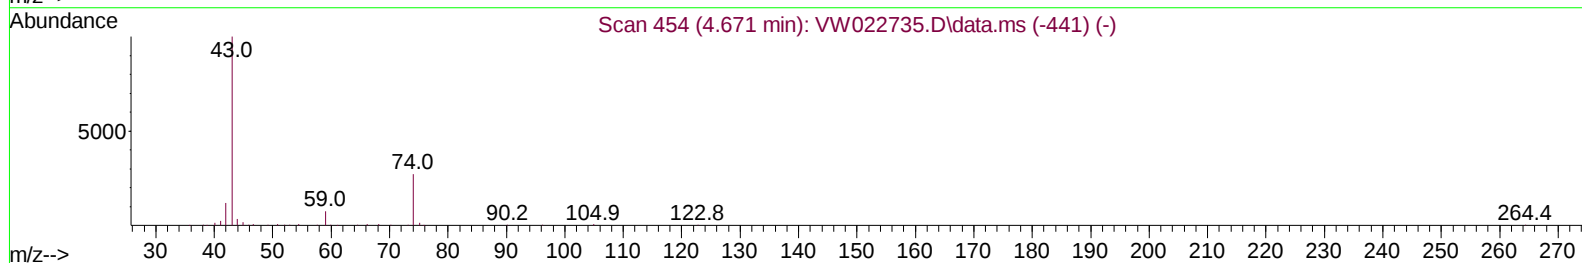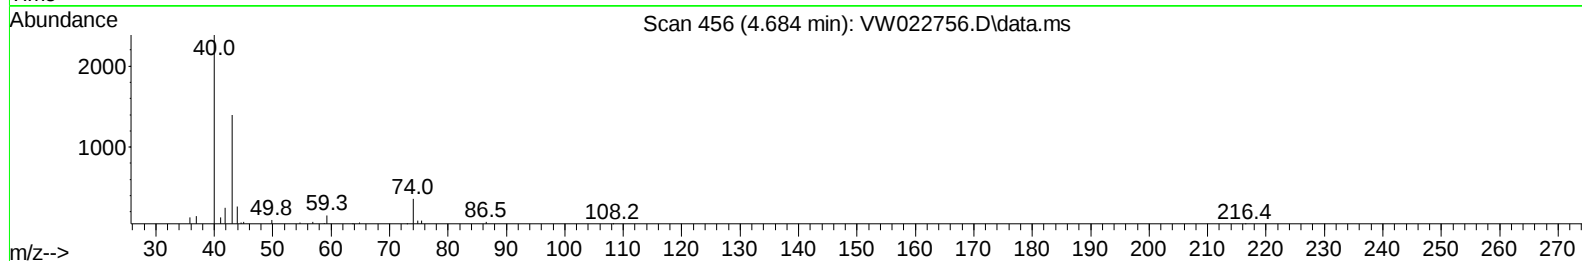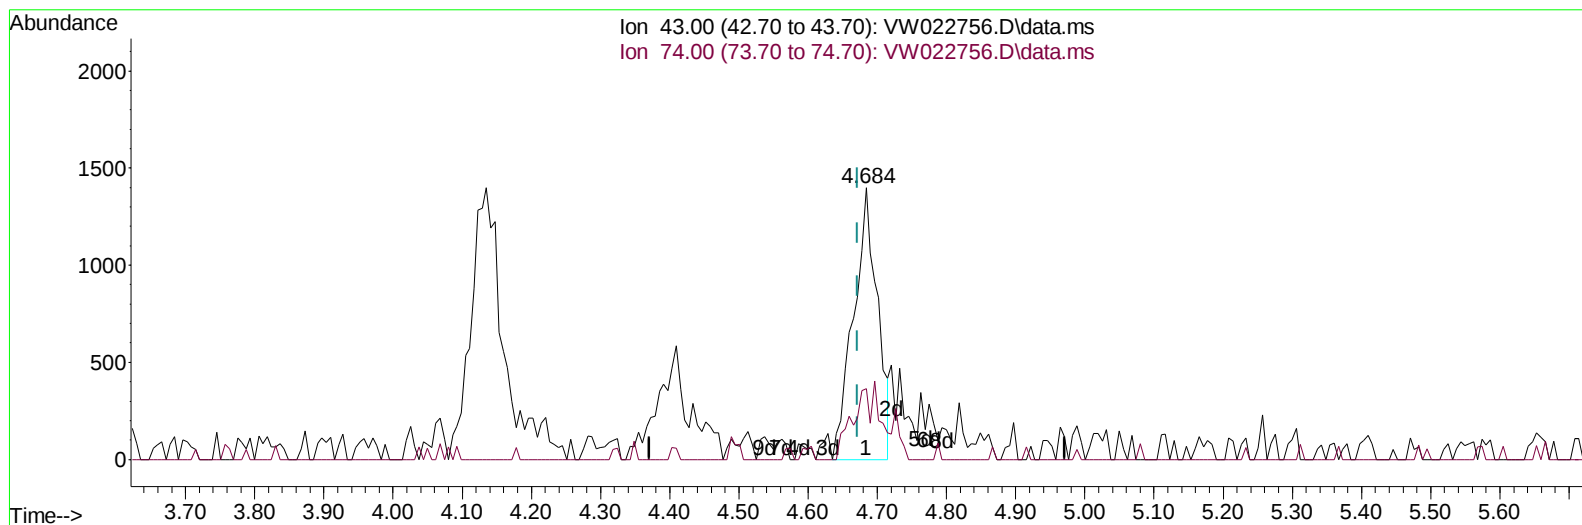

TIC: VW022756.D\data.ms

(15) Methyl Acetate (T)

4.684min (+ 0.013) 11.63 ug/L

response 3356

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.40	12.19#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022756.D
 Acq On : 02 May 2022 21:53
 Operator : SY/VA
 Sample : N2638-09
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL04

Manual IntegrationsAPPROVED

Quant Time: May 03 01:46:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/17/2022
 Supervised By :Semsettin Yesilyurt 05/17/2022

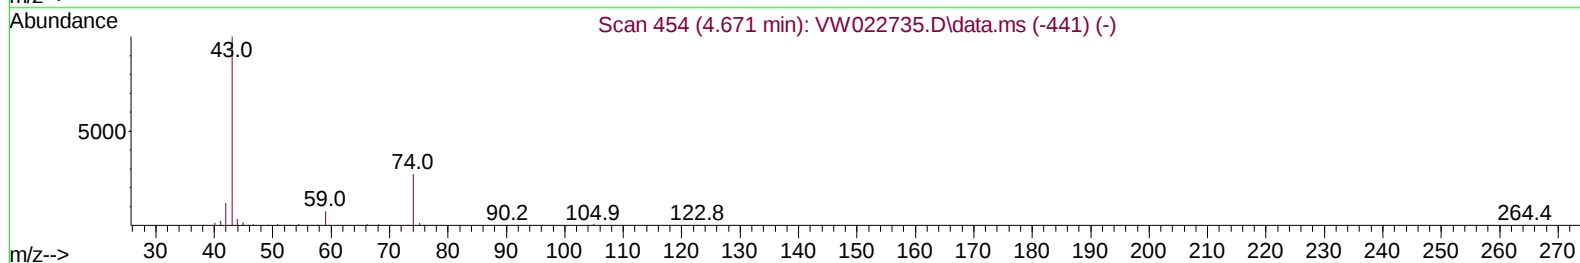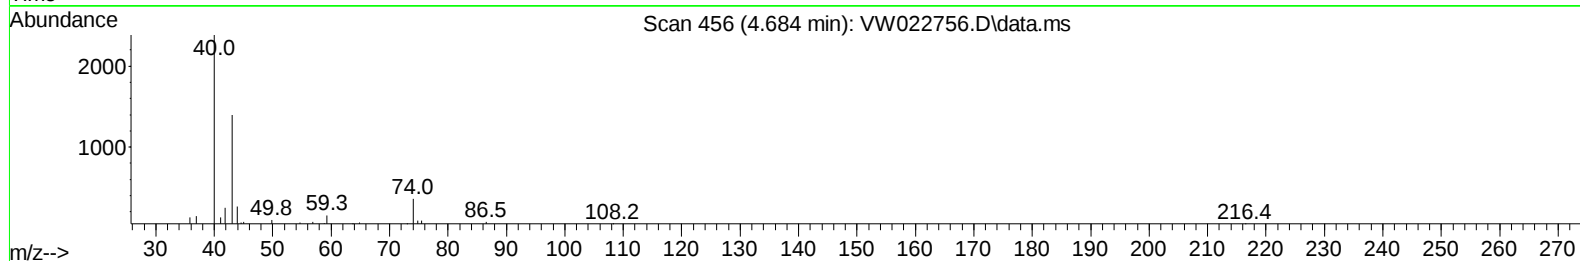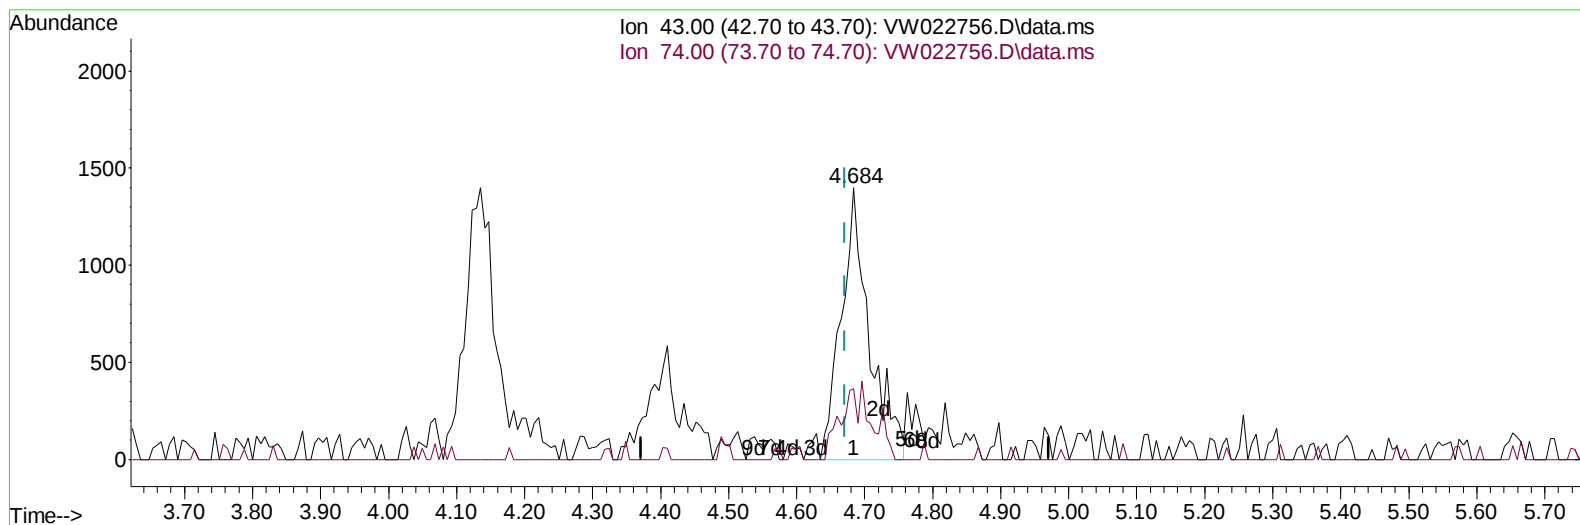

TIC: VW022756.D\data.ms

(15) Methyl Acetate (T)

4.684min (+ 0.013) 14.01 ug/L m

response 4041

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.40	10.12#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022756.D
 Acq On : 02 May 2022 21:53
 Operator : SY/VA
 Sample : N2638-09
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL04

Manual IntegrationsAPPROVED

Quant Time: May 03 01:46:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/17/2022
 Supervised By :Semsettin Yesilyurt 05/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	49167	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	53134	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	24841	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	19000	18.836	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.360%	
7) Chloroethane-d5	2.879	69	18415	28.060	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	112.240%	
11) 1,1-Dichloroethene-d2	4.019	63	20436	15.679	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.720%	
21) 2-Butanone-d5	7.086	46	15729	82.011	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	164.020%#	
24) Chloroform-d	7.653	84	33243	23.078	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.320%	
26) 1,2-Dichloroethane-d4	8.305	65	24626	31.170	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	124.680%	
32) Benzene-d6	8.281	84	62608	20.443	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	81.760%	
36) 1,2-Dichloropropane-d6	9.274	67	21066	24.487	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	97.960%	
41) Toluene-d8	10.323	98	56319	19.036	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	76.160%	
43) trans-1,3-Dichloroprop...	10.573	79	8803	22.223	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	88.880%	
47) 2-Hexanone-d5	10.921	63	10617	64.648	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	129.300%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	27108	33.807	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	135.240%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	21817	25.124	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.480%	
Target Compounds						
					Qvalue	
13) Acetone	4.135	43	4046	28.177	ug/L	86
15) Methyl Acetate	4.684	43	4041m	14.008	ug/L	
46) Tetrachloroethene	10.860	164	817	1.263	ug/L #	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022756.D
Acq On : 02 May 2022 21:53
Operator : SY/VA
Sample : N2638-09
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL04

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/17/2022
Supervised By :Semsettin Yesilyurt 05/17/2022

Quant Time: May 03 01:46:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

