

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022741.D
 Acq On : 02 May 2022 15:52
 Operator : SY/VA
 Sample : N2623-01
 Misc : 5.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFJ1

Quant Time: May 03 01:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	350288	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	302125	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	101702	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	175931	24.480	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.920%
7) Chloroethane-d5	2.885	69	117081	25.041	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.160%
11) 1,1-Dichloroethene-d2	4.019	63	171695	18.490	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.960%
21) 2-Butanone-d5	7.080	46	65387	47.853	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.700%
24) Chloroform-d	7.653	84	249667	24.328	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.320%
26) 1,2-Dichloroethane-d4	8.305	65	142963	25.399	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	8.275	84	497618	28.575	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	114.320%
36) 1,2-Dichloropropane-d6	9.274	67	141720	28.971	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.880%
41) Toluene-d8	10.323	98	444921	26.448	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.800%
43) trans-1,3-Dichloroprop...	10.579	79	56541	25.103	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.400%
47) 2-Hexanone-d5	10.927	63	48378	51.806	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.620%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	102866	22.561	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	90974	25.589	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.360%
Target Compounds					Qvalue	
13) Acetone	4.123	43	16911	16.530	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022741.D
Acq On : 02 May 2022 15:52
Operator : SY/VA
Sample : N2623-01
Misc : 5.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFJ1

Quant Time: May 03 01:43:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

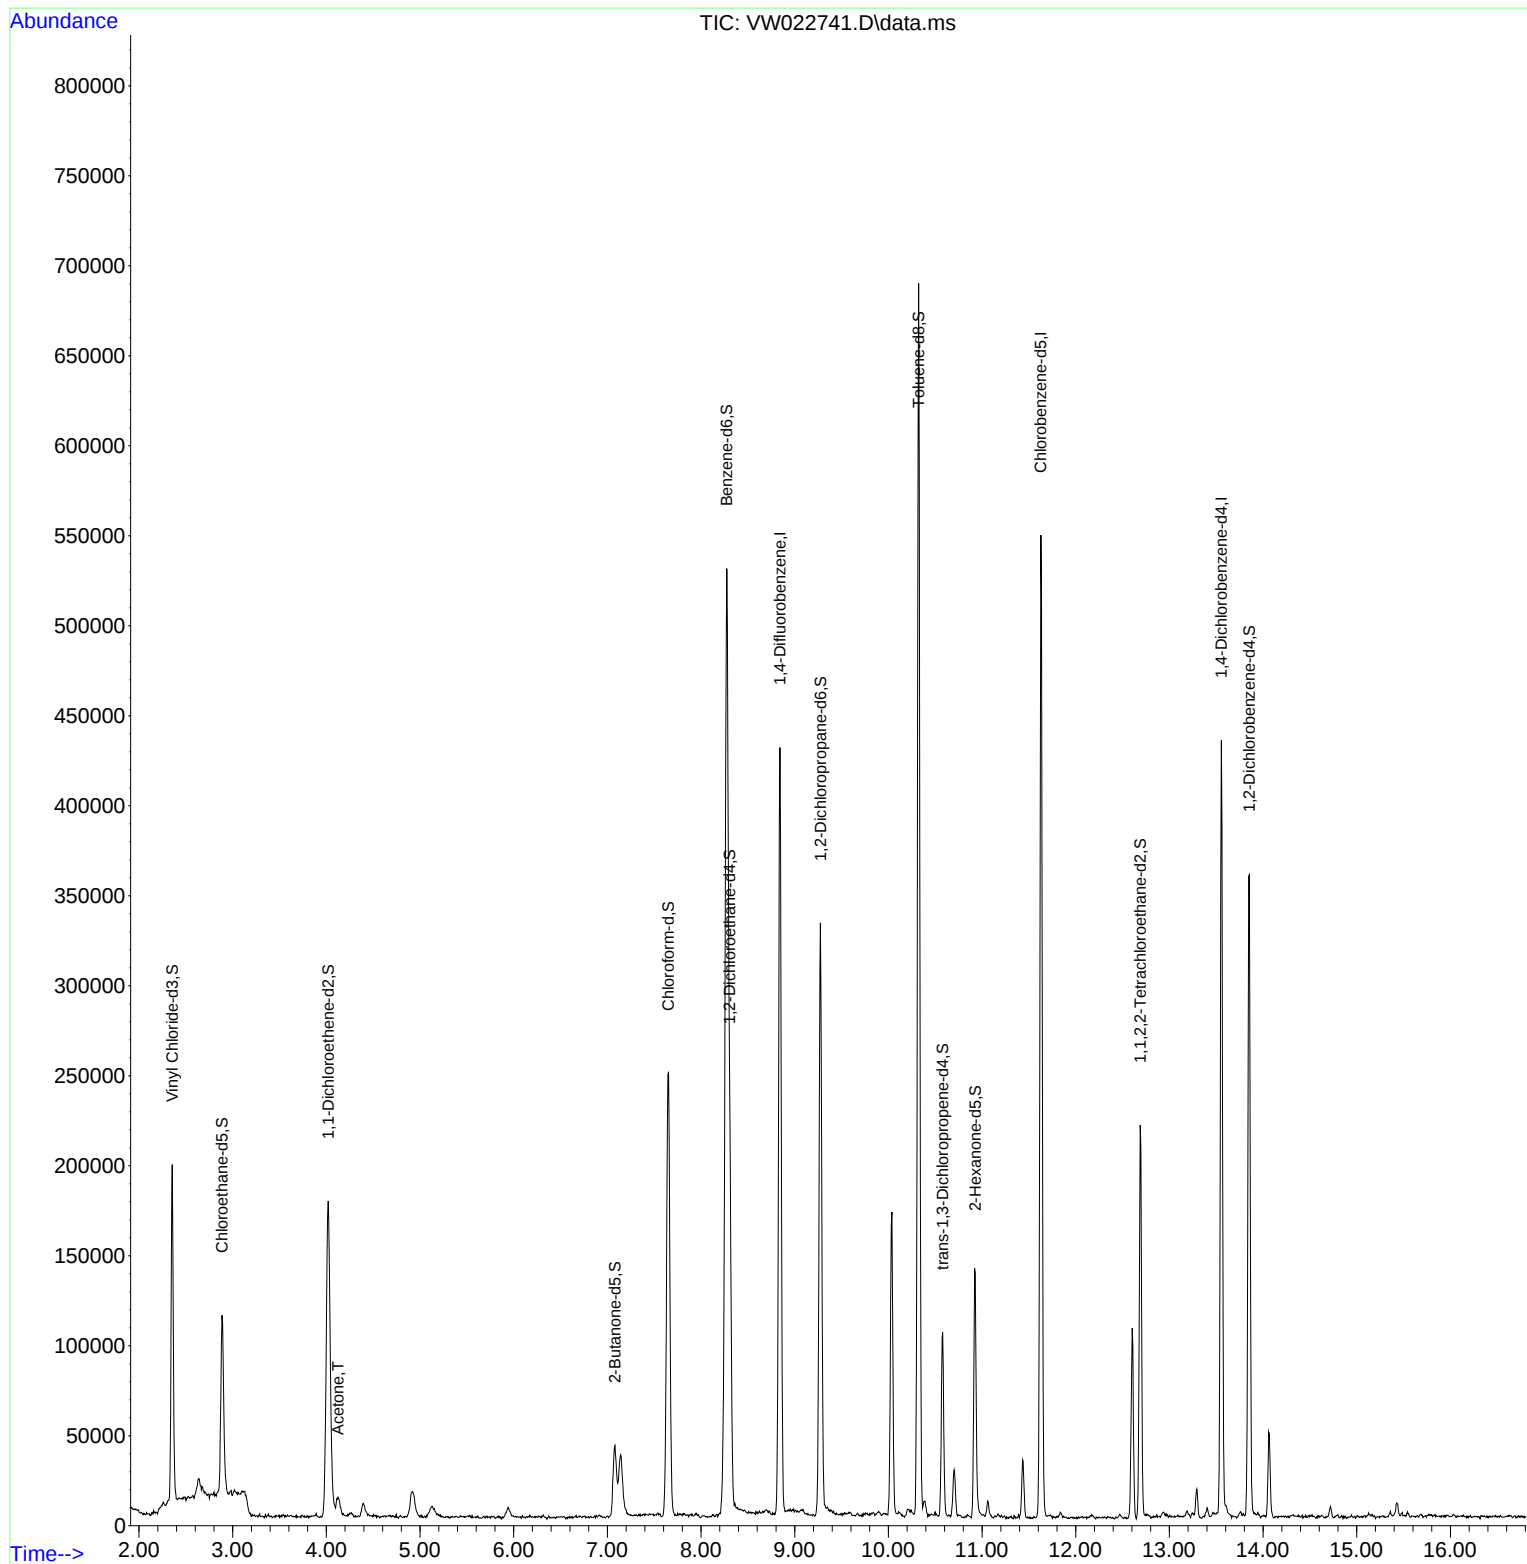

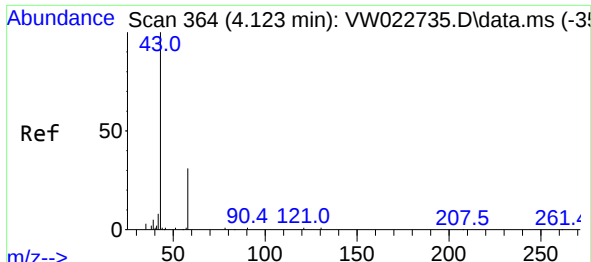

#13
 Acetone
 Concen: 16.530 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW022741.D
 Acq: 02 May 2022 15:52

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFJ1

Tgt Ion: 43 Resp: 16911
 Ion Ratio Lower Upper
 43 100
 58 29.5 0.0 64.0

