

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
 Data File : VW022750.D
 Acq On : 02 May 2022 19:28
 Operator : SY/VA
 Sample : N2639-16
 Misc : 5.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL24

Manual Integrations
 APPROVED

Reviewed By : Semsettin
 Yesilyurt

05/03/2022
 Supervised By : Mahesh
 Dadoda

05/04/2022

Quant Time: May 03 01:45:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 03 01:41:22 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)	Qvalue

Internal Standards								
1) 1,4-Difluorobenzene		8.842	114	329566	25.000	ug/L	0.00	
28) Chlorobenzene-d5		11.628	117	326726	25.000	ug/L	0.00	
58) 1,4-Dichlorobenzene-d4		13.560	152	156237	25.000	ug/L	0.00	
System Monitoring Compounds								
4) Vinyl Chloride-d3		2.355	65	170707	25.247	ug/L	0.00	
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.000%		
7) Chloroethane-d5		2.885	69	113063	25.702	ug/L	0.00	
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.800%		
11) 1,1-Dichloroethene-d2		4.019	63	159317	18.235	ug/L	0.00	
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.960%		
21) 2-Butanone-d5		7.080	46	64540	50.203	ug/L	0.00	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.400%		
24) Chloroform-d		7.647	84	247950	25.680	ug/L	0.00	
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.720%		
26) 1,2-Dichloroethane-d4		8.305	65	142780m	26.962	ug/L	0.00	
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.840%		
32) Benzene-d6		8.275	84	498450	26.468	ug/L	0.00	
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.880%		
36) 1,2-Dichloropropane-d6		9.268	67	144789	27.370	ug/L	0.00	
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.480%		
41) Toluene-d8		10.323	98	469163	25.789	ug/L	0.00	
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.160%		
43) trans-1,3-Dichloroprop...		10.579	79	59357	24.369	ug/L	0.00	
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.480%		
47) 2-Hexanone-d5		10.920	63	51110	50.611	ug/L	0.00	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.220%		
56) 1,1,2,2-Tetrachloroeth...		12.688	84	122720	24.889	ug/L	0.00	
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.560%		
66) 1,2-Dichlorobenzene-d4		13.847	152	147525	27.012	ug/L	0.00	
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.040%		
Target Compounds								
46) Tetrachloroethene		10.859	164	3395	0.853	ug/L		96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050222\
Data File : VW022750.D
Acq On : 02 May 2022 19:28
Operator : SY/VA
Sample : N2639-16
Misc : 5.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL24


Manual Integrations
APPROVED


Reviewed By : Semsettin
Yesilyurt

05/03/2022
Supervised By : Mahesh
Dadoda

05/04/2022


Quant Time: May 03 01:45:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 03 01:41:22 2022
Response via : Initial Calibration

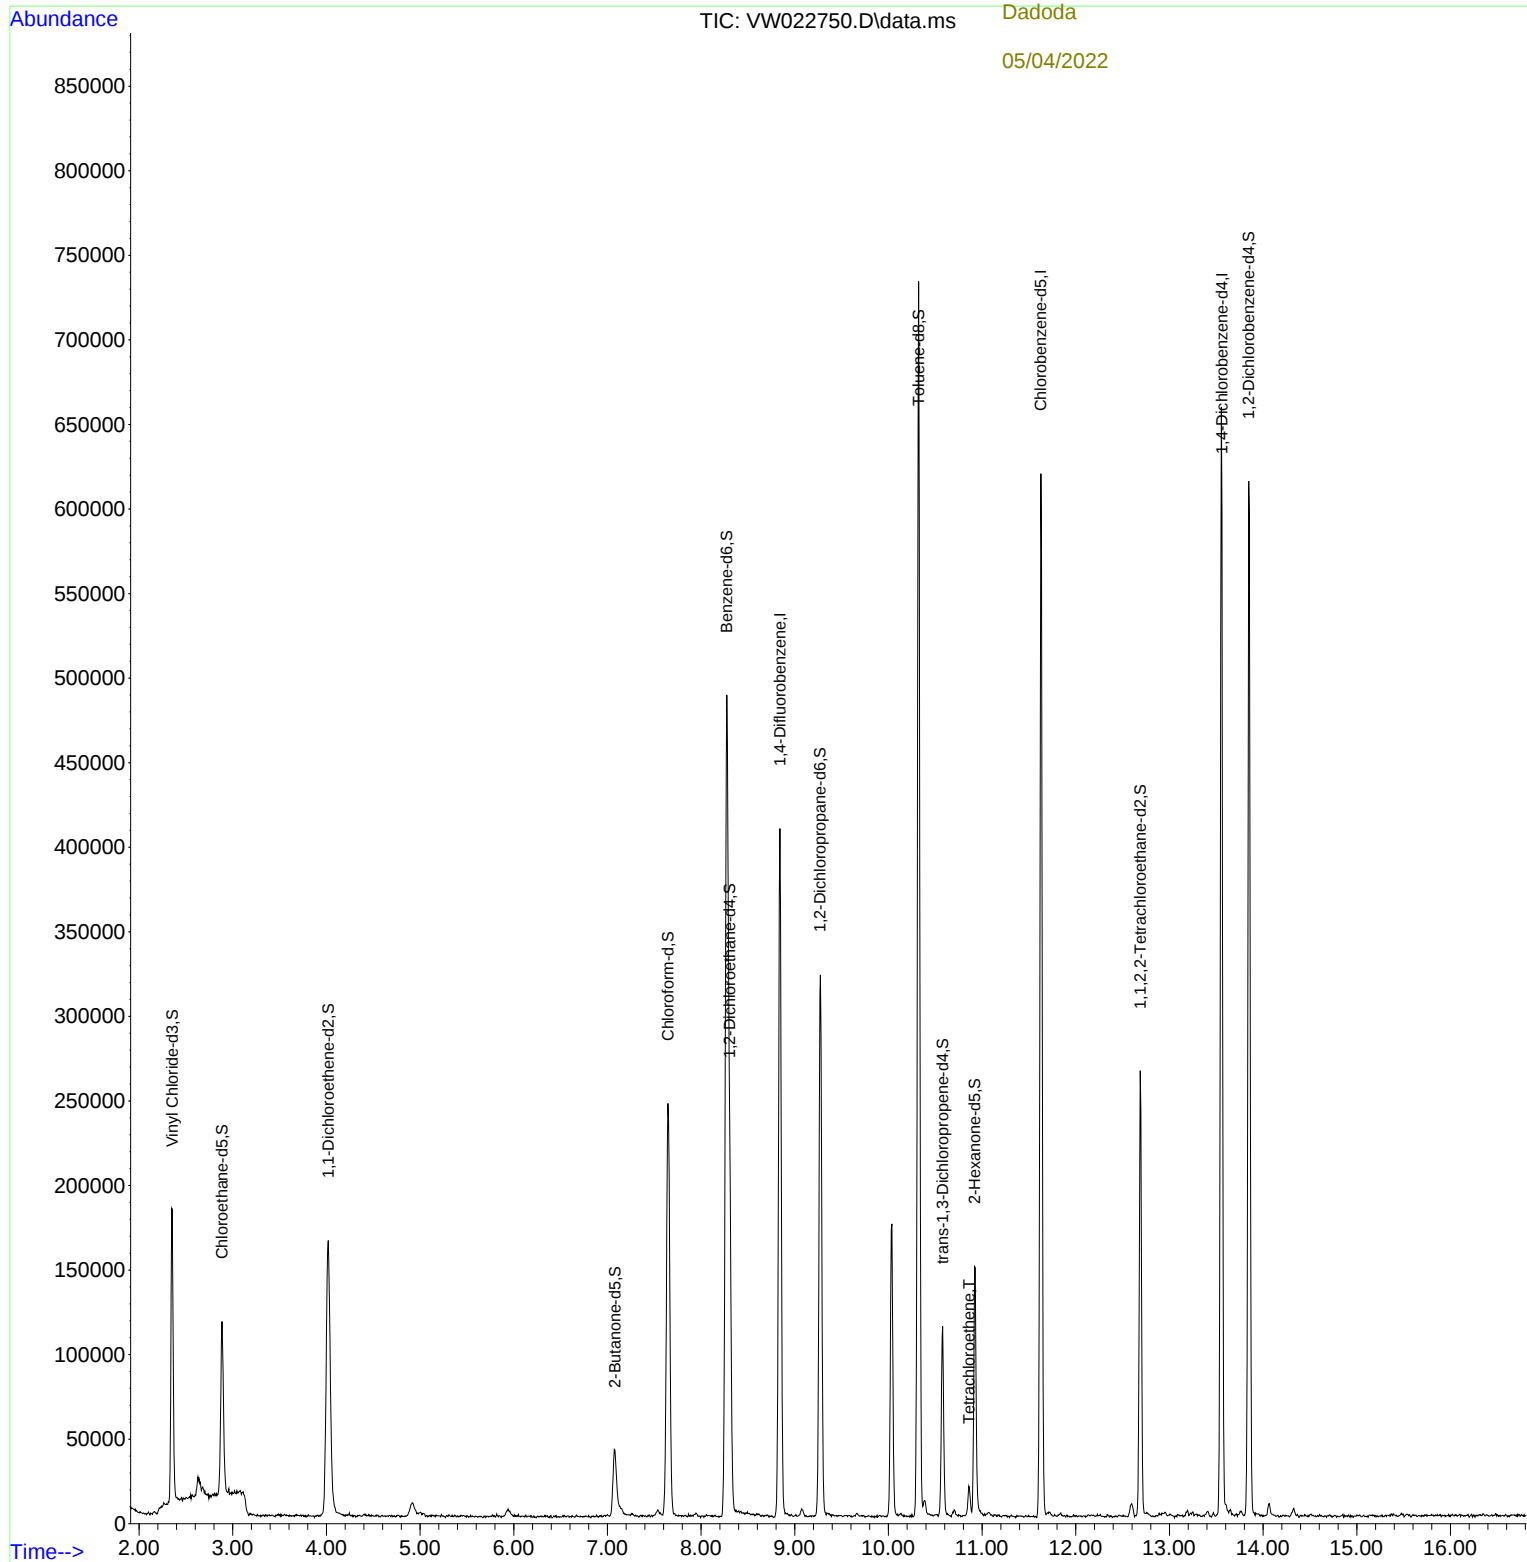

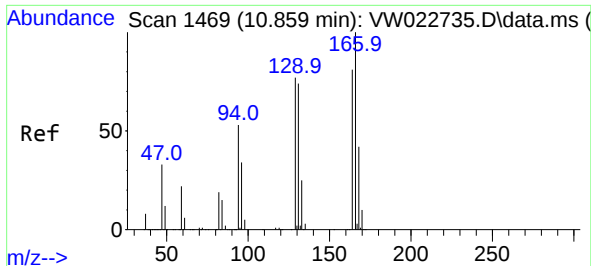

#46
Tetrachloroethene
Concen: 0.853 ug/L
RT: 10.859 min Scan# 1469
Delta R.T. 0.000 min
Lab File: VW022750.D
Acq: 02 May 2022 19:28

Instrument :
MSVOA_W
ClientSampleId :
EXL24

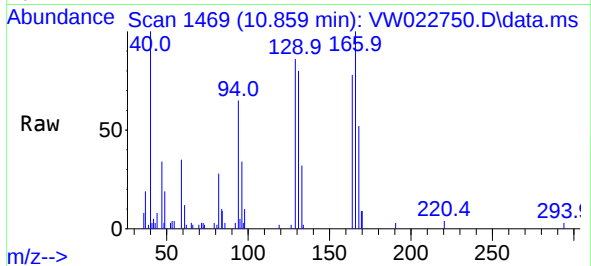

Tgt Ion	Ratio	Lower	Upper
164	100		
129	109.9	76.9	142.7
131	103.0	75.1	139.5
166	127.4	96.0	178.2

Manual Integrations
APPROVED

Reviewed By :Semsettin
Yesilyurt

05/03/2022
Supervised By :Mahesh
Dadoda

05/04/2022

