

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050421\
Data File : VW018926.D
Acq On : 04 May 2021 18:20
Operator : SY/VA
Sample : M2272-08
Misc : 4.73G/10ML/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6C5

Manual Integrations
APPROVED

MMDadoda
5/6/2021 5:40:53 PM

Quant Time: May 05 00:08:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWL042921SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 05 00:05:43 2021
Response via : Initial Calibration

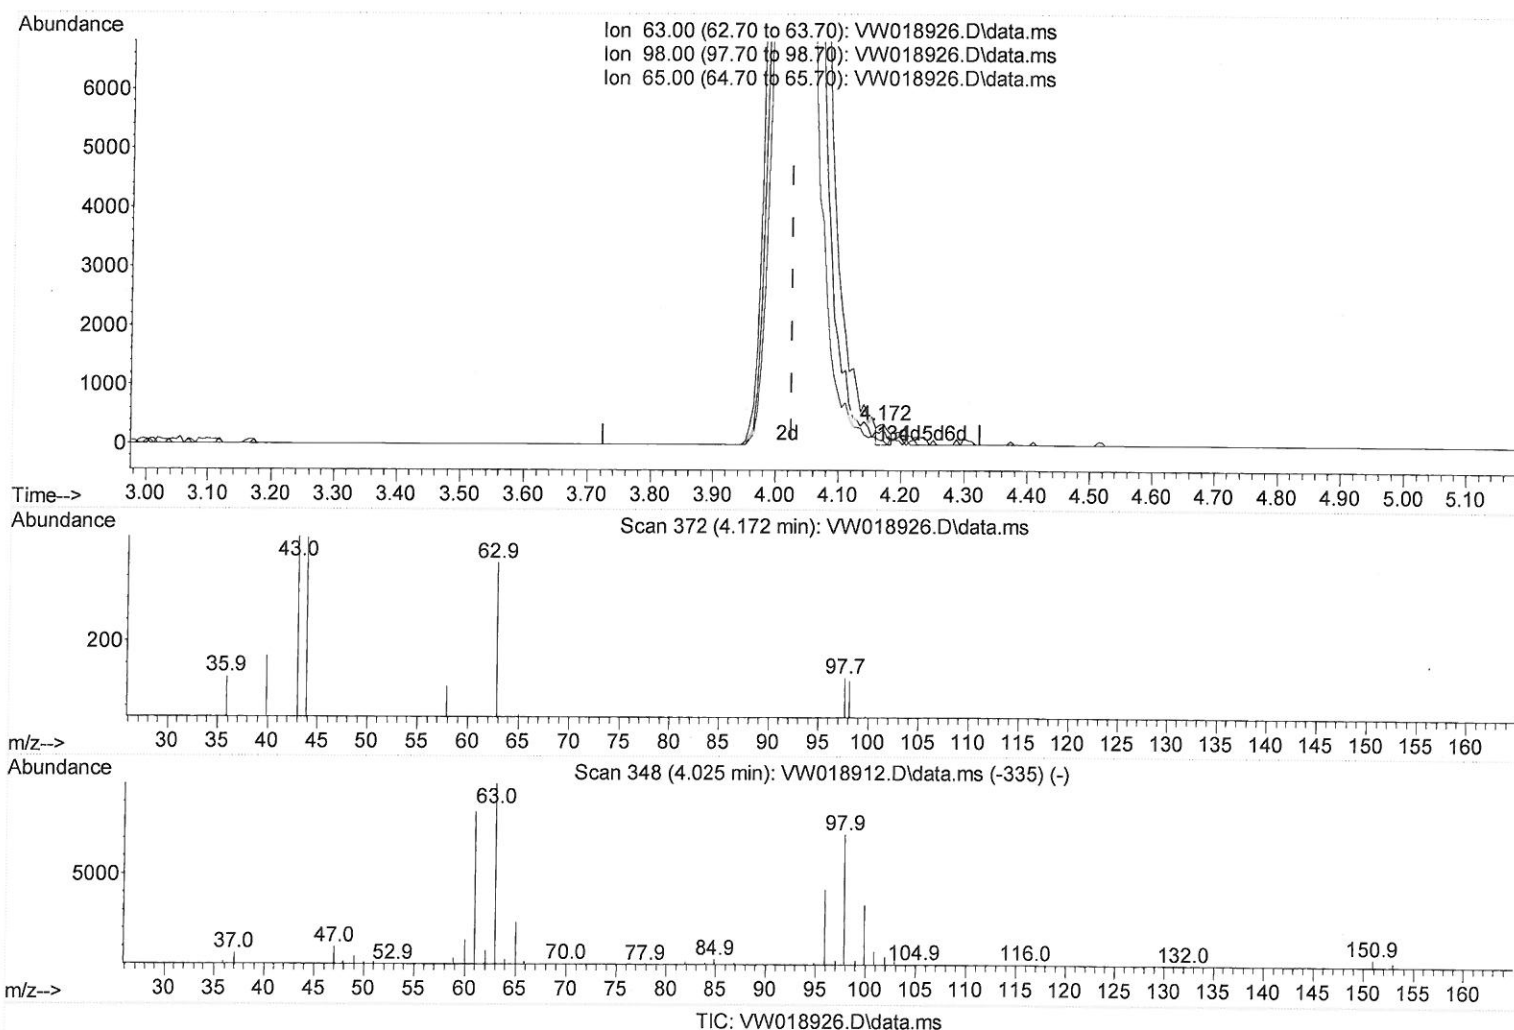

(11) 1,1-Dichloroethene-d2 (S)

4.172min (+ 0.146) 0.03 ug/L

response 404

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.20	77.48
65.00	23.70	24.01
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050421\
 Data File : VW018926.D
 Acq On : 04 May 2021 18:20
 Operator : SY/VA
 Sample : M2272-08
 Misc : 4.73G/10ML/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6C5

Manual Integrations
 APPROVED

MMDadoda
 5/6/2021 5:40:53 PM

Quant Time: May 05 00:08:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 05 00:05:43 2021
 Response via : Initial Calibration

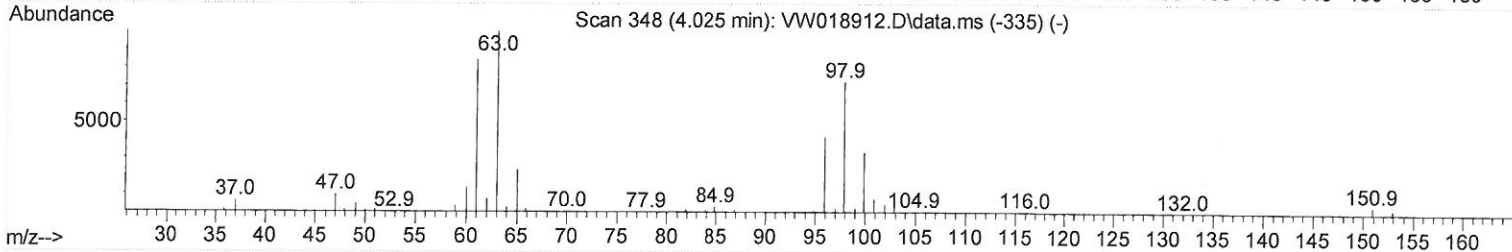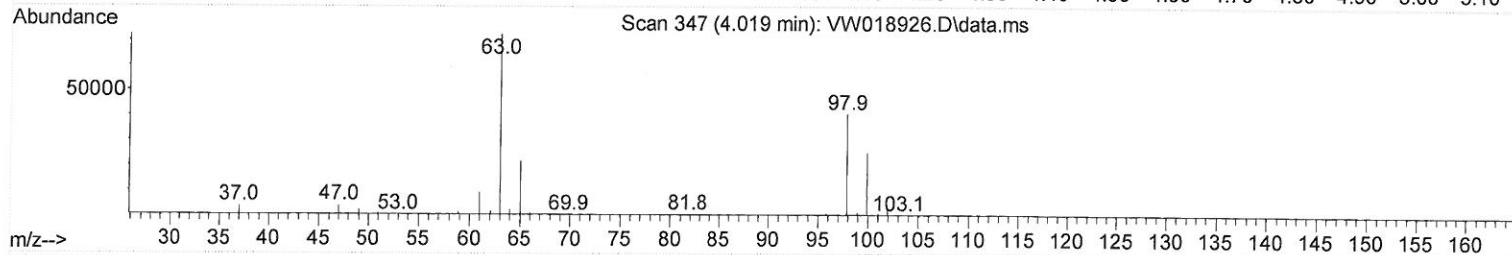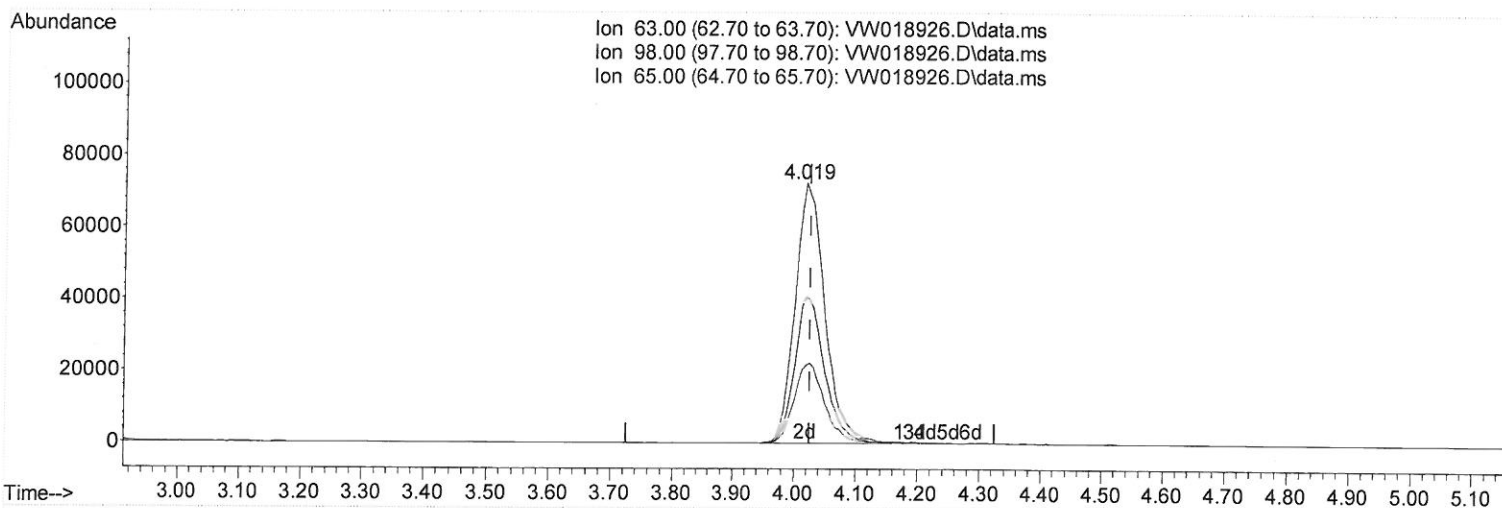

TIC: VW018926.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.006) 15.80 ug/L m

response 244480

Ion	Exp%	Act%
-----	------	------

63.00	100.00	100.00
-------	--------	--------

98.00	70.20	0.13#
-------	-------	-------

65.00	23.70	0.04#
-------	-------	-------

0.00	0.00	0.00
------	------	------

Handwritten signature: S. S. / 17/12/1 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050421\
 Data File : VW018926.D
 Acq On : 04 May 2021 18:20
 Operator : SY/VA
 Sample : M2272-08
 Misc : 4.73G/10ML/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6C5

Manual Integrations
 APPROVED

MMDadoda
 5/6/2021 5:40:53 PM

Quant Time: May 05 00:08:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 05 00:05:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	607288	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	542487	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	248117	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	157279	20.19	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	80.76%		
7) Chloroethane-d5	2.891	69	128577	21.30	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	85.20%		
11) 1,1-Dichloroethene-d2	4.019	63	244480m	15.80	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	63.20%		
21) 2-Butanone-d5	7.080	46	77043	37.97	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	75.94%		
24) Chloroform-d	7.653	84	360144	22.59	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	90.36%		
26) 1,2-Dichloroethane-d4	8.305	65	199074	22.36	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	89.44%		
32) Benzene-d6	8.275	84	713937	23.29	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	93.16%		
36) 1,2-Dichloropropane-d6	9.274	67	212082	23.32	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	93.28%		
41) Toluene-d8	10.323	98	655862	22.94	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	91.76%		
43) trans-1,3-Dichloroprop...	10.579	79	83415	20.19	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	80.76%		
47) 2-Hexanone-d5	10.927	63	66108	40.60	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	81.20%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	159138	20.65	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	82.60%		
66) 1,2-Dichlorobenzene-d4	13.853	152	199340	23.45	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	93.80%		
Target Compounds						
16) Methylene chloride	4.922	84	61704	6.15	ug/L	95
42) Toluene	10.390	91	11097	0.31	ug/L	99
46) Tetrachloroethene	10.866	164	13566	2.08	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

05/17/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050421\
Data File : VW018926.D
Acq On : 04 May 2021 18:20
Operator : SY/VA
Sample : M2272-08
Misc : 4.73G/10ML/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
EW6C5

Manual Integrations
APPROVED

MMDadoda
5/6/2021 5:40:53 PM

Quant Time: May 05 00:08:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 05 00:05:43 2021
Response via : Initial Calibration

