

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050423\
 Data File : VW025852.D
 Acq On : 04 May 2023 18:09
 Operator : SY/MD
 Sample : 02574-22RE
 Misc : 4.94g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCQ4

Quant Time: May 04 23:20:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 23:16:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	897782	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	811177	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	366026	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	274861	21.605	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.400%
7) Chloroethane-d5	2.899	69	211039	22.375	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.520%
11) 1,1-Dichloroethene-d2	4.021	65	130280	20.451	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.800%
21) 2-Butanone-d5	7.075	46	193385	45.981	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.960%
24) Chloroform-d	7.648	84	546342	21.104	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.400%
26) 1,2-Dichloroethane-d4	8.307	65	323069	22.069	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.280%
32) Benzene-d6	8.276	84	1132925	21.374	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.480%
36) 1,2-Dichloropropane-d6	9.270	67	368639	21.737	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.960%
41) Toluene-d8	10.325	98	976362	20.657	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.640%
43) trans-1,3-Dichloroprop...	10.575	79	144094	20.961	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.840%
47) 2-Hexanone-d5	10.922	63	133626	46.208	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.420%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	295442	22.857	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	312108	23.391	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.560%
Target Compounds					Qvalue	
13) Acetone	4.118	43	48763	13.076	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050423\
Data File : VW025852.D
Acq On : 04 May 2023 18:09
Operator : SY/MD
Sample : 02574-22RE
Misc : 4.94g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCQ4

Quant Time: May 04 23:20:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 04 23:16:54 2023
Response via : Initial Calibration

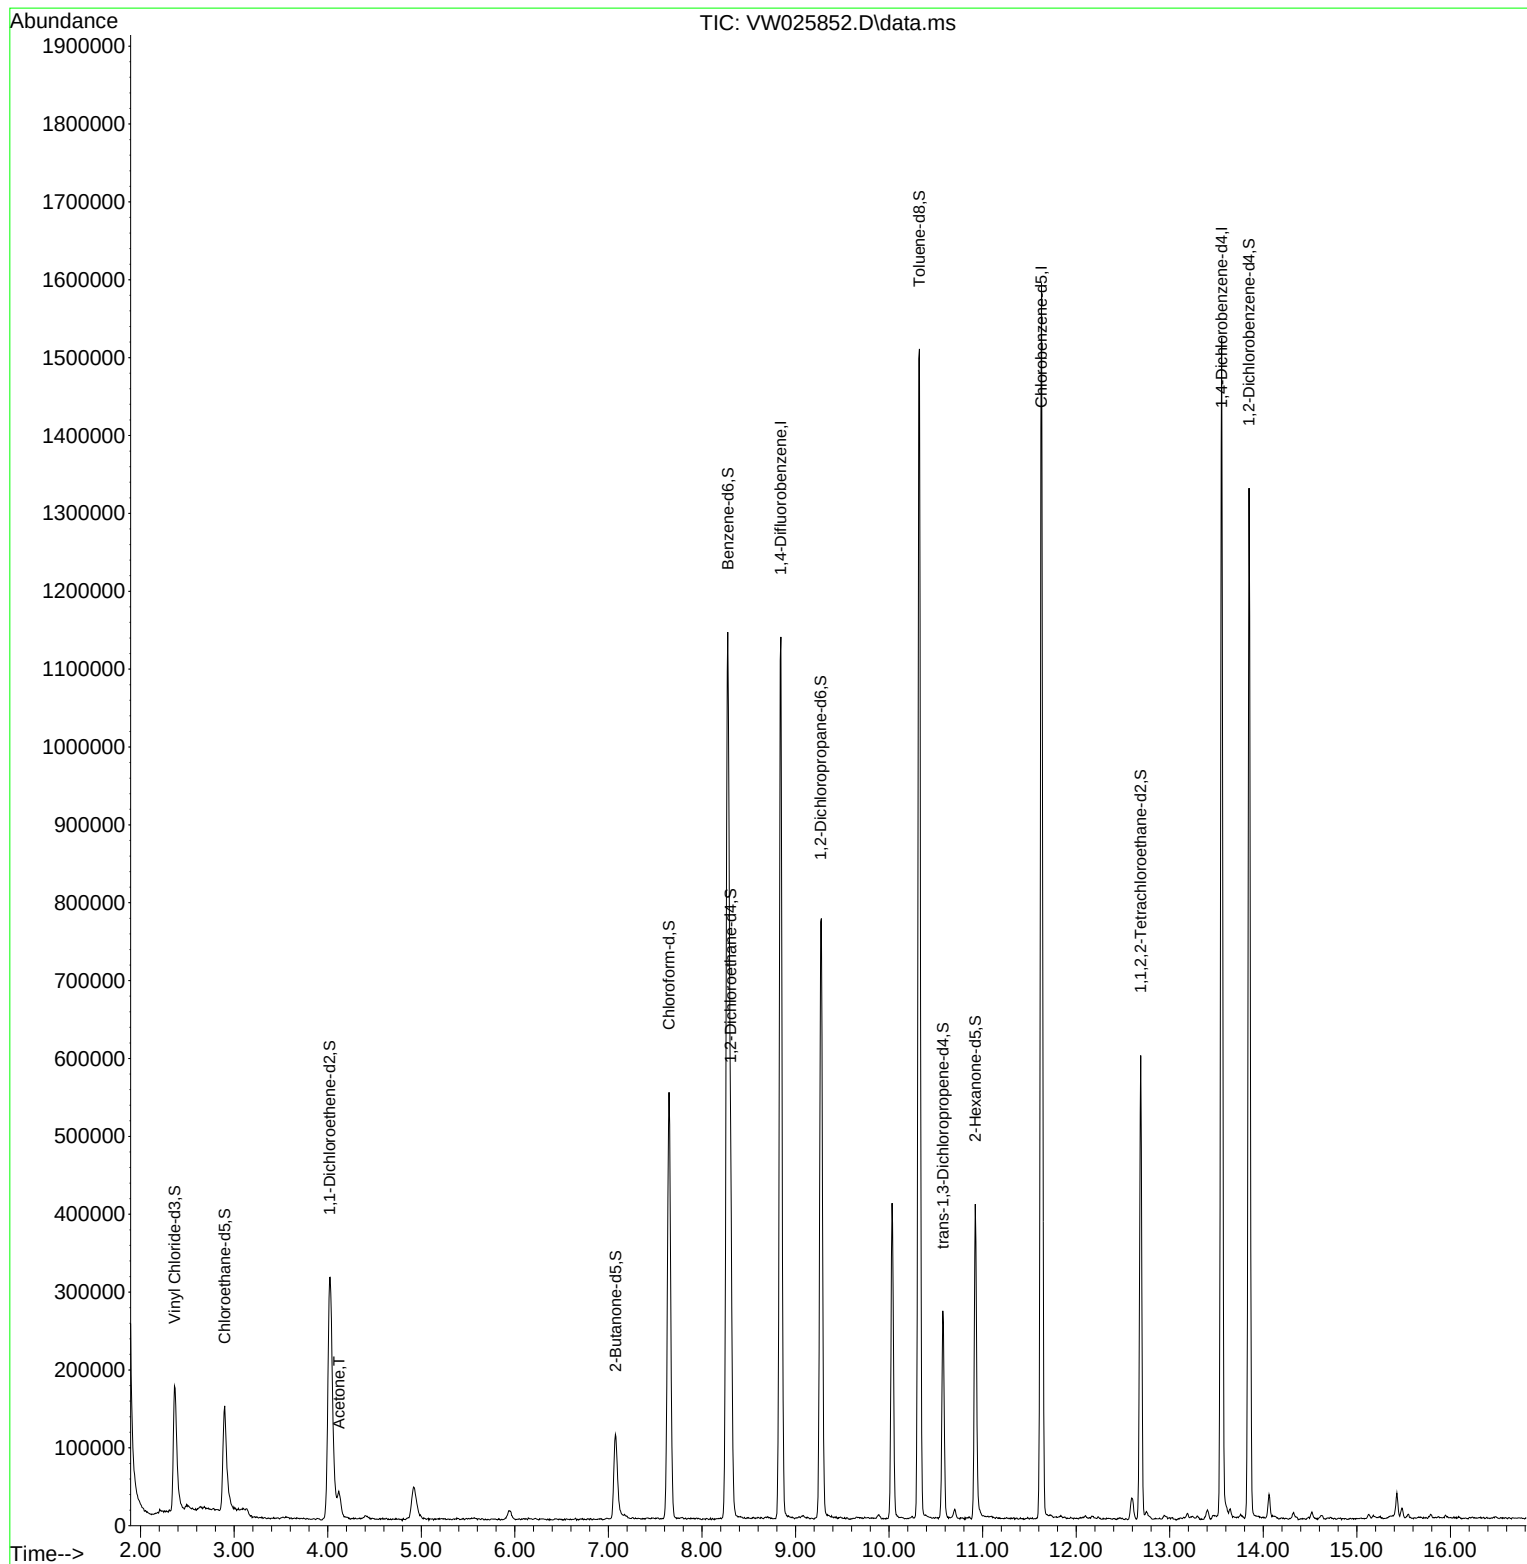

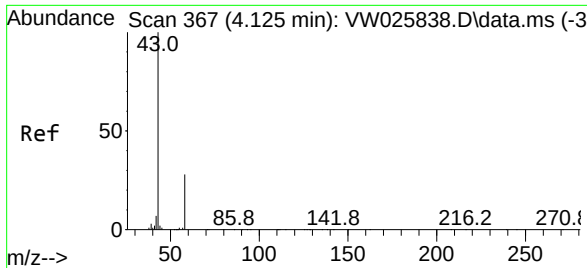

#13
 Acetone
 Concen: 13.076 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025852.D
 Acq: 04 May 2023 18:09

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCQ4

Tgt Ion: 43 Resp: 48763
 Ion Ratio Lower Upper
 43 100
 58 29.1 0.0 58.2

