

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050423\
 Data File : VW025855.D
 Acq On : 04 May 2023 19:21
 Operator : SY/MD
 Sample : 02592-01
 Misc : 2.56g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JRED2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2023
 Supervised By :Mahesh Dadoda 05/07/2023

Quant Time: May 04 23:21:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 23:16:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	901883	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	741528	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	259113	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	249924	19.555	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.240%		
7) Chloroethane-d5	2.893	69	209601	22.122	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.480%		
11) 1,1-Dichloroethene-d2	4.021	65	125633	19.632	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	78.520%		
21) 2-Butanone-d5	7.075	46	132175	31.284	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	62.560%		
24) Chloroform-d	7.648	84	496972	19.110	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	76.440%		
26) 1,2-Dichloroethane-d4	8.307	65	280765m	19.092	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	76.360%		
32) Benzene-d6	8.276	84	1042861	21.523	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.080%		
36) 1,2-Dichloropropane-d6	9.270	67	333015	21.481	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	85.920%		
41) Toluene-d8	10.325	98	894539	20.704	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.800%		
43) trans-1,3-Dichloroprop...	10.574	79	91370	14.540	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	58.160%		
47) 2-Hexanone-d5	10.922	63	84652	32.022	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	64.040%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	211290	17.882	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	71.520%		
66) 1,2-Dichlorobenzene-d4	13.848	152	196208	20.772	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	83.080%		
Target Compounds					Qvalue	
13) Acetone	4.118	43	18509	4.941	ug/L	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050423\
Data File : VW025855.D
Acq On : 04 May 2023 19:21
Operator : SY/MD
Sample : 02592-01
Misc : 2.56g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
JRED2

Quant Time: May 04 23:21:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 04 23:16:54 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2023
Supervised By :Mahesh Dadoda 05/07/2023

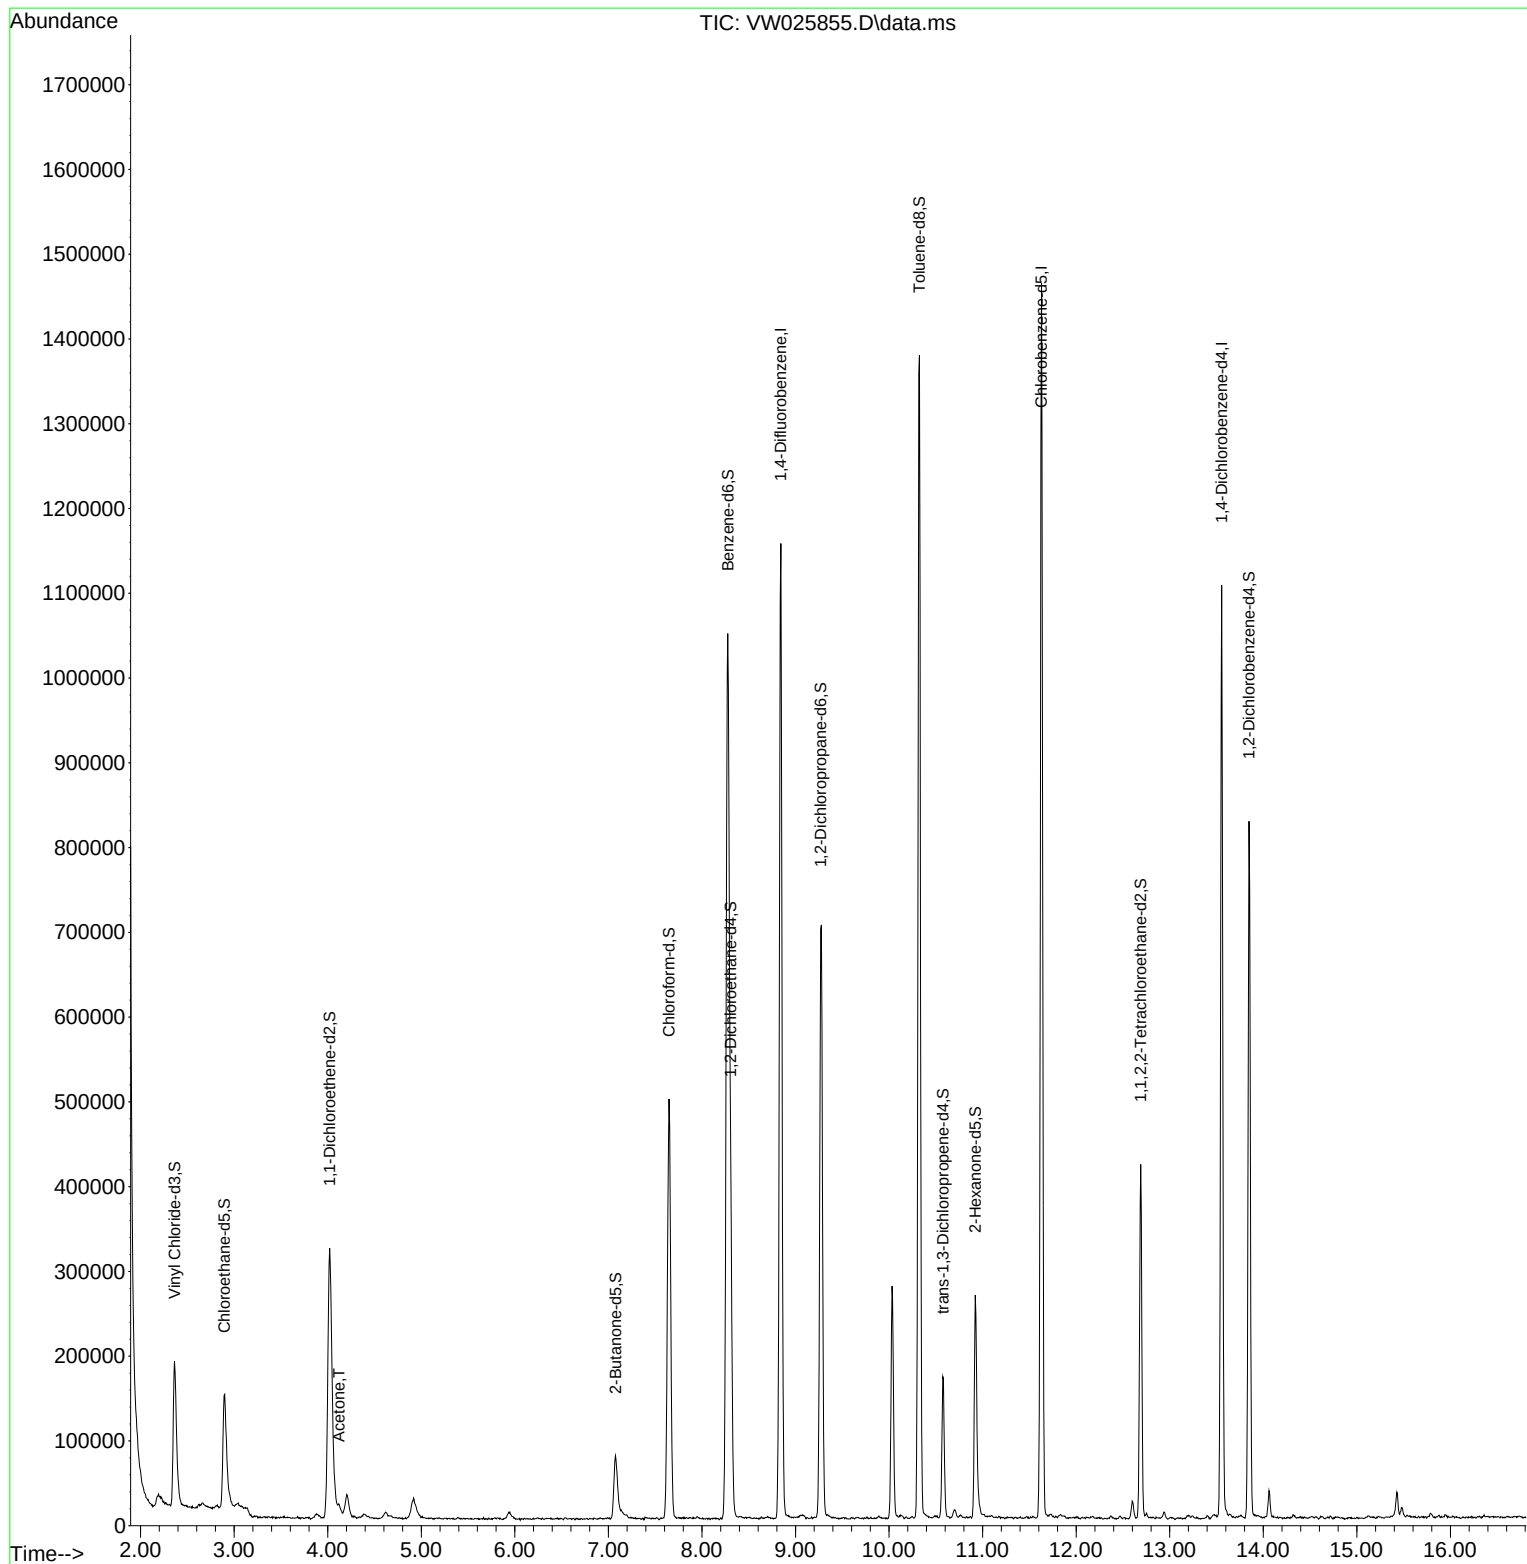

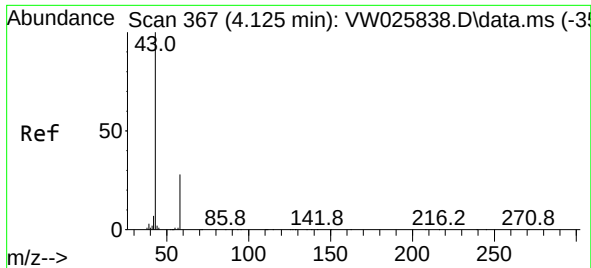

#13

Acetone

Concen: 4.941 ug/L

RT: 4.118 min Scan# 30

Delta R.T. -0.006 min

Lab File: VW025855.D

Acq: 04 May 2023 19:21

Instrument :

MSVOA_W

ClientSampleId :

JRED2

Tgt Ion: 43 Resp: 18509

Ion Ratio Lower Upper

43 100

58 20.0 0.0 58.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2023

Supervised By :Mahesh Dadoda 05/07/2023

