


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW050620\  
 Data File : VW015404.D  
 Acq On : 06 May 2020 09:12  
 Operator : SY/VA  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W050620S.M  
 Title : SW846 8260  
 Last Update : Tue May 05 18:41:17 2020

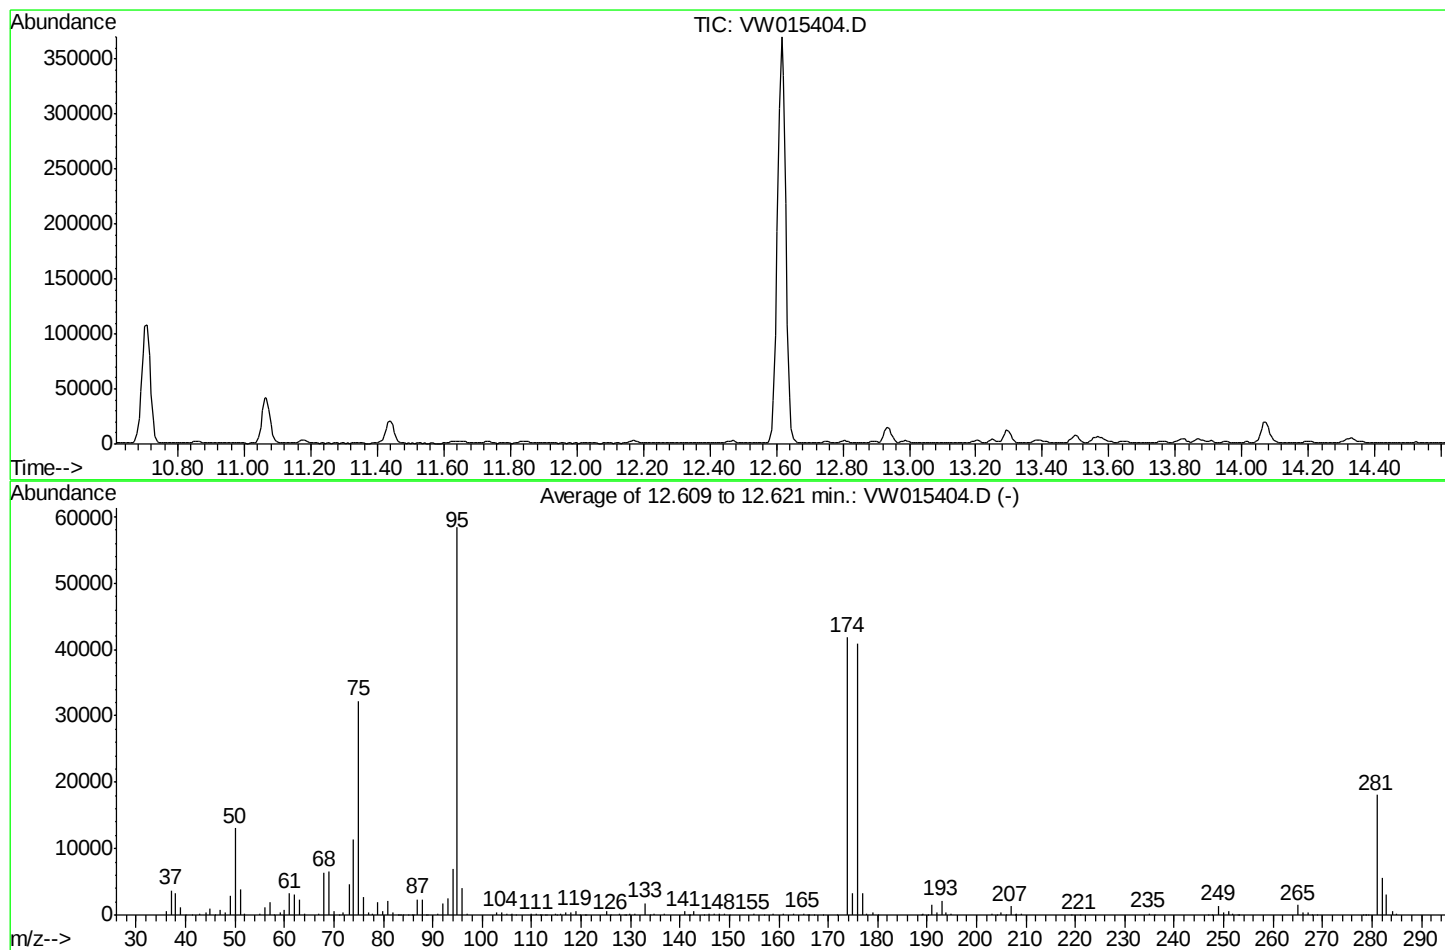

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 22.3      | 13052   | PASS             |
| 75          | 95           | 30           | 60           | 55.3      | 32312   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 58418   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 3978    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 71.6      | 41813   | PASS             |
| 175         | 174          | 5            | 9            | 8.1       | 3381    | PASS             |
| 176         | 174          | 95           | 101          | 97.9      | 40944   | PASS             |
| 177         | 176          | 5            | 9            | 7.9       | 3240    | PASS             |