

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050719\
Quantitation Report (QT/LSC Reviewed)


Data File : VW010315.D
Acq On : 07 May 2019 23:15
Operator : SY/VA
Sample : K2613-23
Misc : 6.20G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BFHF8

Quant Time: May 08 07:13:17 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM050719S.M
Quant Title : VOC Analysis
QLast Update : Wed May 08 02:05:40 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
5/10/2019 6:03:23 PM

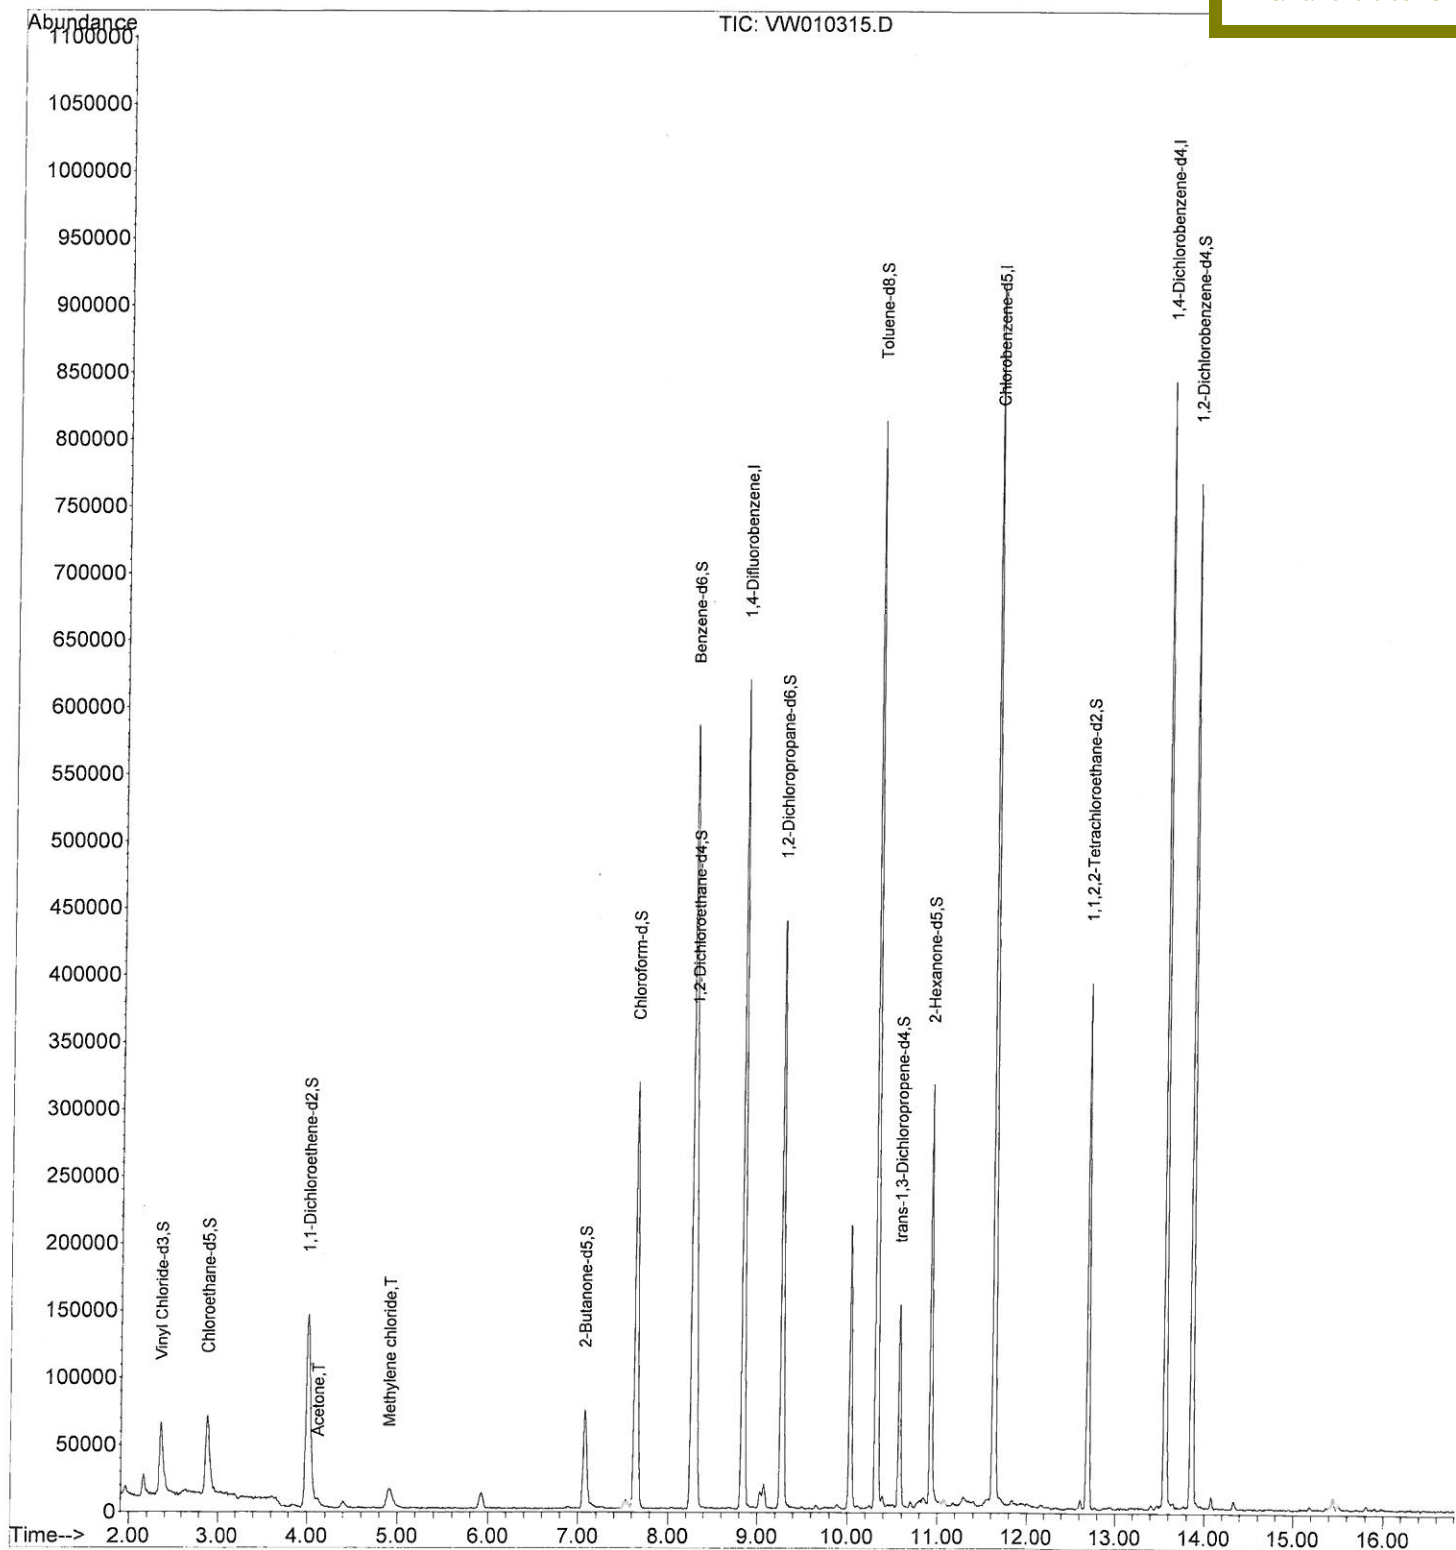

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW050719\
 Data File : VW010315.D
 Acq On : 07 May 2019 23:15
 Operator : SY/VA
 Sample : K2613-23
 Misc : 6.20G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFHF8

Quant Time: May 08 04:40:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM050719S.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 08 02:05:40 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 5/10/2019 6:03:23 PM

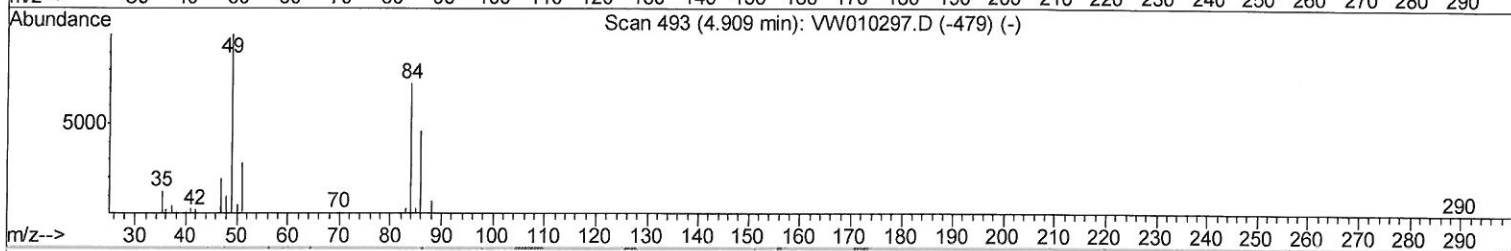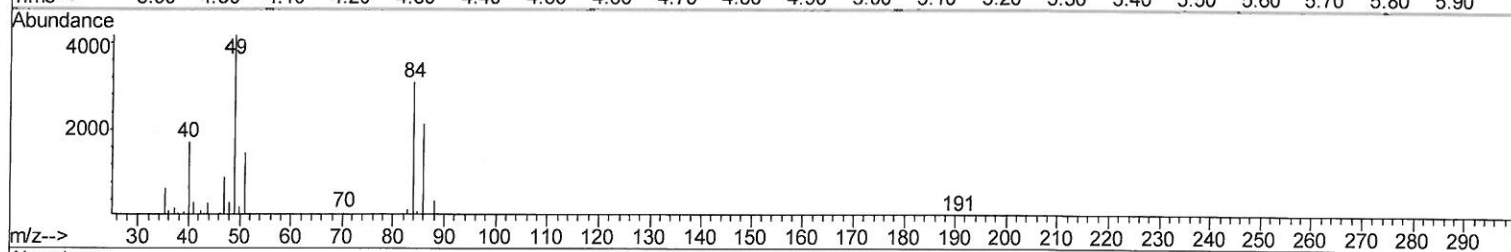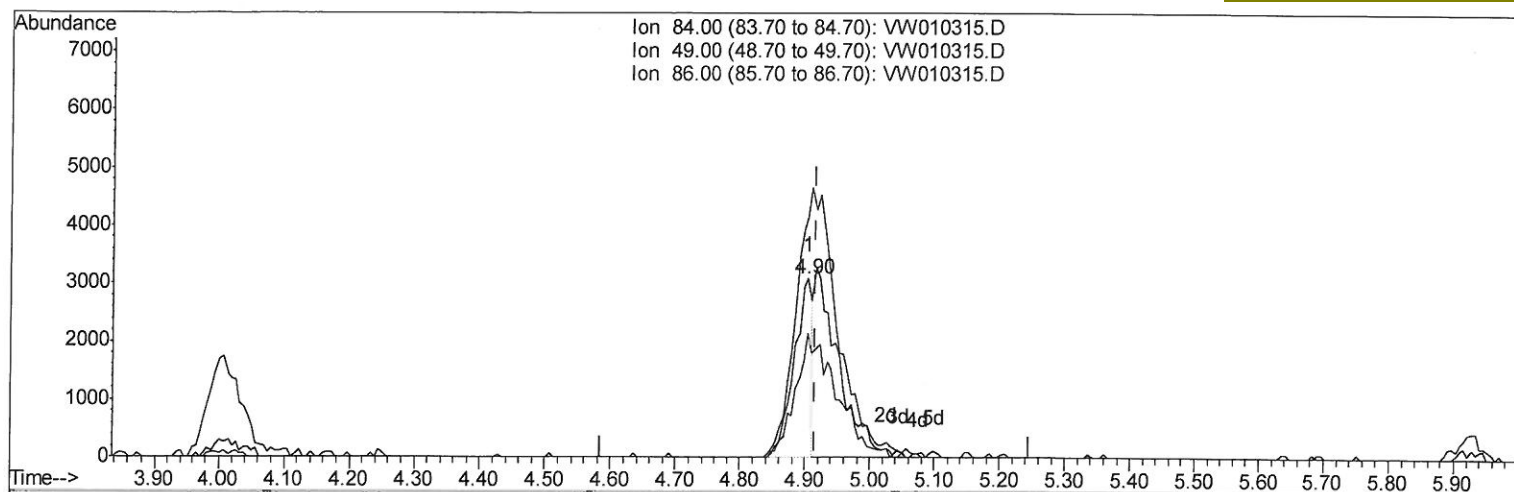

TIC: VW010315.D

(16) Methylene chloride (T)

4.903min (-0.012) 0.92ug/L

response 5920

Ion	Exp%	Act%
84.00	100	100
49.00	134.90	134.80
86.00	62.60	69.64
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW050719\
 Data File : VW010315.D
 Acq On : 07 May 2019 23:15
 Operator : SY/VA
 Sample : K2613-23
 Misc : 6.20G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFHF8

Quant Time: May 08 04:40:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM050719S.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 08 02:05:40 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 5/10/2019 6:03:23 PM

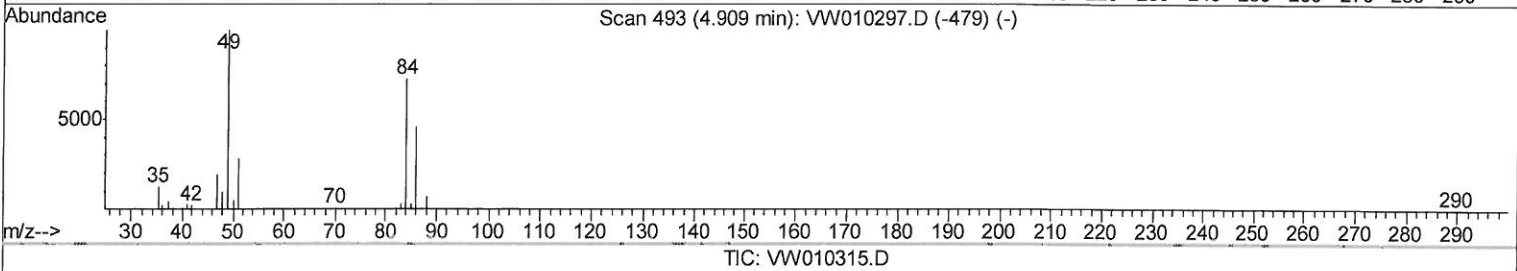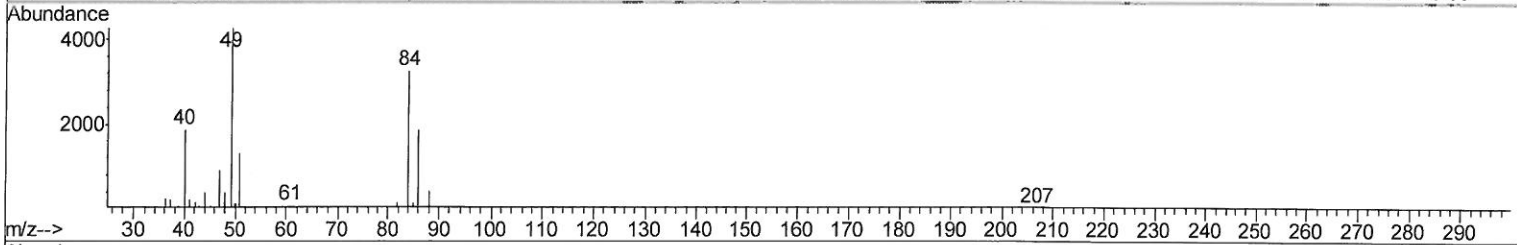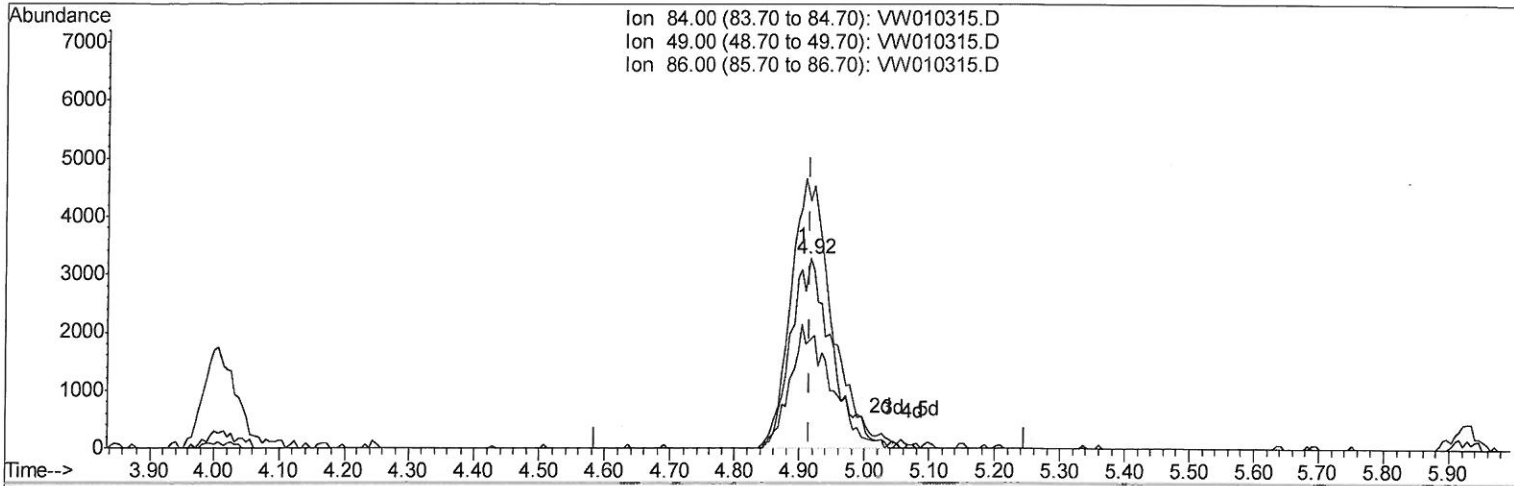

(16) Methylene chloride (T)

4.916min (+0.000) 2.23ug/L m

response 14396

Ion	Exp%	Act%
84.00	100	100
49.00	134.90	130.55
86.00	62.60	57.40
0.00	0.00	0.00

205/09/19 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050719\
Quantitation Report (QT/LSC Reviewed)

Data File : VW010315.D
Acq On : 07 May 2019 23:15
Operator : SY/VA
Sample : K2613-23
Misc : 6.20G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BFHF8

Manual Integrations
APPROVED

MMDadoda
5/10/2019 6:03:23 PM

Quant Time: May 08 07:13:17 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM050719S.M
Quant Title : VOC Analysis
Qlast Update : Wed May 08 02:05:40 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	477700	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	481654	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	201885	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	92701	16.67	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.68%		
7) Chloroethane-d5	2.89	69	86497	18.59	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.36%		
10) 1,1-Dichloroethene-d2	4.01	63	183854	13.27	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	53.08%		
20) 2-Butanone-d5	7.07	46	122340	47.48	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.96%		
24) Chloroform-d	7.64	84	314992	24.76	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	99.04%		
26) 1,2-Dichloroethane-d4	8.31	65	202923	26.94	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	107.76%		
29) Benzene-d6	8.27	84	576182	22.02	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.08%		
33) 1,2-Dichloropropane-d6	9.27	67	202441	25.31	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.24%		
37) Toluene-d8	10.32	98	500155	21.44	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.76%		
38) trans-1,3-Dichloropropene-	10.58	79	79234	21.67	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.68%		
39) 2-Hexanone-d5	10.93	63	91103	44.58	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	89.16%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	181000	23.80	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	95.20%		
61) 1,2-Dichlorobenzene-d4	13.86	152	190975	27.72	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	110.88%		

Target Compounds

			Qvalue	
13) Acetone	4.12	43	6248	2.834 ug/L 91
16) Methylene chloride	4.92	84	14396m	2.226 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed