

Data Path : W:\HPCHEM1\MSVOA W\DATA\VW050818\
 Data File : VW002325.D
 Acq On : 09 May 2018 05:49
 Operator : JC/SY
 Sample : J2754-01
 Misc : 6.34G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 LS-SOIL-PILE-1A

Quant Time: May 09 08:42:33 2018
 Quant Method : W:\HPCHEM1\MSVOA_W\METHOD\82W050818S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 08 03:57:58 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	213739	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	342435	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	290005	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	123899	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	95661	42.15	ug/l	0.00
Spiked Amount	50.000		Recovery	=	84.30%	
35) Dibromofluoromethane	7.88	113	89817	40.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	81.84%	
50) Toluene-d8	10.33	98	286882	34.28	ug/l	0.00
Spiked Amount	50.000		Recovery	=	68.56%	
62) 4-Bromofluorobenzene	12.63	95	102727	33.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	67.92%	
Target Compounds						
20) Methylene Chloride	4.90	84	15648	7.32	ug/l	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA W\DATA\VW050818\
Data File : VW002325.D
Acq On : 09 May 2018 05:49
Operator : JC/SY
Sample : J2754-01
Misc : 6.34G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
LS-SOIL-PILE-1A

Quant Time: May 09 08:42:33 2018
Quant Method : W:\HPCHEM1\MSVOA_W\METHOD\82W050818S.M
Quant Title : SW846 8260
QLast Update : Tue May 08 03:57:58 2018
Response via : Initial Calibration

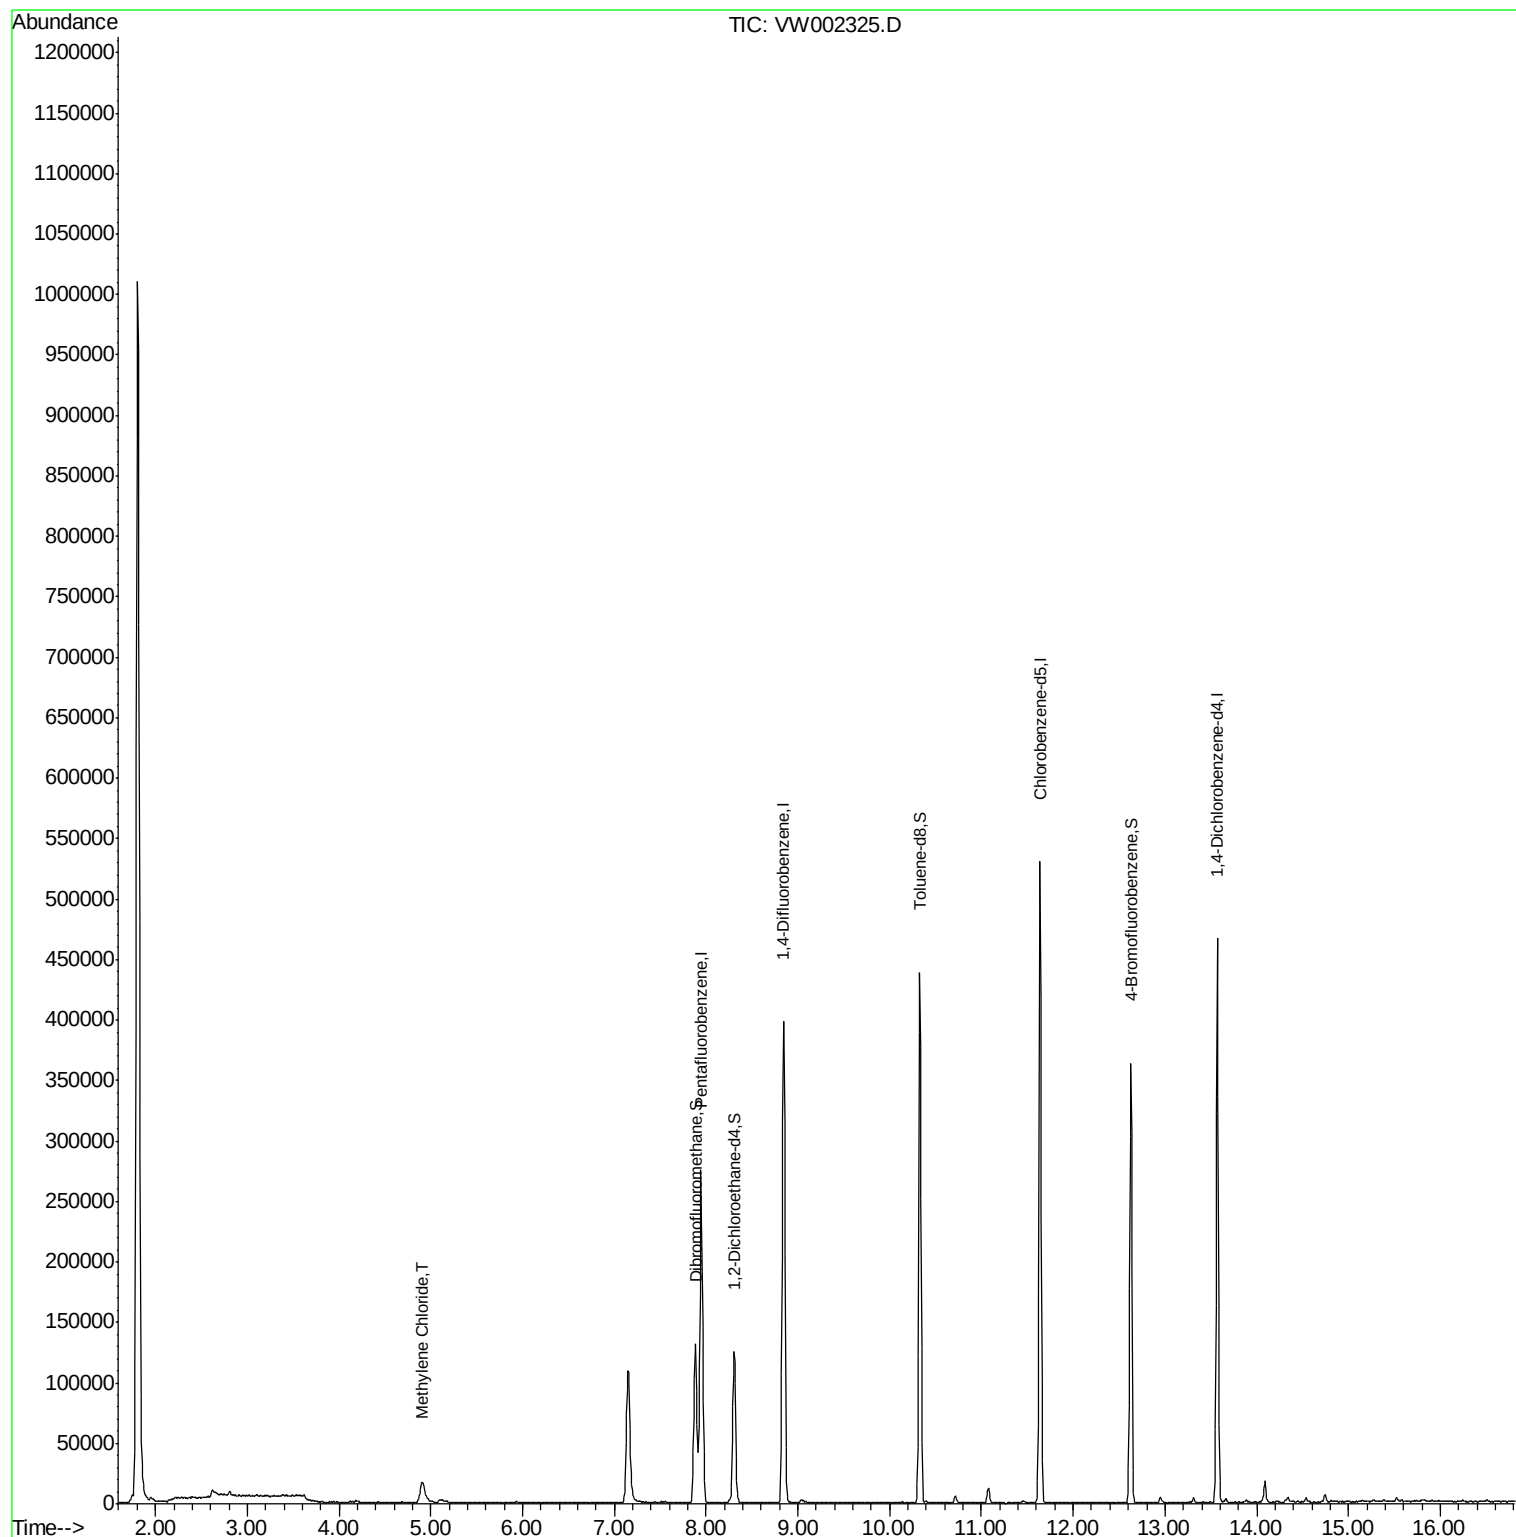

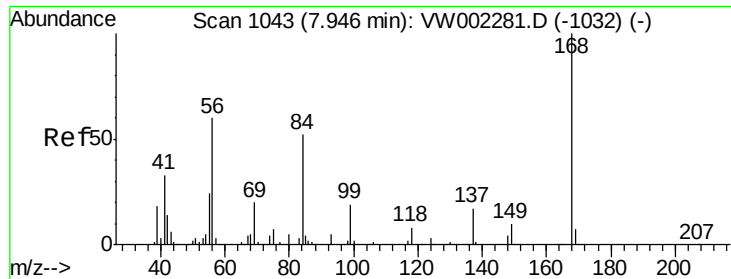

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.95 min Scan# 1043

Delta R.T. -0.00 min

Lab File: VW002325.D

Acq: 09 May 2018 05:49

Instrument :

MSVOA_W

ClientSampleId :


LS-SOIL-PILE-1A

Tot Ion:168 Resp: 213739

Ion Ratio Lower Upper




168 100

99 49.8 43.7 65.5

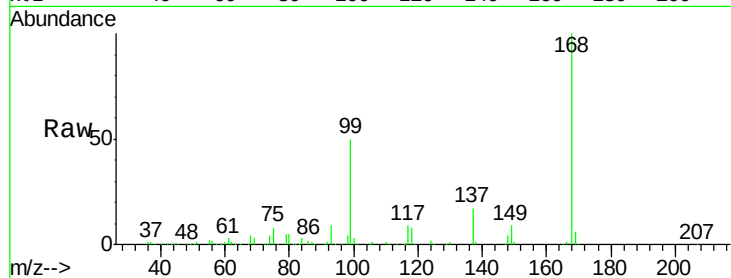

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

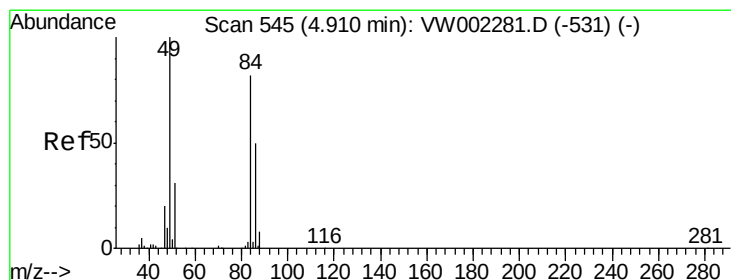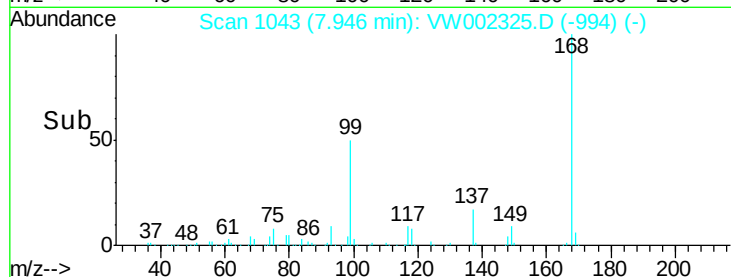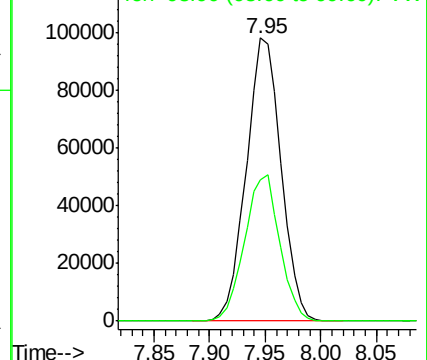

#20

Methylene Chloride

Concen: 7.32 ug/l

RT: 4.90 min Scan# 544

Delta R.T. -0.01 min

Lab File: VW002325.D

Acq: 09 May 2018 05:49

Tgt Ion: 84 Resp: 15648


Ion Ratio Lower Upper

84 100

49 133.8 97.7 146.5

51 44.8 30.2 45.4

86 63.7 48.9 73.3


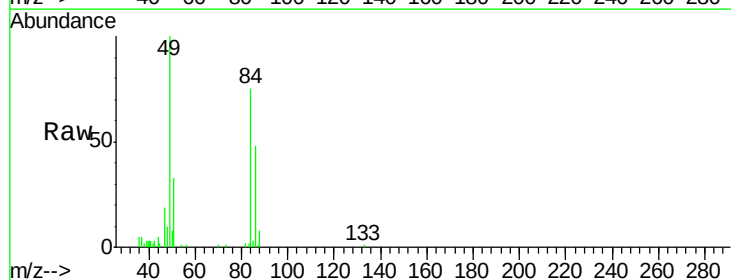



Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW



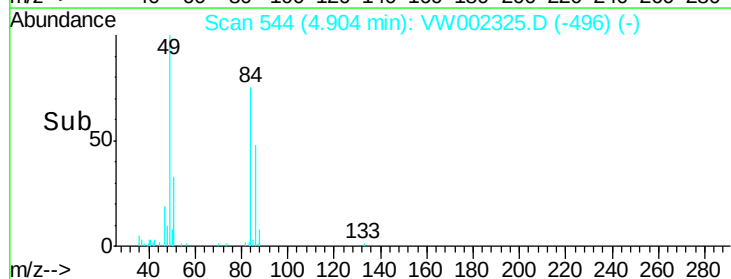
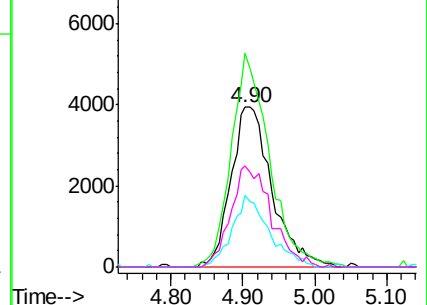


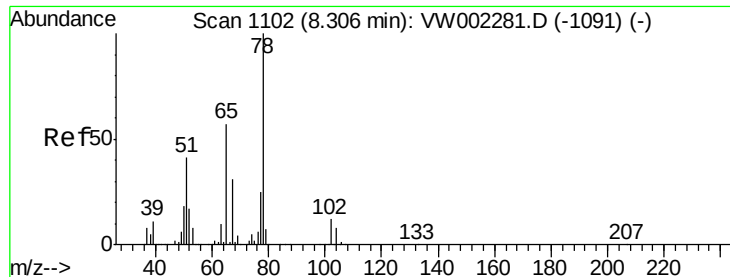

#33
 1,2-Dichloroethane-d4
 Concen: 42.15 ug/l
 RT: 8.31 min Scan# 1102
 Delta R.T. -0.00 min
 Lab File: VW002325.D
 Acq: 09 May 2018 05:49




Instrument :
 MSVOA_W
 ClientSampleId :
 LS-SOIL-PILE-1A


Tot Ion: 65 Resp: 95661
 Ion Ratio Lower Upper
 65 100
 67 52.3 0.0 107.2

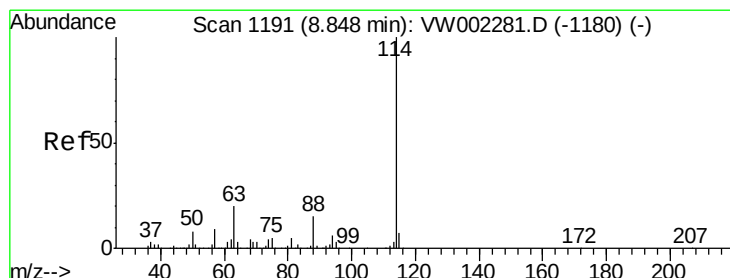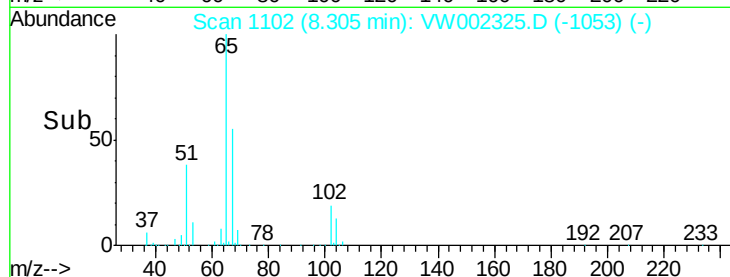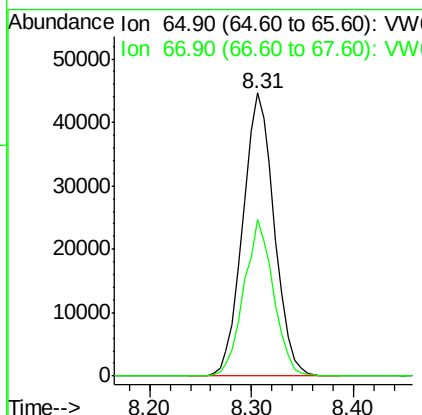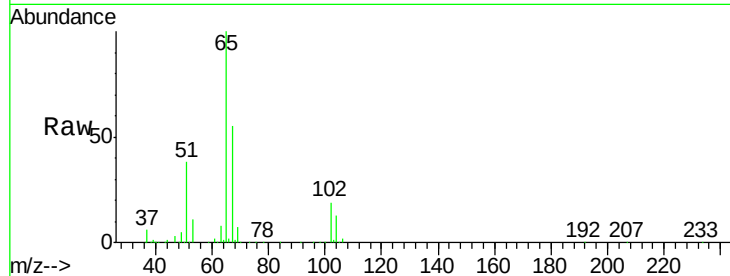

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.85 min Scan# 1191
 Delta R.T. -0.00 min
 Lab File: VW002325.D
 Acq: 09 May 2018 05:49

Tgt Ion: 114 Resp: 342435
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 39.0
 88 14.5 0.0 29.6


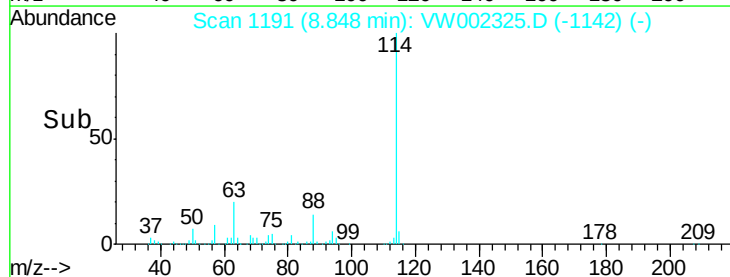
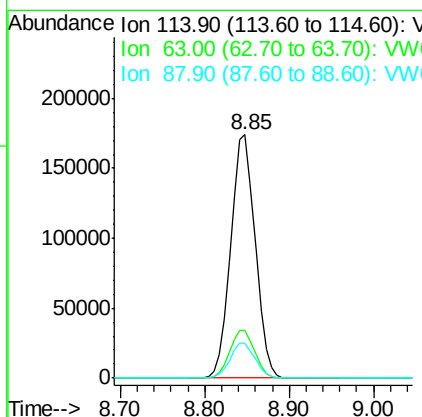
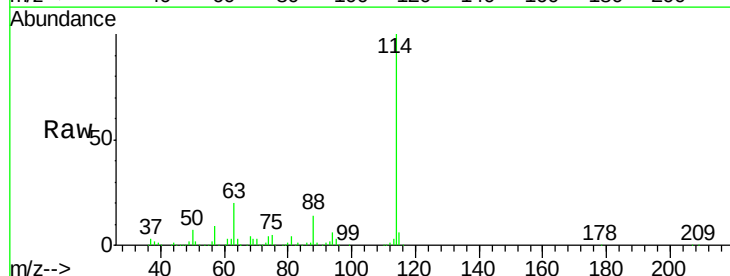


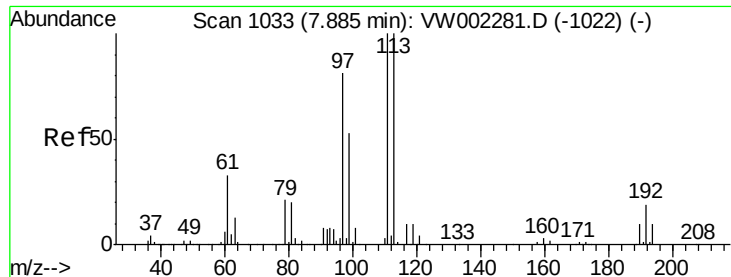

#35
 Dibromofluoromethane
 Concen: 40.92 ug/l
 RT: 7.88 min Scan# 1033
 Delta R.T. -0.00 min
 Lab File: VW002325.D
 Acq: 09 May 2018 05:49




Instrument :
 MSVOA_W
 ClientSampleId :
 LS-SOIL-PILE-1A


Tot Ion:113 Resp: 89817
 Ion Ratio Lower Upper
 113 100
 111 103.7 81.5 122.3
 192 21.4 16.4 24.6

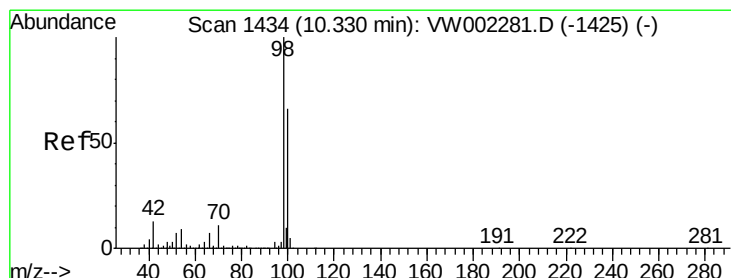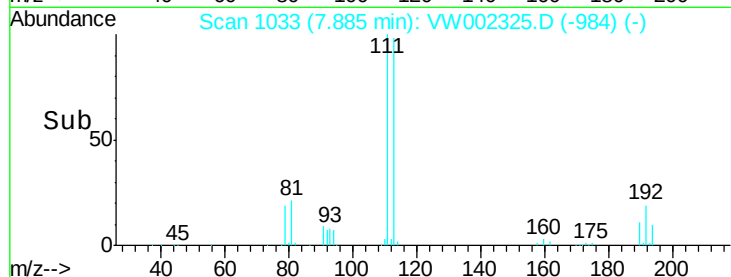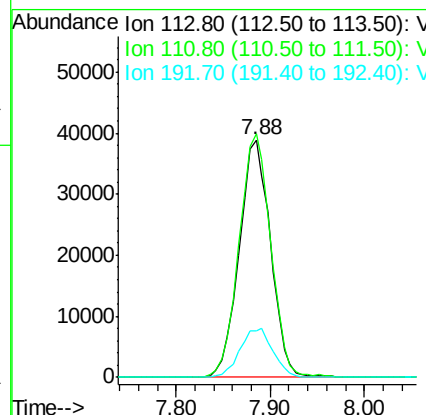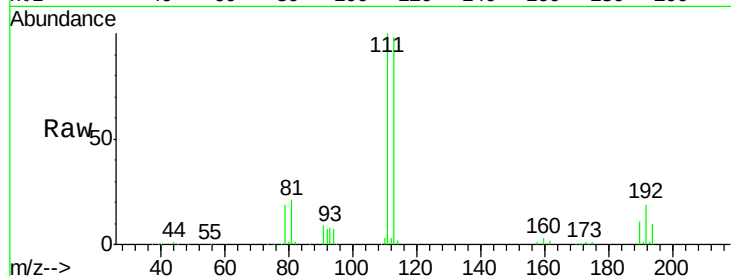

#50
 Toluene-d8
 Concen: 34.28 ug/l
 RT: 10.33 min Scan# 1434
 Delta R.T. -0.00 min
 Lab File: VW002325.D
 Acq: 09 May 2018 05:49

Tgt Ion: 98 Resp: 286882
 Ion Ratio Lower Upper
 98 100
 100 63.9 51.4 77.2

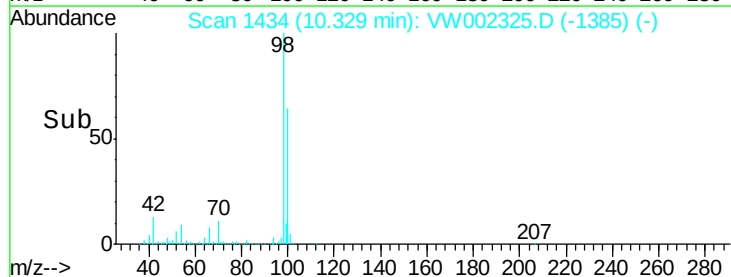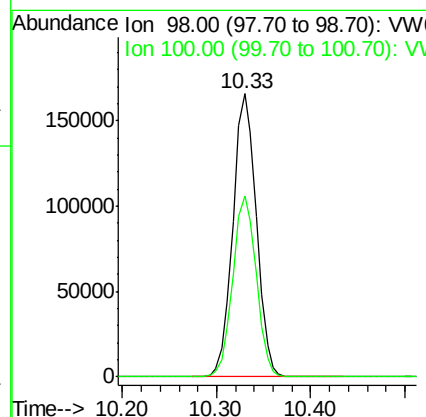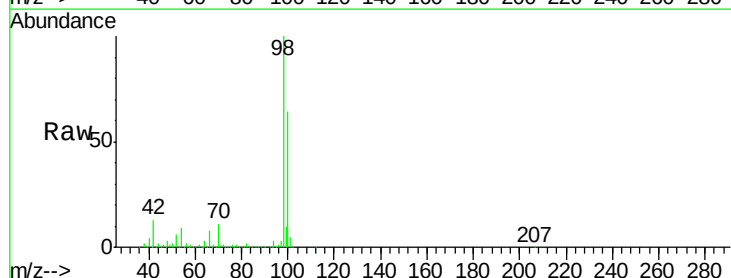

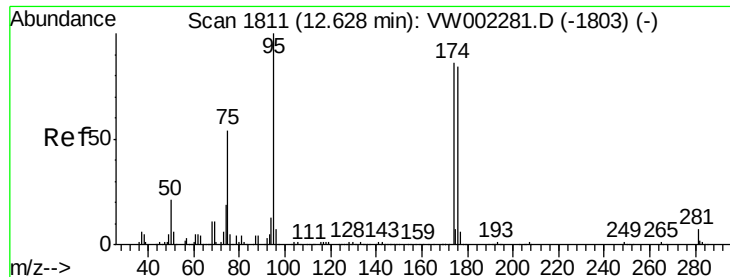

#62

4-Bromofluorobenzene

Concen: 33.96 ug/l

RT: 12.63 min Scan# 1811

Delta R.T. -0.00 min

Lab File: VW002325.D

Acq: 09 May 2018 05:49

Instrument :

MSVOA_W

ClientSampleId :

LS-SOIL-PILE-1A


Tot Ion: 95 Resp: 102727

Ion Ratio Lower Upper

95 100

174 89.3 0.0 176.8




176 85.5 0.0 170.4

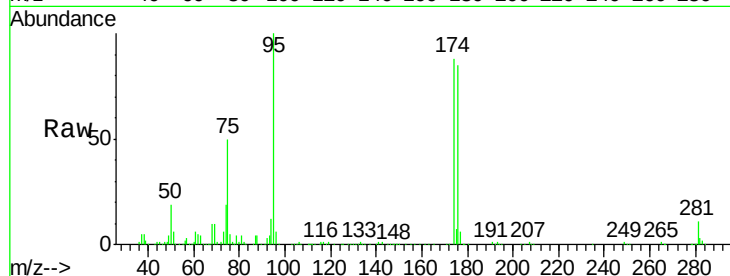

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

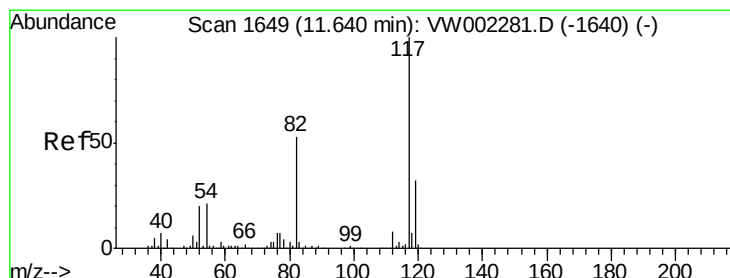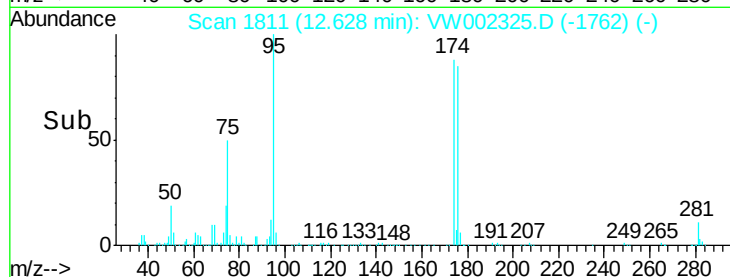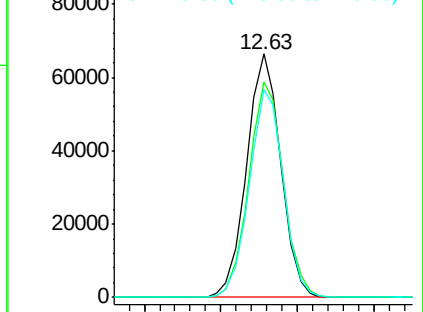

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.64 min Scan# 1649

Delta R.T. -0.00 min

Lab File: VW002325.D

Acq: 09 May 2018 05:49


Tgt Ion: 117 Resp: 290005

Ion Ratio Lower Upper

117 100

82 53.1 42.6 63.8



119 32.3 25.2 37.8

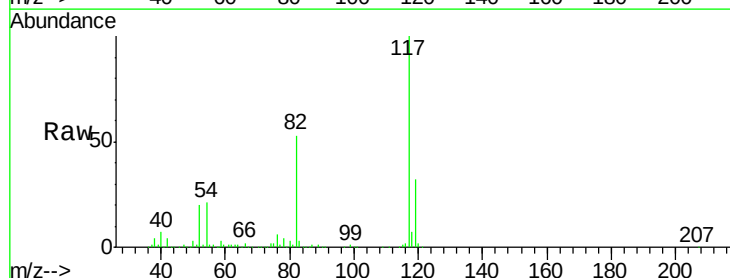


Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW

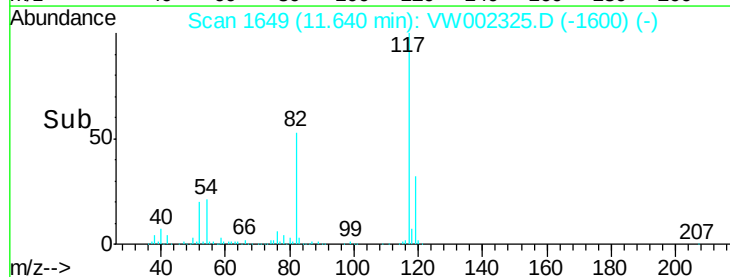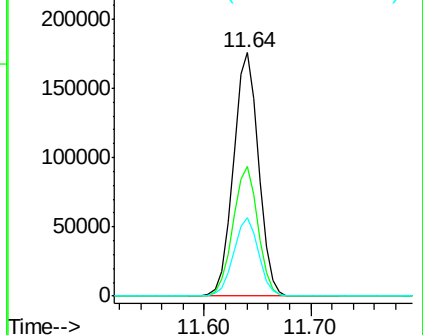


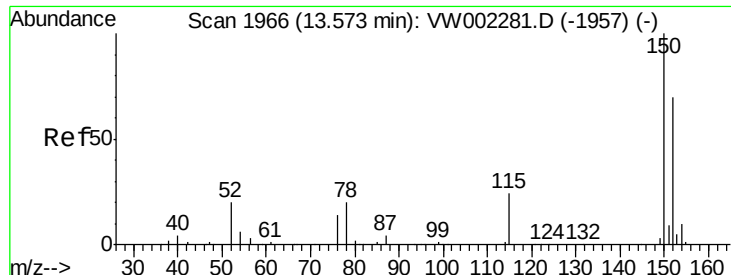

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.57 min Scan# 1966
 Delta R.T. -0.00 min
 Lab File: VW002325.D
 Acq: 09 May 2018 05:49

Instrument :
 MSVOA_W
 ClientSampleId :
 LS-SOIL-PILE-1A

Tot Ion	Ratio	Lower	Upper
152	100		
115	55.2	28.5	85.5
150	155.4	0.0	342.6

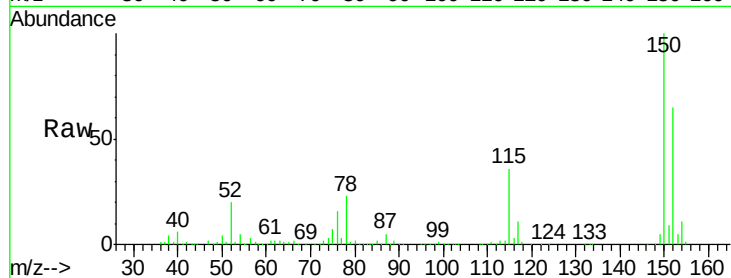

Abundance Ion 151.90 (151.60 to 152.60): V
 Ion 114.90 (114.60 to 115.60): V
 Ion 149.90 (149.60 to 150.60): V

