


Data Path : W:\HPCHEM1\MSVOA W\DATA\VW050818\
 Data File : VW002277.D
 Acq On : 07 May 2018 22:06
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_W\METHOD\82W050818S.M
 Title : SW846 8260
 Last Update : Tue May 08 03:57:58 2018

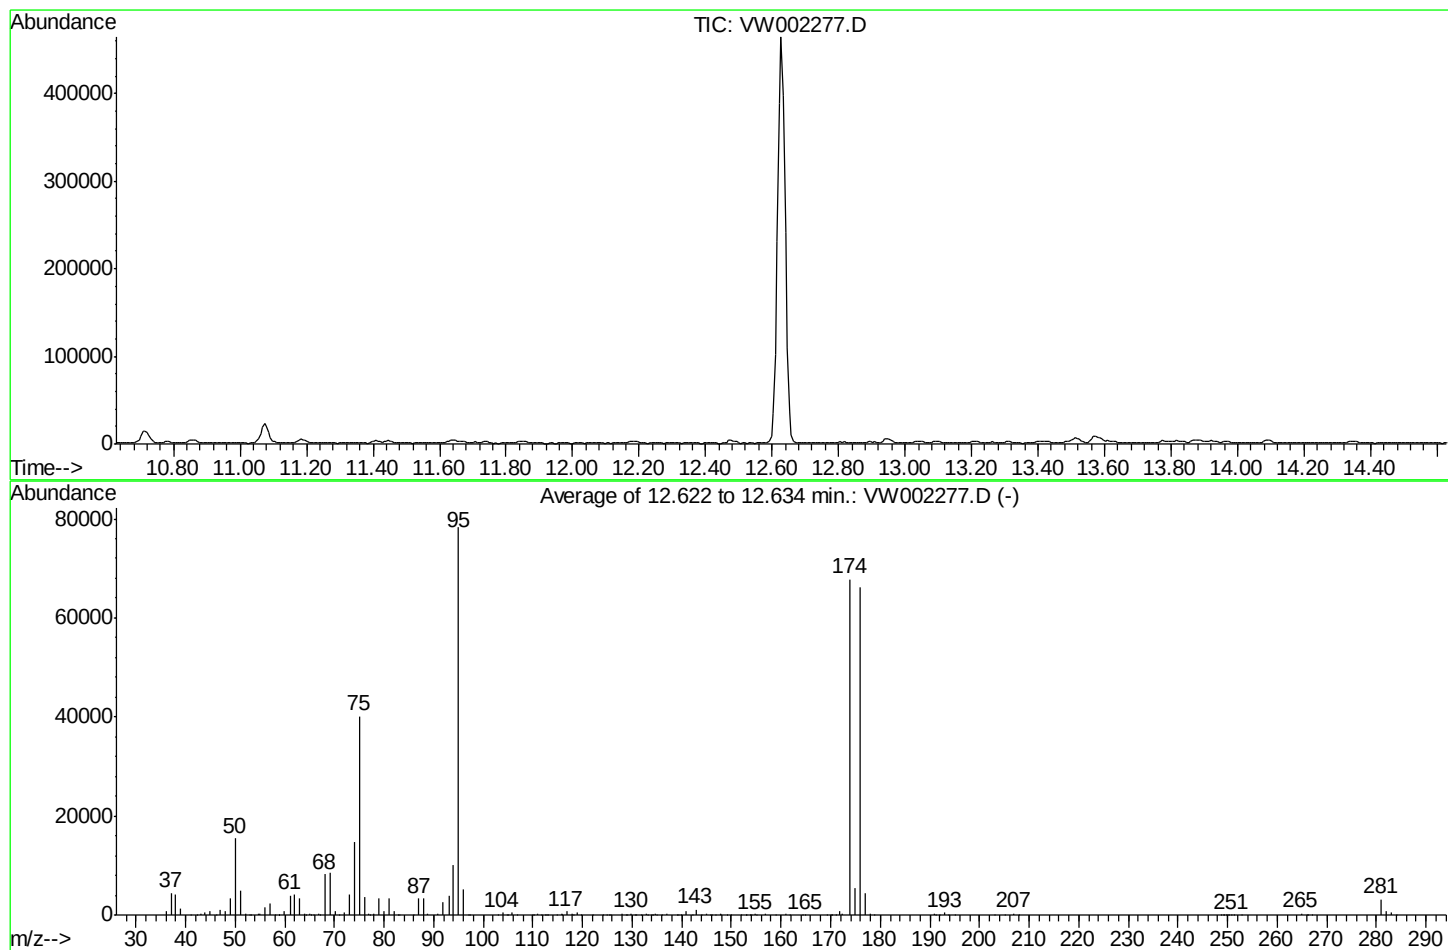

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	15471	PASS
75	95	30	60	51.3	40178	PASS
95	95	100	100	100.0	78280	PASS
96	95	5	9	6.7	5270	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.6	67829	PASS
175	174	5	9	8.1	5464	PASS
176	174	95	101	97.4	66096	PASS
177	176	5	9	6.8	4526	PASS