


Data Path : W:\HPCHEM1\MSVOA W\DATA\VW050818\
 Data File : VW002308.D
 Acq On : 08 May 2018 21:54
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_W\METHOD\82W050818S.M
 Title : SW846 8260
 Last Update : Tue May 08 03:57:58 2018

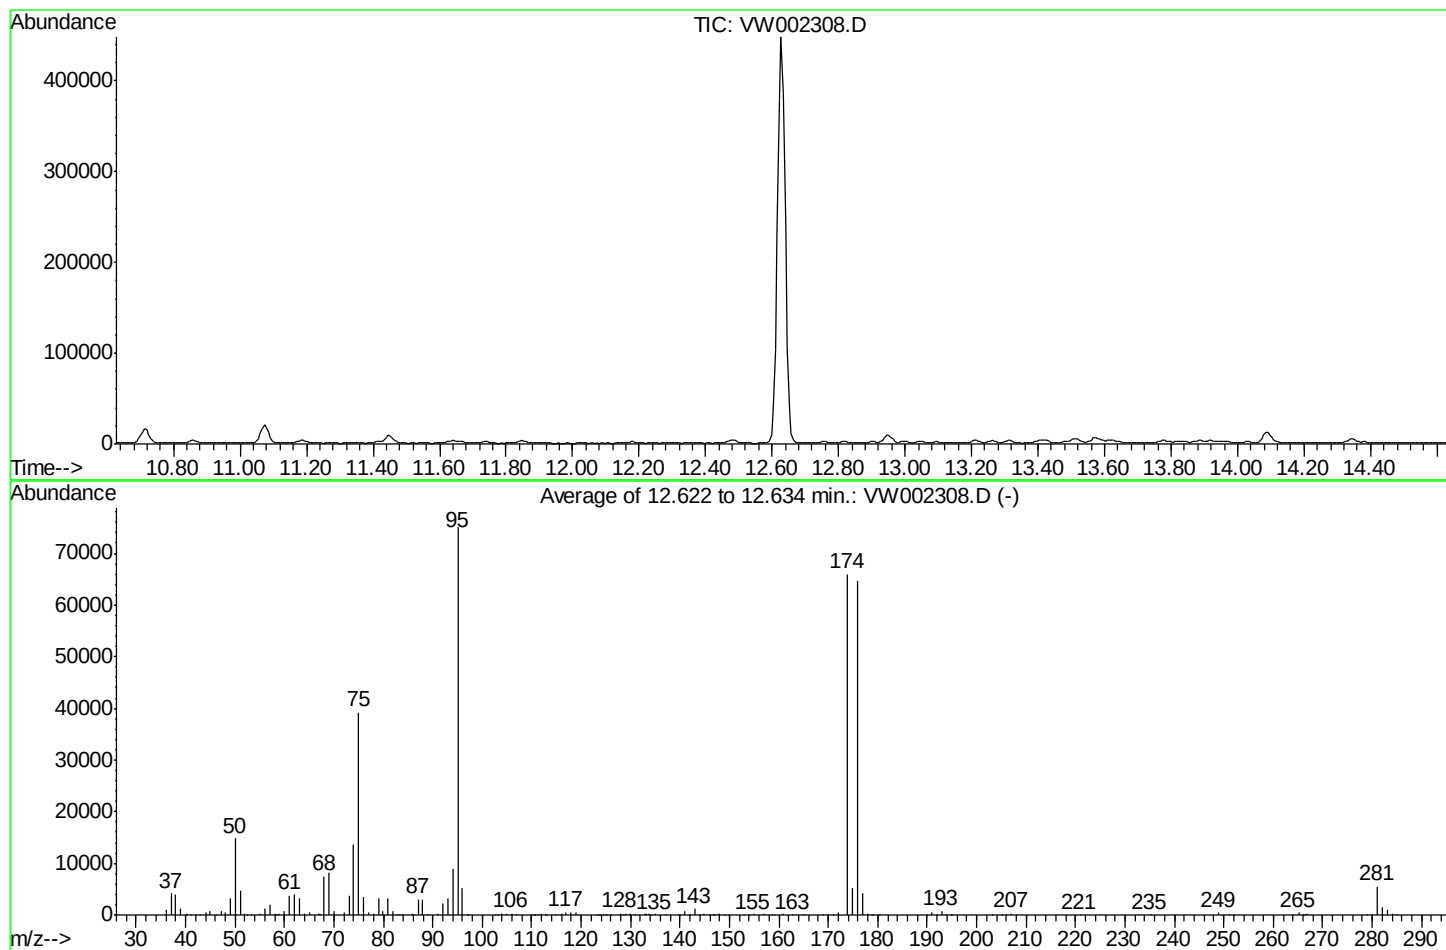

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	14821	PASS
75	95	30	60	52.2	39178	PASS
95	95	100	100	100.0	75040	PASS
96	95	5	9	6.9	5189	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.9	65965	PASS
175	174	5	9	7.9	5226	PASS
176	174	95	101	97.9	64600	PASS
177	176	5	9	6.6	4281	PASS