


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW050820\
 Data File : VW015421.D
 Acq On : 08 May 2020 11:16
 Operator : SY/VA
 Sample : BFB29
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB29

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM050420S.M
 Title : VOC Analysis
 Last Update : Sat May 09 06:17:32 2020

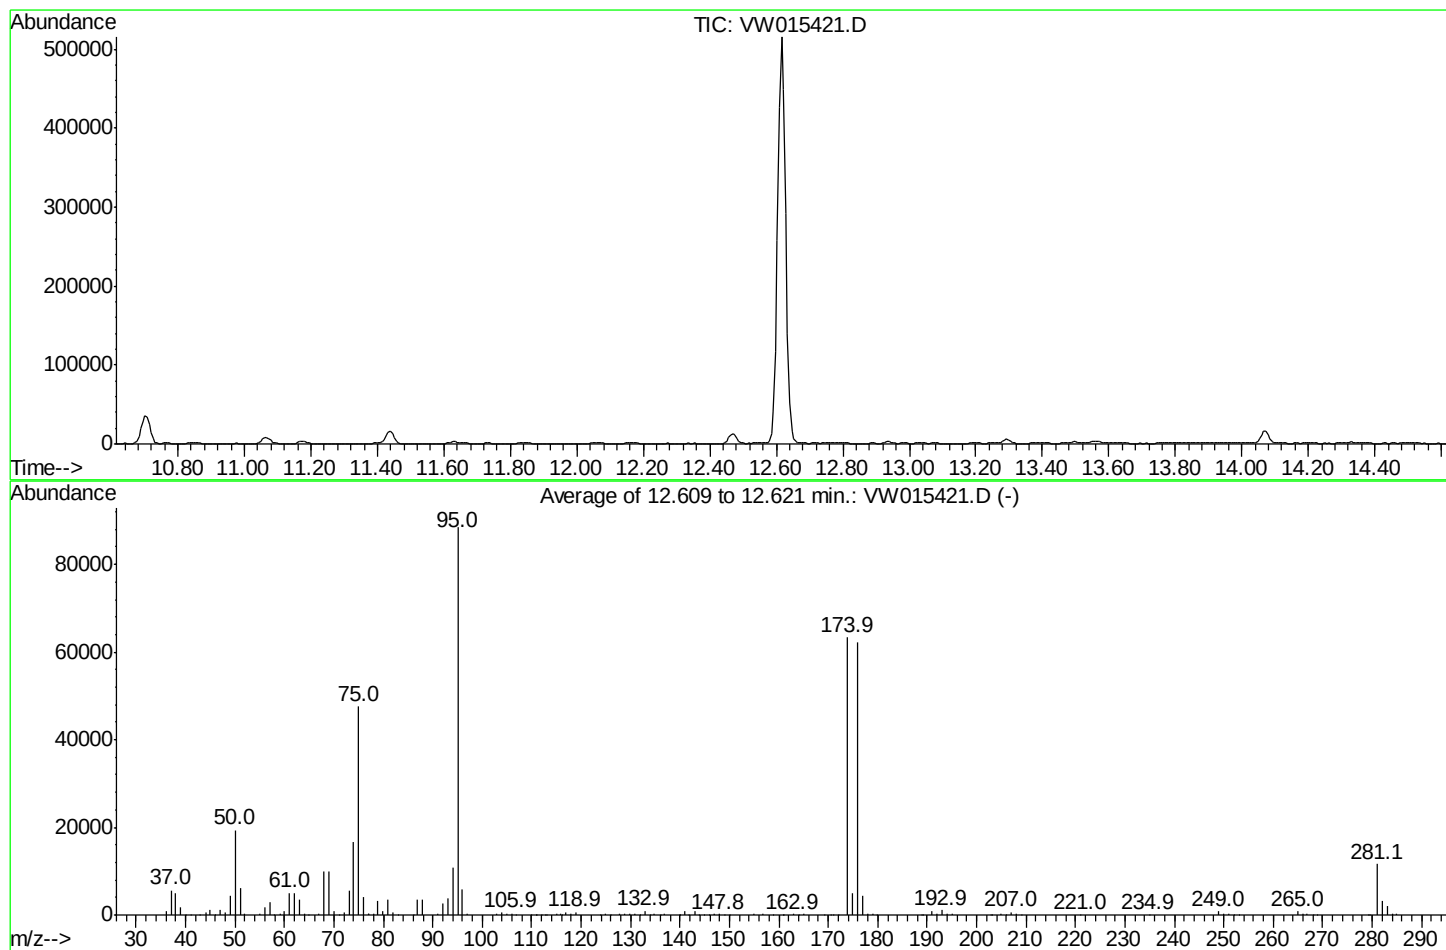

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	19408	PASS
75	95	30	80	53.7	47509	PASS
95	95	100	100	100.0	88461	PASS
96	95	5	9	6.7	5943	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.5	63253	PASS
175	174	5	9	8.0	5087	PASS
176	174	95	101	98.5	62317	PASS
177	176	5	9	6.9	4285	PASS

m/z	Abundance
36.00	988.0
37.00	5177.0
38.00	4346.0
39.10	1552.0
39.90	215.0
41.00	59.0
43.10	166.0
44.00	843.0
45.00	903.0
46.00	66.0
47.00	1025.0
47.90	570.0
49.00	4139.0
50.00	18176.0
51.00	5795.0
52.10	257.0
54.90	316.0
56.00	1528.0
57.00	2726.0
58.00	189.0
59.10	91.0
60.00	1046.0
61.00	4613.0
62.00	4724.0
63.00	3533.0
64.10	307.0
65.00	75.0
67.00	235.0
68.00	9649.0
69.00	9558.0
70.00	708.0
72.10	586.0
73.00	4837.0
74.00	15953.0
75.00	46120.0
76.00	3811.0
77.00	487.0
77.90	300.0
78.90	3022.0
80.00	848.0
80.90	2991.0
81.90	710.0
82.90	108.0
87.00	3403.0
87.90	3484.0
91.00	392.0
92.00	2736.0
93.00	3906.0
94.00	10431.0
95.00	88512.0
96.00	6079.0
96.90	211.0
103.00	151.0
103.90	408.0
104.90	158.0
105.90	422.0
106.80	127.0
109.90	61.0
110.80	102.0
111.80	150.0
112.90	117.0
114.90	137.0
116.10	267.0
116.90	621.0
117.90	341.0
118.90	655.0
123.80	82.0
125.00	229.0
126.00	84.0
127.80	247.0
128.90	152.0
129.90	287.0
130.80	182.0
133.00	516.0
134.00	189.0
134.90	182.0
137.00	178.0
140.90	820.0
141.80	84.0
142.90	886.0
144.80	95.0
145.90	125.0
146.90	197.0
147.80	225.0
148.90	76.0
149.90	116.0
154.90	162.0
156.80	153.0
158.90	93.0
161.00	155.0
162.90	90.0
164.80	101.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

168.90	97.0
171.10	55.0
173.90	64408.0
175.00	5317.0
175.90	68552.0
176.90	4564.0
177.90	126.0
178.90	132.0
191.00	424.0
192.00	97.0
192.90	543.0
193.90	116.0
195.00	73.0
203.10	97.0
205.00	134.0
207.10	410.0
207.90	62.0
208.90	52.0
249.00	391.0
250.00	101.0
251.00	226.0
265.10	511.0
266.00	98.0
266.80	114.0
279.60	91.0
281.00	6908.0
282.10	1395.0
283.00	1133.0
283.90	229.0
284.90	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

m/z	Abundance
36.00	1087.0
37.00	6225.0
38.00	5431.0
39.00	2145.0
40.00	211.0
41.00	71.0
43.10	119.0
44.00	972.0
45.00	1192.0
45.80	81.0
47.00	1185.0
48.00	704.0
49.00	4950.0
50.00	21544.0
51.00	6518.0
52.00	287.0
55.00	332.0
56.00	1960.0
57.00	2948.0
57.90	115.0
59.10	223.0
60.00	1010.0
61.00	5835.0
62.00	5438.0
63.00	4064.0
64.00	302.0
65.00	110.0
67.00	337.0
68.00	11242.0
69.00	11357.0
70.00	961.0
70.90	65.0
72.00	688.0
73.00	5781.0
74.00	18896.0
75.00	53616.0
76.00	4721.0
77.10	600.0
78.00	358.0
78.90	3489.0
80.00	988.0
80.90	3951.0
81.90	782.0
82.90	81.0
86.00	203.0
86.90	4242.0
88.00	4001.0
90.90	397.0
92.00	2559.0
93.00	4323.0
94.00	12485.0
95.00	98528.0
96.00	6593.0
96.90	242.0
102.90	317.0
103.90	520.0
104.90	192.0
105.90	392.0
106.70	79.0
109.80	222.0
111.00	137.0
112.00	127.0
113.00	81.0
114.90	232.0
115.90	344.0
117.00	652.0
117.90	400.0
118.90	741.0
123.90	71.0
125.00	337.0
125.80	131.0
127.90	316.0
128.90	180.0
129.90	376.0
130.90	187.0
132.90	948.0
133.90	233.0
134.90	300.0
135.90	60.0
136.80	168.0
140.00	51.0
140.80	875.0
141.90	126.0
142.90	934.0
143.80	76.0
144.80	104.0
145.90	115.0
146.90	157.0
147.80	230.0
148.90	142.0
149.90	98.0
154.90	336.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

156.80	265.0
158.90	152.0
160.80	206.0
163.00	244.0
164.10	71.0
164.80	169.0
168.90	101.0
170.50	56.0
171.00	63.0
172.00	209.0
173.90	71776.0
175.00	5769.0
175.90	68192.0
176.90	4639.0
178.00	213.0
179.00	290.0
189.10	52.0
190.90	968.0
192.10	250.0
192.90	1235.0
194.10	219.0
195.00	162.0
202.80	123.0
204.90	234.0
206.00	105.0
207.00	717.0
208.00	137.0
208.90	62.0
234.90	105.0
249.00	854.0
250.00	255.0
251.00	393.0
252.00	109.0
265.00	887.0
266.10	177.0
266.80	198.0
268.90	50.0
279.50	150.0
281.10	11740.0
282.00	3526.0
283.00	2213.0
284.10	433.0
285.00	125.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

m/z	Abundance
36.00	889.0
37.00	5420.0
38.00	4765.0
39.00	1845.0
40.00	290.0
41.10	106.0
43.00	195.0
44.00	810.0
45.00	1039.0
46.00	135.0
47.00	909.0
48.00	650.0
49.00	4204.0
50.00	18504.0
51.00	5899.0
51.90	268.0
55.00	308.0
56.00	1684.0
57.00	2973.0
57.90	139.0
59.00	286.0
60.00	858.0
61.00	4676.0
62.00	4380.0
63.00	3219.0
63.90	301.0
64.90	79.0
67.00	256.0
68.00	9116.0
69.00	9201.0
70.00	748.0
71.00	83.0
72.00	617.0
73.00	5740.0
74.00	15499.0
75.00	42792.0
76.00	3892.0
76.90	539.0
78.10	323.0
78.90	2788.0
79.90	792.0
80.90	3223.0
81.90	689.0
83.10	114.0
86.00	159.0
86.90	3186.0
87.90	3024.0
91.00	378.0
92.00	2526.0
92.90	3491.0
94.00	9431.0
95.00	78344.0
96.00	5157.0
97.00	166.0
102.90	367.0
103.80	454.0
104.80	218.0
105.90	389.0
106.90	90.0
109.90	102.0
110.80	171.0
112.00	142.0
112.80	110.0
115.00	162.0
115.90	297.0
116.90	619.0
118.00	510.0
118.90	700.0
123.90	56.0
125.00	466.0
125.90	209.0
127.90	252.0
128.80	142.0
129.90	347.0
130.90	182.0
132.00	93.0
132.90	1331.0
134.80	245.0
136.90	144.0
139.80	56.0
140.90	675.0
141.90	96.0
142.90	770.0
143.80	59.0
145.90	181.0
146.90	301.0
147.90	212.0
149.00	121.0
149.90	105.0
155.00	170.0
156.70	118.0
158.80	88.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

160.80	134.0
162.90	234.0
165.00	253.0
169.20	117.0
171.90	162.0
173.90	53576.0
174.90	4175.0
175.90	50208.0
176.90	3654.0
177.90	251.0
178.90	472.0
179.70	62.0
188.90	139.0
191.00	1508.0
192.00	327.0
193.00	1697.0
194.00	272.0
195.00	268.0
202.90	177.0
204.90	351.0
206.00	82.0
206.90	1002.0
208.00	286.0
209.00	117.0
221.00	56.0
234.90	129.0
249.00	1138.0
250.00	404.0
251.00	447.0
252.00	143.0
253.00	61.0
265.00	1159.0
266.00	307.0
266.90	234.0
268.00	77.0
279.20	88.0
281.00	16075.0
282.00	4768.0
283.00	2680.0
284.00	635.0
285.00	306.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

Scan 1749 (12.567 min): VW015421.D
BFB29

m/z	Abundance
39.90	184.0
41.00	74.0
42.90	88.0
44.10	298.0
55.20	53.0
69.00	77.0
169.00	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29