

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050824\
 Data File : VW028593.D
 Acq On : 08 May 2024 09:49
 Operator : SY/MD
 Sample : VW0508SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 09 00:53:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 09 00:53:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	287178	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	257652	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	113609	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	124179	22.771	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.080%
7) Chloroethane-d5	2.899	69	98602	23.614	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.440%
11) 1,1-Dichloroethene-d2	4.021	65	54877	24.086	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	96.360%
21) 2-Butanone-d5	7.075	46	63982	44.971	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.940%
24) Chloroform-d	7.648	84	219970	24.514	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.040%
26) 1,2-Dichloroethane-d4	8.227	65	47	0.009	ug/L	-0.08
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.276	84	441693	25.694	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.760%
36) 1,2-Dichloropropane-d6	9.276	67	132566	25.628	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.520%
41) Toluene-d8	10.324	98	393958	25.878	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.520%
43) trans-1,3-Dichloroprop...	10.574	79	52128	25.050	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.200%
47) 2-Hexanone-d5	10.922	63	42614	47.765	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.520%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	103430	23.845	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	13.848	152	118080	27.269	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.080%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	4.015	101	1604	0.364	ug/L #	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050824\
Data File : VW028593.D
Acq On : 08 May 2024 09:49
Operator : SY/MD
Sample : VW0508SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 09 00:53:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 09 00:53:18 2024
Response via : Initial Calibration

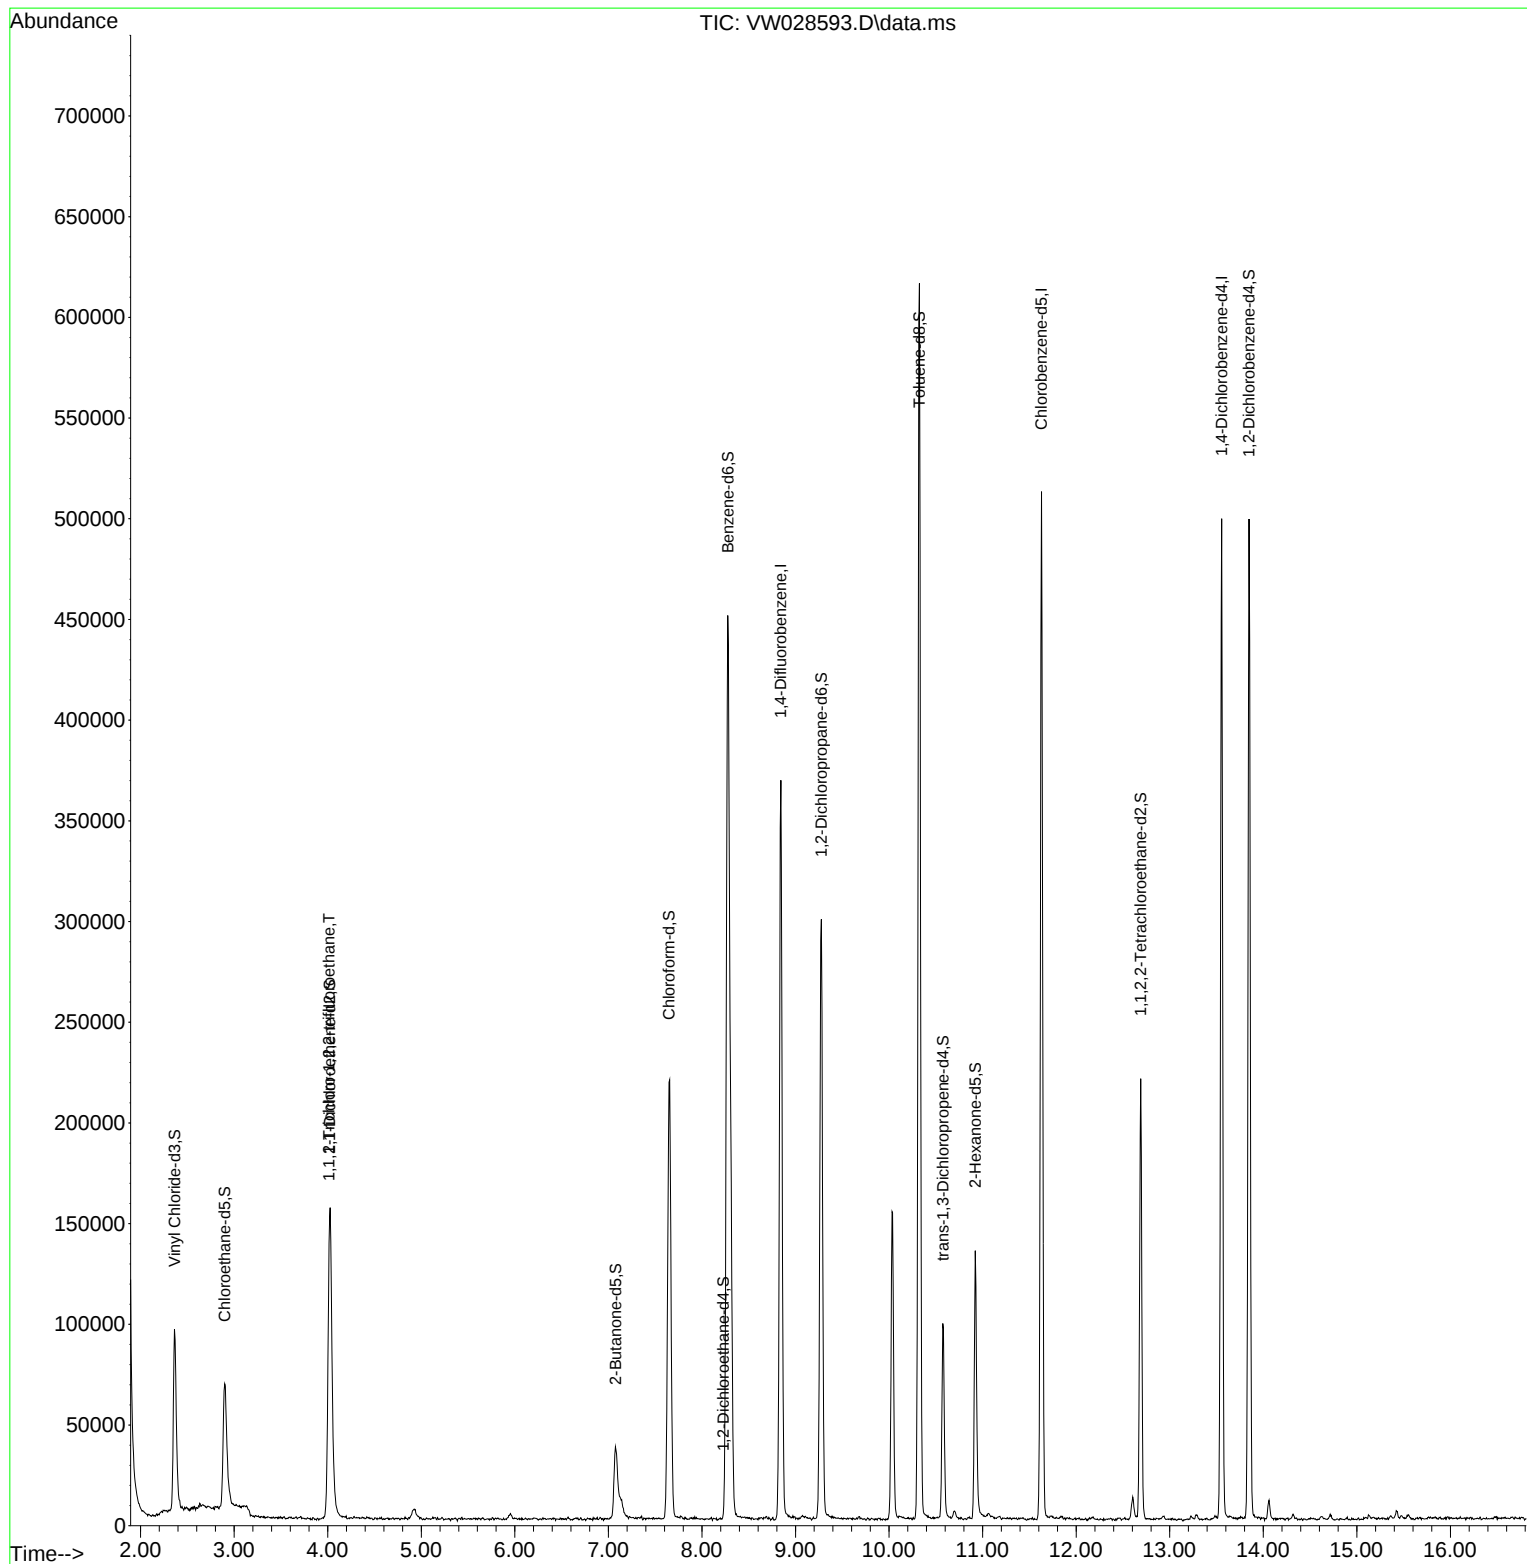

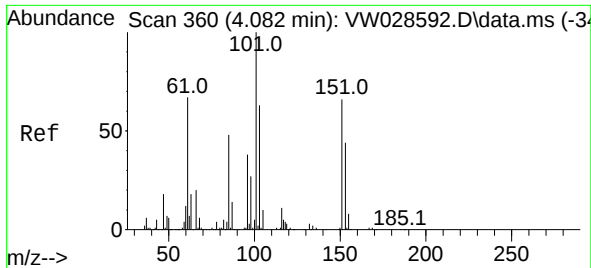

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.364 ug/L
 RT: 4.015 min Scan# 349
 Delta R.T. -0.067 min
 Lab File: VW028593.D
 Acq: 08 May 2024 09:49

Instrument :
 MSVOA_W
 ClientSampleId :

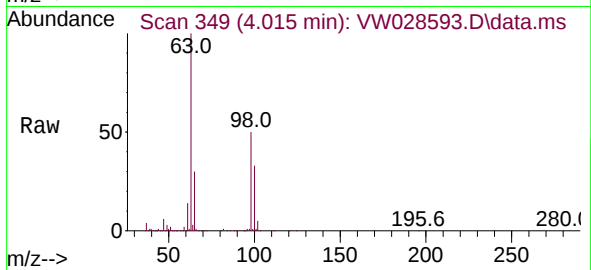

Tgt Ion:	101	Resp:	1604
Ion	Ratio	Lower	Upper
101	100		
85	1.5	35.8	53.8#
151	2.7	49.6	74.4#

