

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050923\
 Data File : VW025898.D
 Acq On : 09 May 2023 11:16
 Operator : SY/MD
 Sample : 02612-30
 Misc : 4.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JREH1

Quant Time: May 09 23:19:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1017112	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	882661	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	391242	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	286899	19.905	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.640%
7) Chloroethane-d5	2.899	69	226671	21.213	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.840%
11) 1,1-Dichloroethene-d2	4.021	65	141894	19.661	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.640%
21) 2-Butanone-d5	7.075	46	170348	35.751	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.500%
24) Chloroform-d	7.648	84	587906	20.046	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.200%
26) 1,2-Dichloroethane-d4	8.307	65	328755	19.823	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.280%
32) Benzene-d6	8.276	84	1215493	21.075	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.280%
36) 1,2-Dichloropropane-d6	9.276	67	392278	21.258	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.040%
41) Toluene-d8	10.325	98	1054292	20.500	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.000%
43) trans-1,3-Dichloroprop...	10.575	79	143805	19.225	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.920%
47) 2-Hexanone-d5	10.922	63	110822	35.219	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.440%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	277090	19.701	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	78.800%
66) 1,2-Dichlorobenzene-d4	13.848	152	316525	22.193	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.760%
Target Compounds					Qvalue	
13) Acetone	4.125	43	13356	3.161	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050923\
Data File : VW025898.D
Acq On : 09 May 2023 11:16
Operator : SY/MD
Sample : 02612-30
Misc : 4.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JREH1

Quant Time: May 09 23:19:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 05 23:47:36 2023
Response via : Initial Calibration

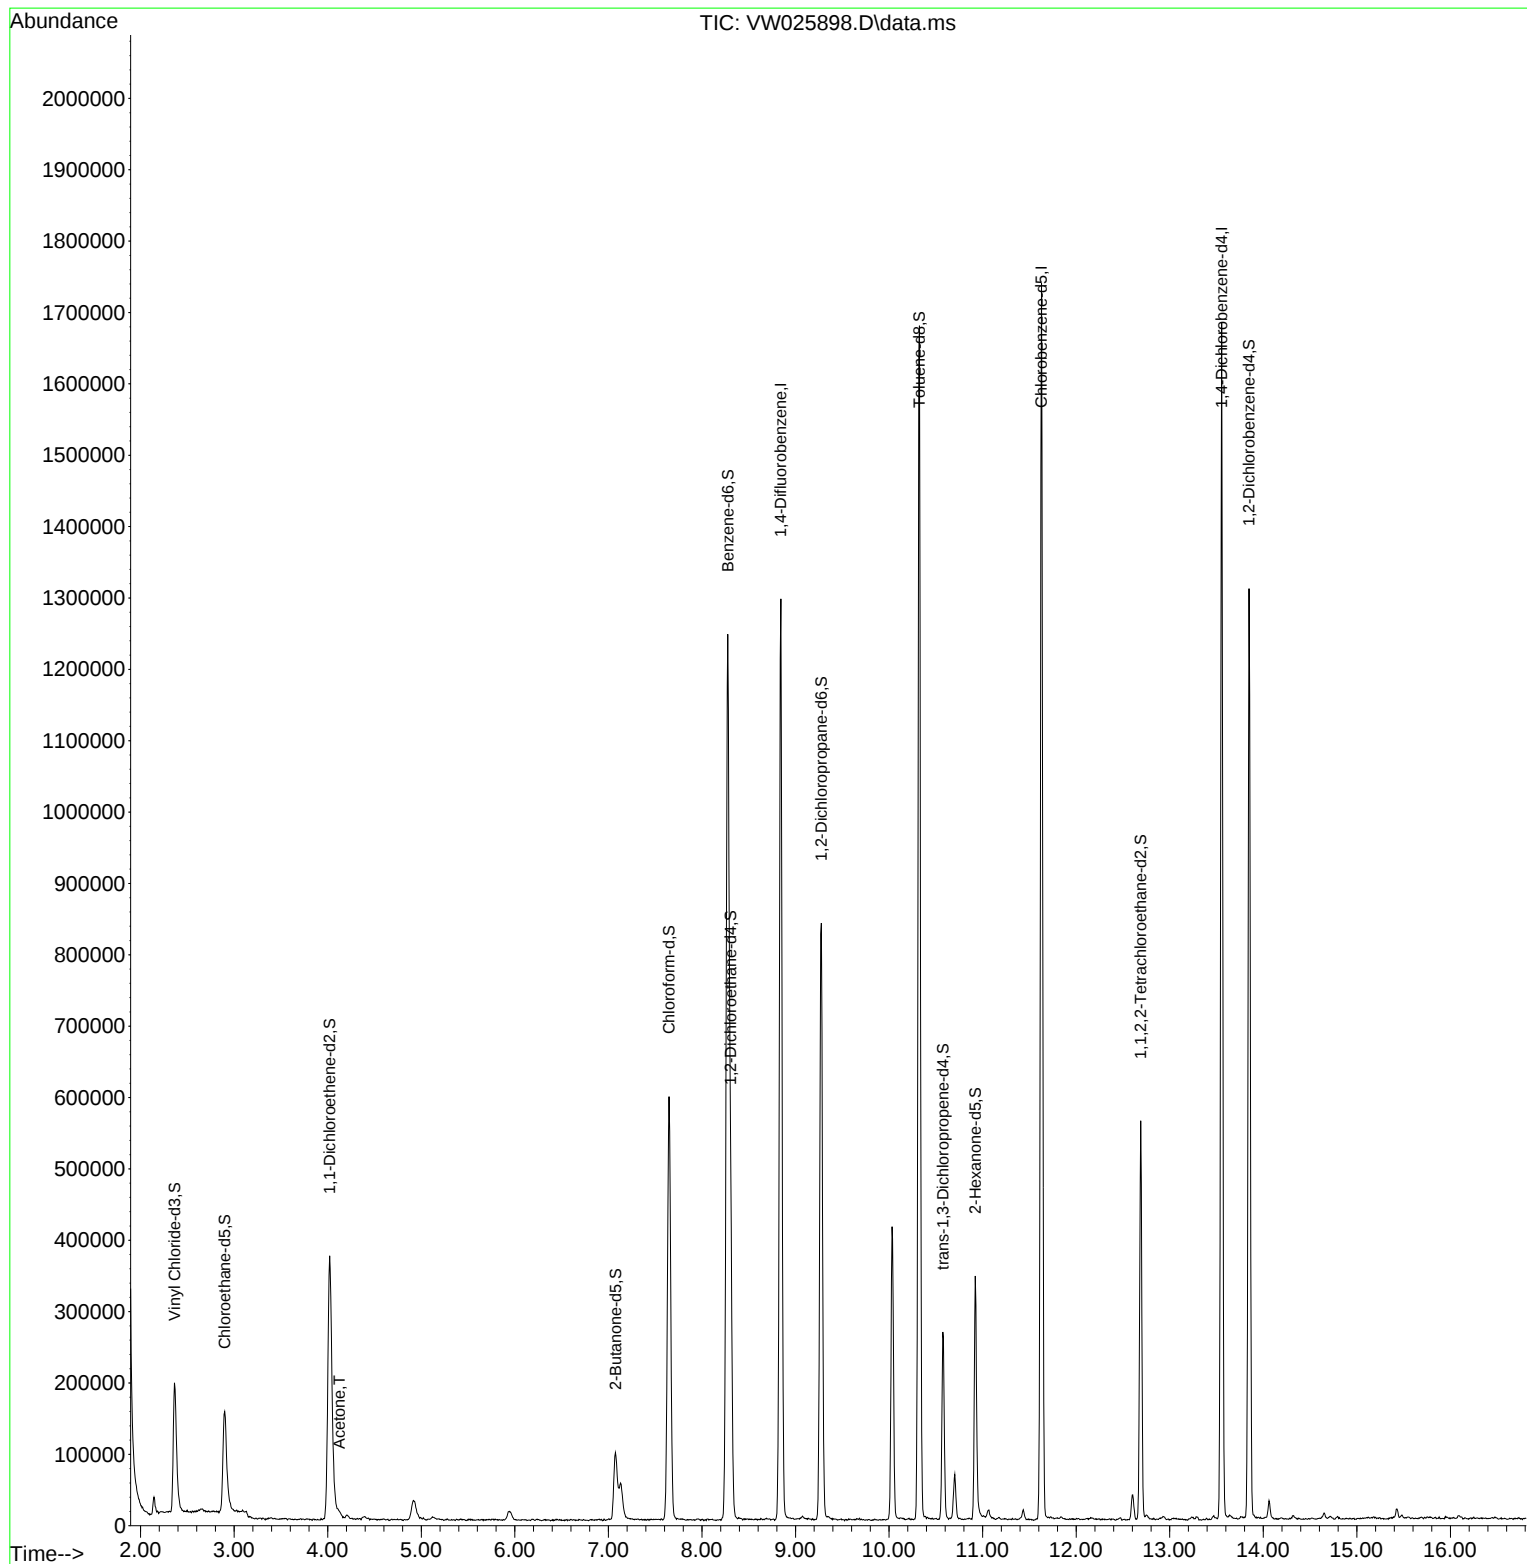

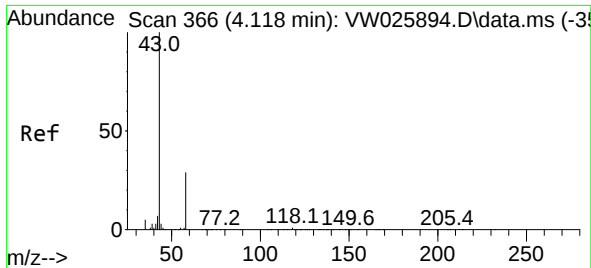

#13
 Acetone
 Concen: 3.161 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025898.D
 Acq: 09 May 2023 11:16

Instrument :
 MSVOA_W
 ClientSampleId :
 JREH1

Tgt Ion: 43 Resp: 13356
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 58.2

