

Data Path : W:\HPCHEM1\MSVOA W\DATA\VW051018\
 Data File : VW002403.D
 Acq On : 11 May 2018 02:29
 Operator : JC/SY
 Sample : J2822-03
 Misc : 5.26G/5ML/MSVOA W/SOIL
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB01-01

Quant Time: May 11 15:02:43 2018
 Quant Method : W:\HPCHEM1\MSVOA_W\METHOD\82W050818S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 08 03:57:58 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	86827	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	125809	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	109768	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	54263	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	37894	41.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	82.20%	
35) Dibromofluoromethane	7.88	113	36471	45.23	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.46%	
50) Toluene-d8	10.33	98	121765	39.60	ug/l	0.00
Spiked Amount 50.000			Recovery	=	79.20%	
62) 4-Bromofluorobenzene	12.63	95	42567	38.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	76.62%	
Target Compounds						
16) Acetone	4.13	43	5133	28.51	ug/l	95
20) Methylene Chloride	4.90	84	11523	13.27	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA W\DATA\VW051018\
Data File : VW002403.D
Acq On : 11 May 2018 02:29
Operator : JC/SY
Sample : J2822-03
Misc : 5.26G/5ML/MSVOA W/SOIL
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB01-01

Quant Time: May 11 15:02:43 2018
Quant Method : W:\HPCHEM1\MSVOA_W\METHOD\82W050818S.M
Quant Title : SW846 8260
QLast Update : Tue May 08 03:57:58 2018
Response via : Initial Calibration

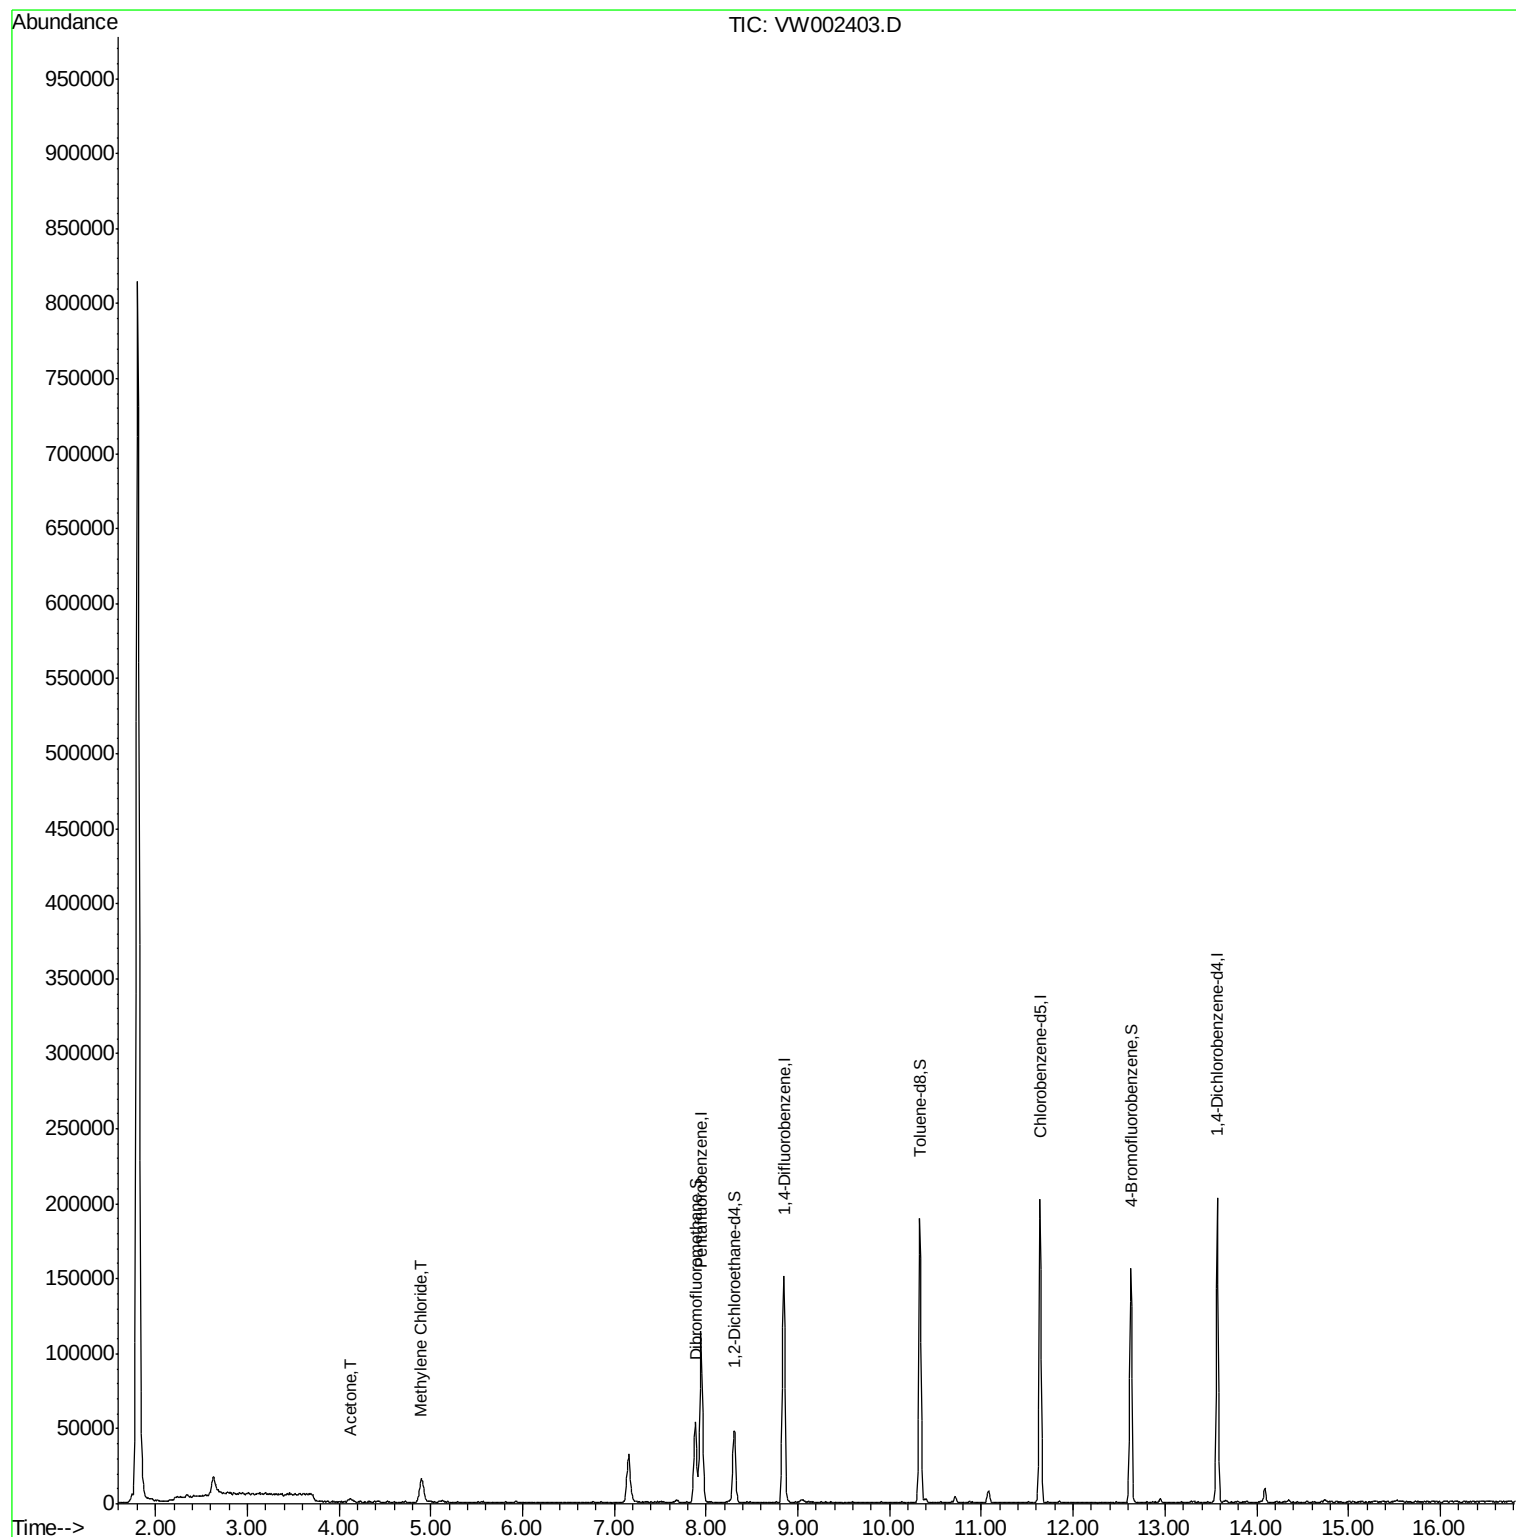



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.95 min Scan# 1043

Delta R.T. -0.00 min

Lab File: VW002403.D

Acq: 11 May 2018 02:29

Instrument :

MSVOA_W

ClientSampled :


SB01-01

Tot Ion:168 Resp: 86827

Ion Ratio Lower Upper




168 100

99 53.5 43.7 65.5

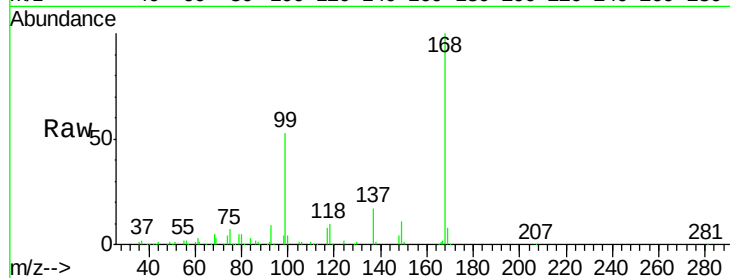

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

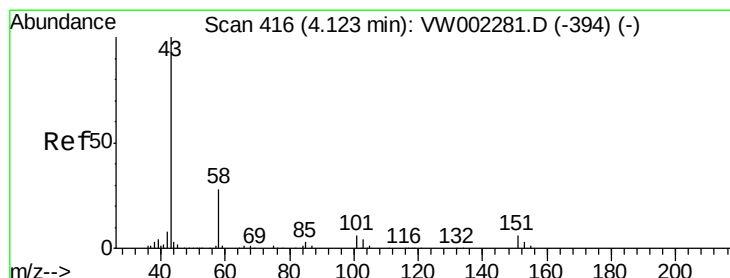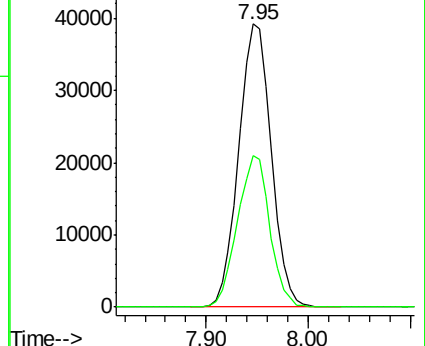

#16

Acetone

Concen: 28.51 ug/l

RT: 4.13 min Scan# 417

Delta R.T. 0.01 min

Lab File: VW002403.D


Acq: 11 May 2018 02:29

Tgt Ion: 43 Resp: 5133

Ion Ratio Lower Upper



43 100


58 25.2 22.2 33.4

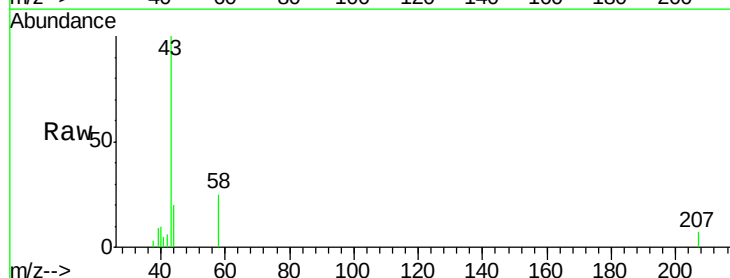

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

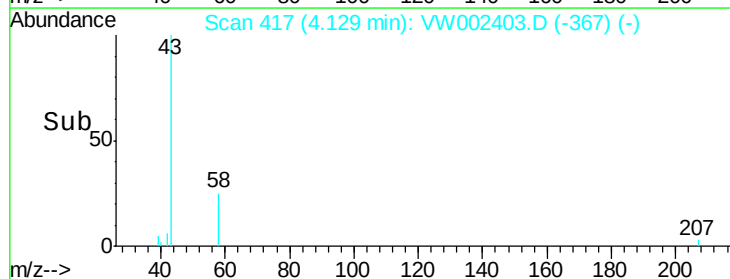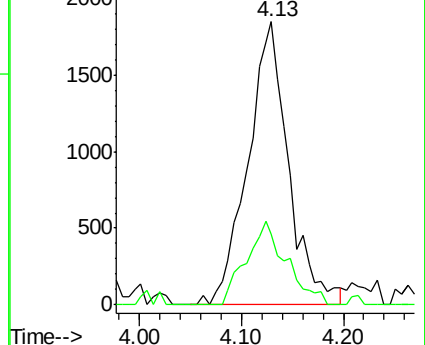







#20
Methylene Chloride
Concen: 13.27 ug/l
RT: 4.90 min Scan# 543
Delta R.T. -0.01 min
Lab File: VW002403.D
Acq: 11 May 2018 02:29

Instrument :
MSVOA_W
ClientSampleId :
SB01-01

Tot Ion: 84 Resp: 11523
Ion Ratio Lower Upper
84 100
49 128.5 97.7 146.5
51 36.1 30.2 45.4
86 62.1 48.9 73.3

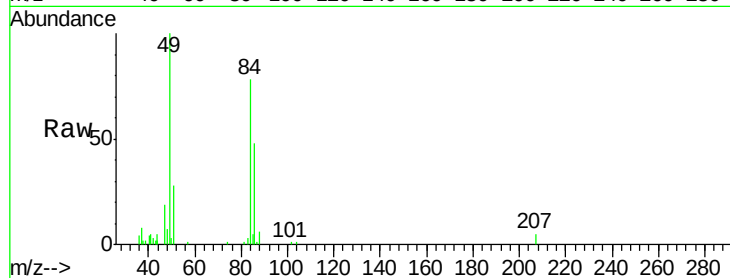


Abundance Ion 83.90 (83.60 to 84.60): VW
Ion 48.90 (48.60 to 49.60): VW
Ion 50.90 (50.60 to 51.60): VW
Ion 85.90 (85.60 to 86.60): VW

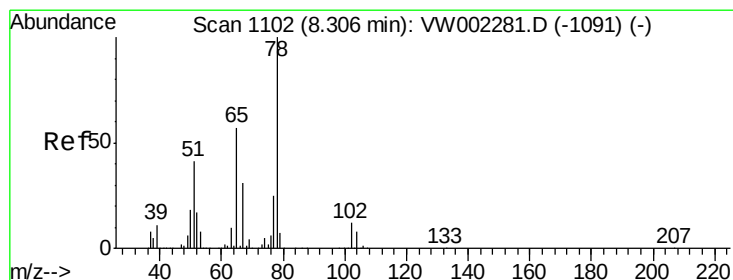
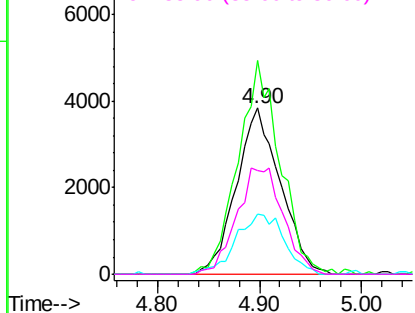



#33
1,2-Dichloroethane-d4
Concen: 41.10 ug/l
RT: 8.31 min Scan# 1103
Delta R.T. 0.01 min
Lab File: VW002403.D
Acq: 11 May 2018 02:29

Tgt Ion: 65 Resp: 37894
Ion Ratio Lower Upper
65 100
67 52.7 0.0 107.2

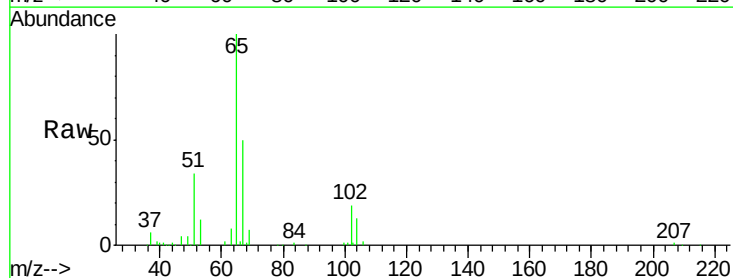

Abundance Ion 64.90 (64.60 to 65.60): VW
Ion 66.90 (66.60 to 67.60): VW

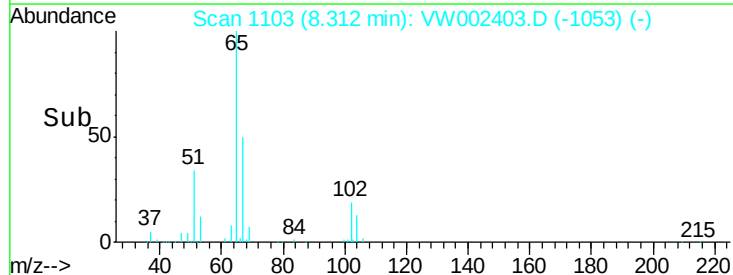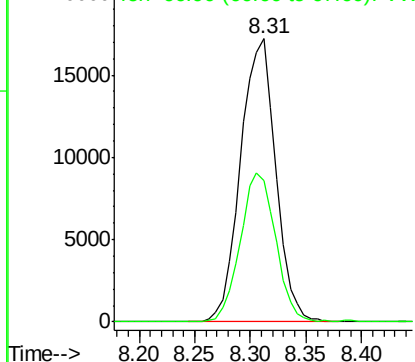




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.85 min Scan# 1191
 Delta R.T. 0.00 min
 Lab File: VW002403.D
 Acq: 11 May 2018 02:29

Instrument :
 MSVOA_W
 ClientSampleId :
 SB01-01




Tot Ion	Ratio	Lower	Upper
114	100		
63	19.2	0.0	39.0
88	14.4	0.0	29.6

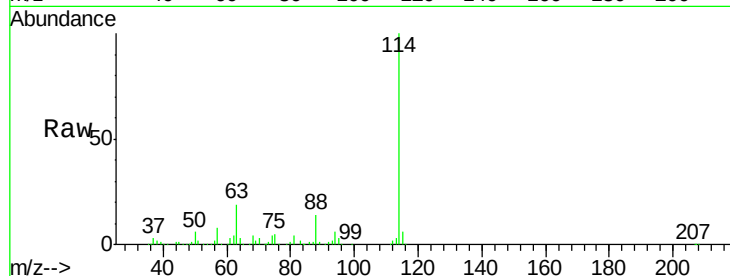

Abundance Ion 113.90 (113.60 to 114.60): V


Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

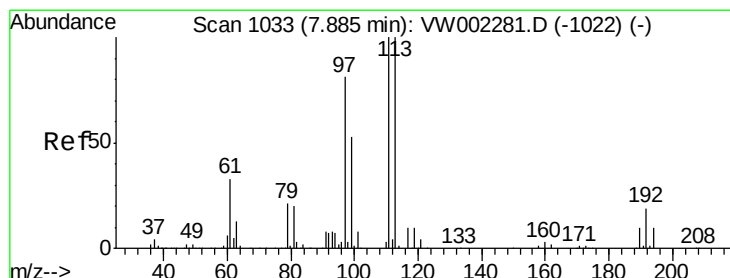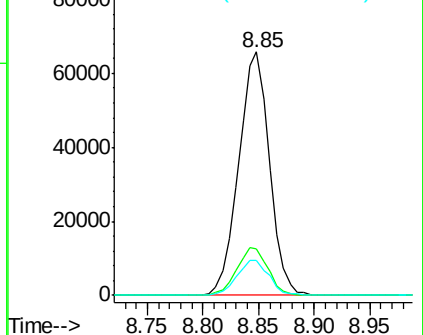

#35
 Dibromofluoromethane
 Concen: 45.23 ug/l
 RT: 7.88 min Scan# 1033
 Delta R.T. 0.00 min
 Lab File: VW002403.D
 Acq: 11 May 2018 02:29



Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.8	81.5	122.3
192	21.5	16.4	24.6

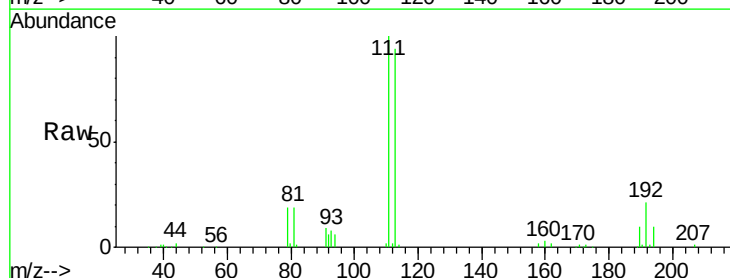


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

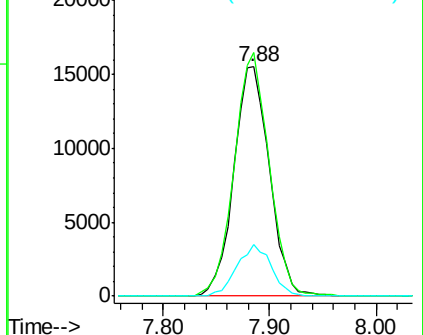



#50

Toluene-d8

Concen: 39.60 ug/l

RT: 10.33 min Scan# 1434

Delta R.T. -0.00 min

Lab File: VW002403.D

Acq: 11 May 2018 02:29

Instrument :

MSVOA_W

ClientSampleId :





SB01-01

Tot Ion: 98 Resp: 121765

Ion Ratio Lower Upper

98 100

100 64.6 51.4 77.2

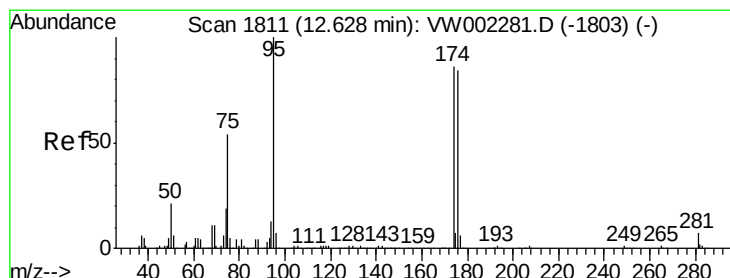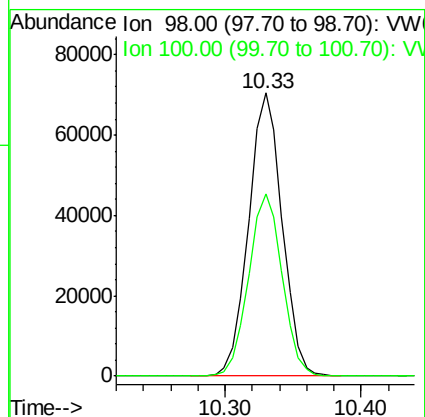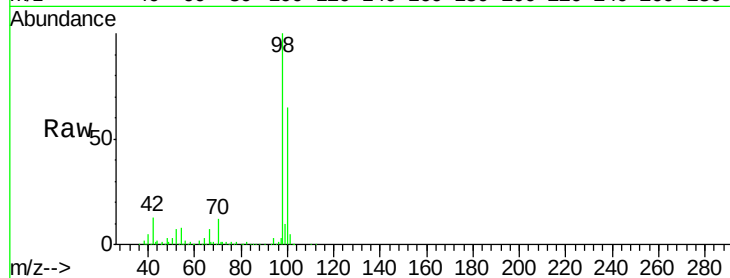

#62

4-Bromofluorobenzene

Concen: 38.31 ug/l

RT: 12.63 min Scan# 1811

Delta R.T. 0.00 min

Lab File: VW002403.D

Acq: 11 May 2018 02:29




Tgt Ion: 95 Resp: 42567


Ion Ratio Lower Upper

95 100

174 90.2 0.0 176.8

176 86.5 0.0 170.4



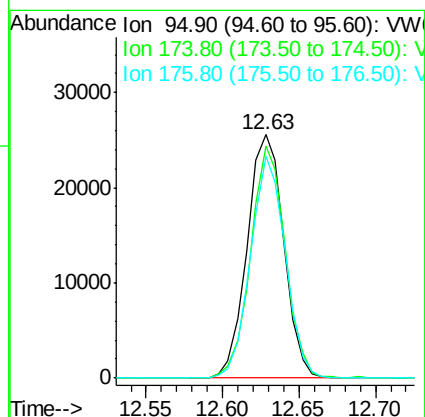
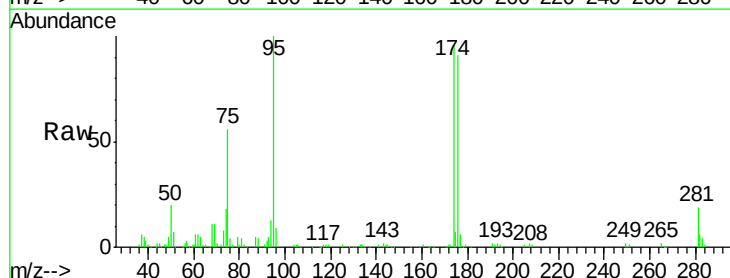


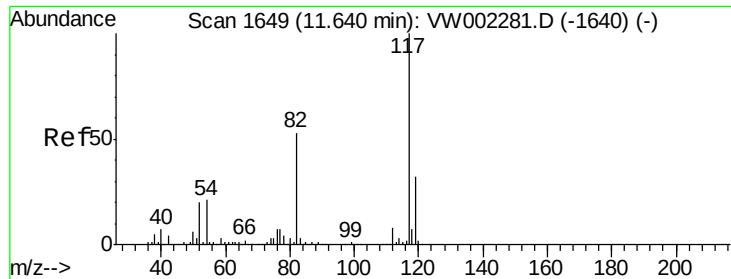

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.64 min Scan# 1649
Delta R.T. 0.00 min
Lab File: VW002403.D
Acq: 11 May 2018 02:29

Instrument :
MSVOA_W
ClientSampled :
SB01-01

Tot Ion:117 Resp: 109768
Ion Ratio Lower Upper
117 100
82 50.9 42.6 63.8
119 33.0 25.2 37.8

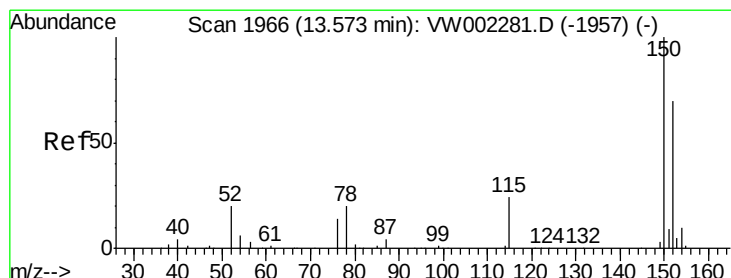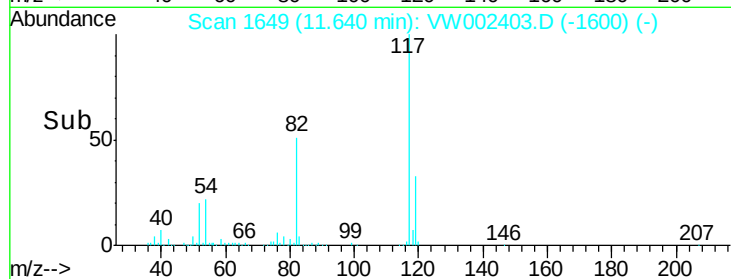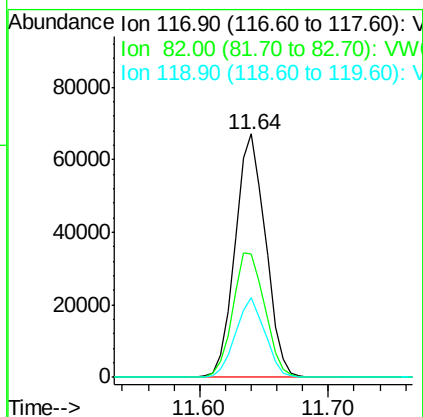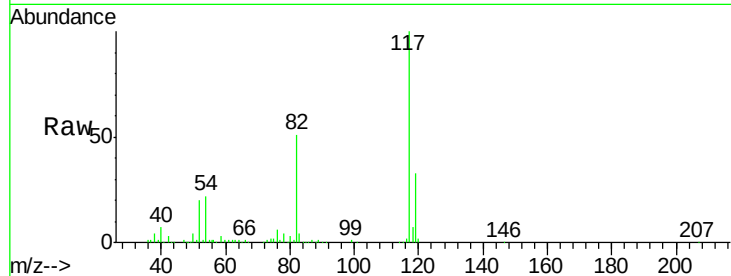

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.57 min Scan# 1966
Delta R.T. 0.00 min
Lab File: VW002403.D
Acq: 11 May 2018 02:29

Tgt Ion:152 Resp: 54263
Ion Ratio Lower Upper
152 100
115 55.5 28.5 85.5
150 154.7 0.0 342.6

