


Data Path : W:\HPCHEM1\MSVOA W\Data\VW051018\
Data File : VW002396.D
Acq On : 10 May 2018 22:43
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_W\METHOD\82W050818S.M
Title : SW846 8260
Last Update : Tue May 08 03:57:58 2018

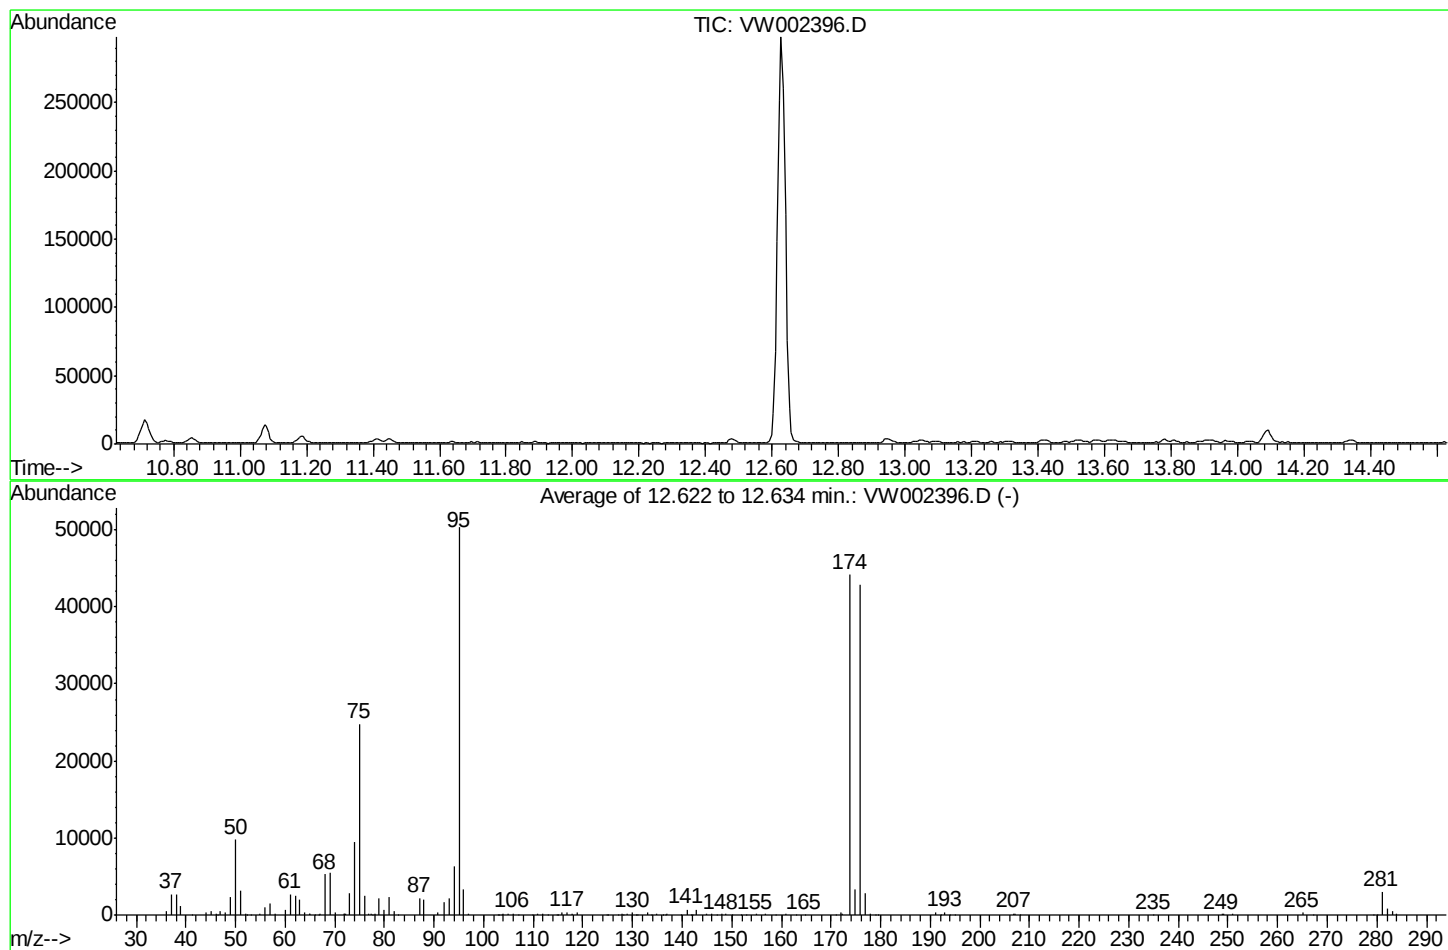

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	9782	PASS
75	95	30	60	49.2	24778	PASS
95	95	100	100	100.0	50328	PASS
96	95	5	9	6.6	3307	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.8	44189	PASS
175	174	5	9	7.6	3342	PASS
176	174	95	101	97.0	42877	PASS
177	176	5	9	6.8	2907	PASS