

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051021\
 Data File : VW018967.D
 Acq On : 10 May 2021 10:42
 Operator : SY/VA
 Sample : M2272-09
 Misc : 5.03G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual Integrations
 APPROVED

MMDadoda
 5/11/2021 1:05:11 PM

Quant Time: May 11 01:27:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 11 01:26:53 2021
 Response via : Initial Calibration

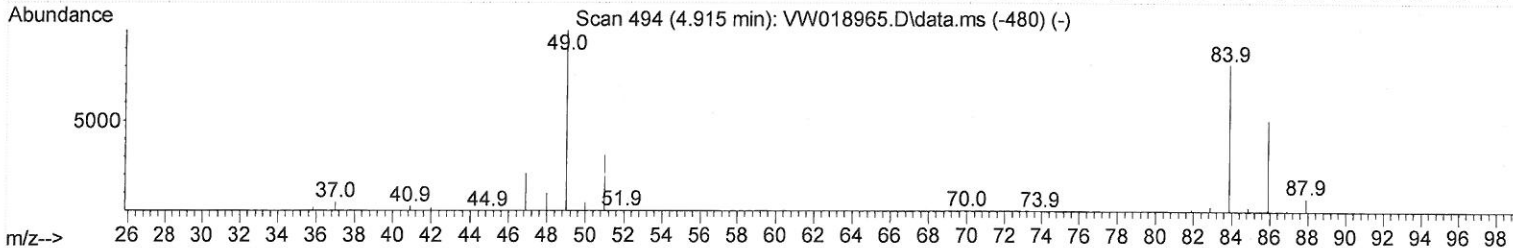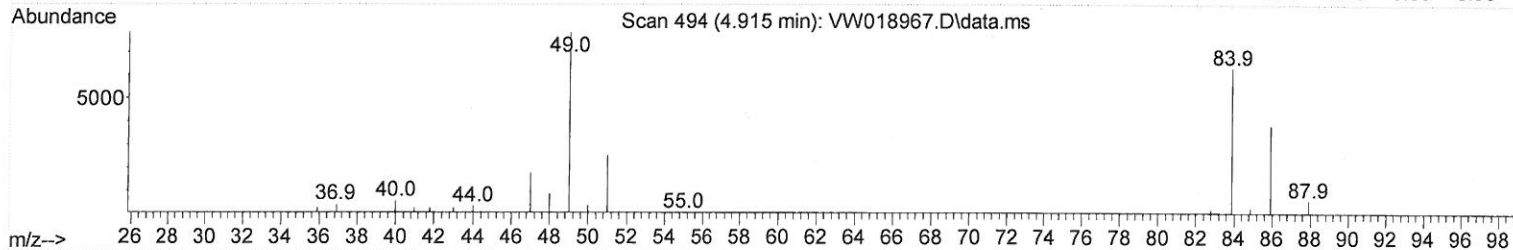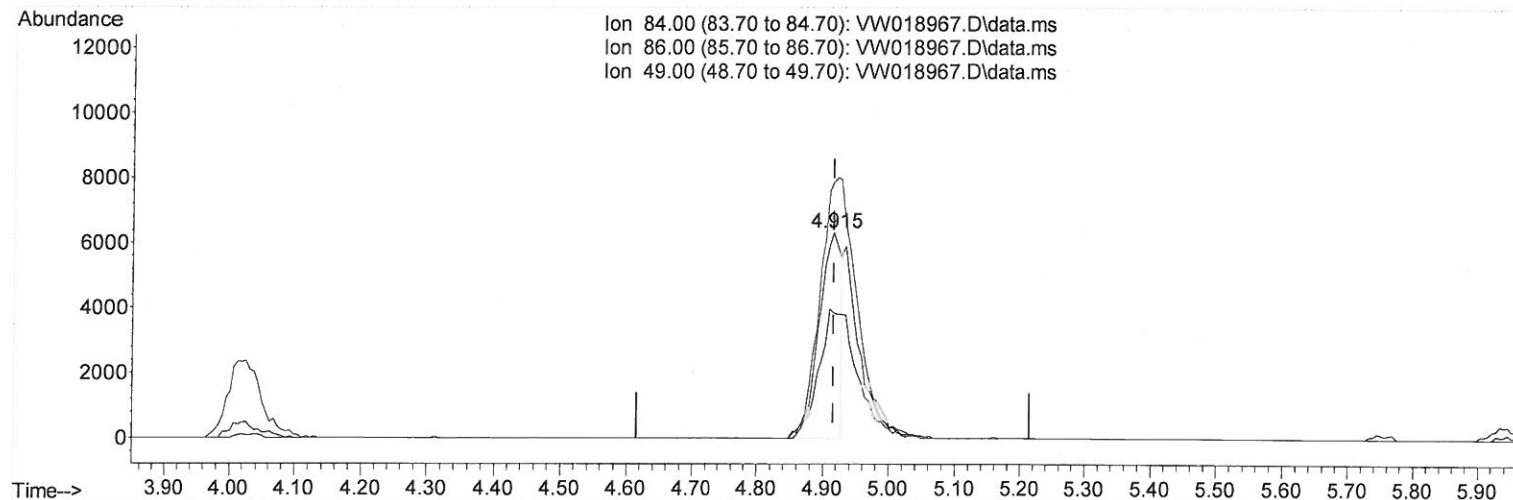

TIC: VW018967.D\data.ms

(16) Methylene chloride (T)

4.915min (0.000) 1.44 ug/L

response 14954

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	60.96
49.00	123.70	124.28
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051021\
Data File : VW018967.D
Acq On : 10 May 2021 10:42
Operator : SY/VA
Sample : M2272-09
Misc : 5.03G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual Integrations
APPROVED

MMDadoda
5/11/2021 1:05:11 PM

Quant Time: May 11 01:27:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 11 01:26:53 2021
Response via : Initial Calibration

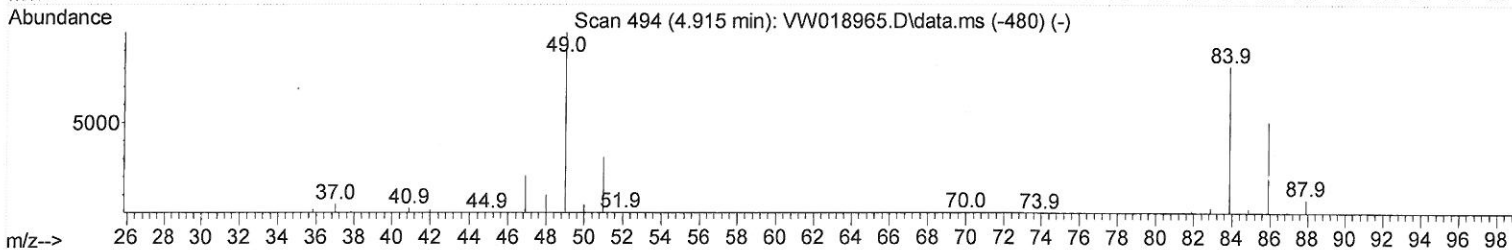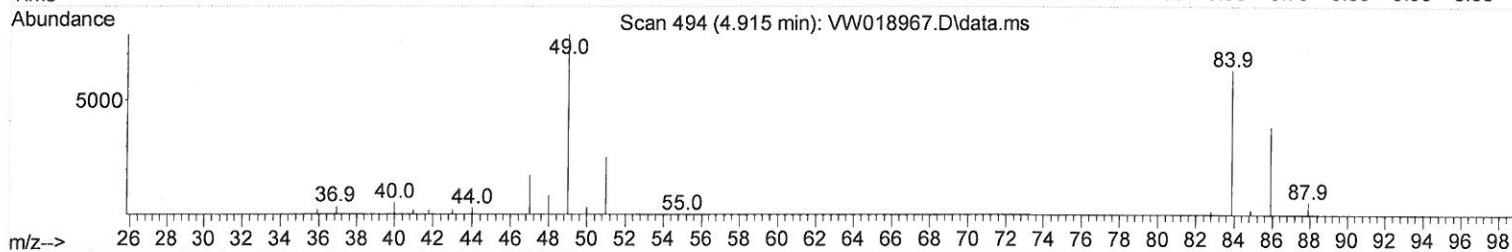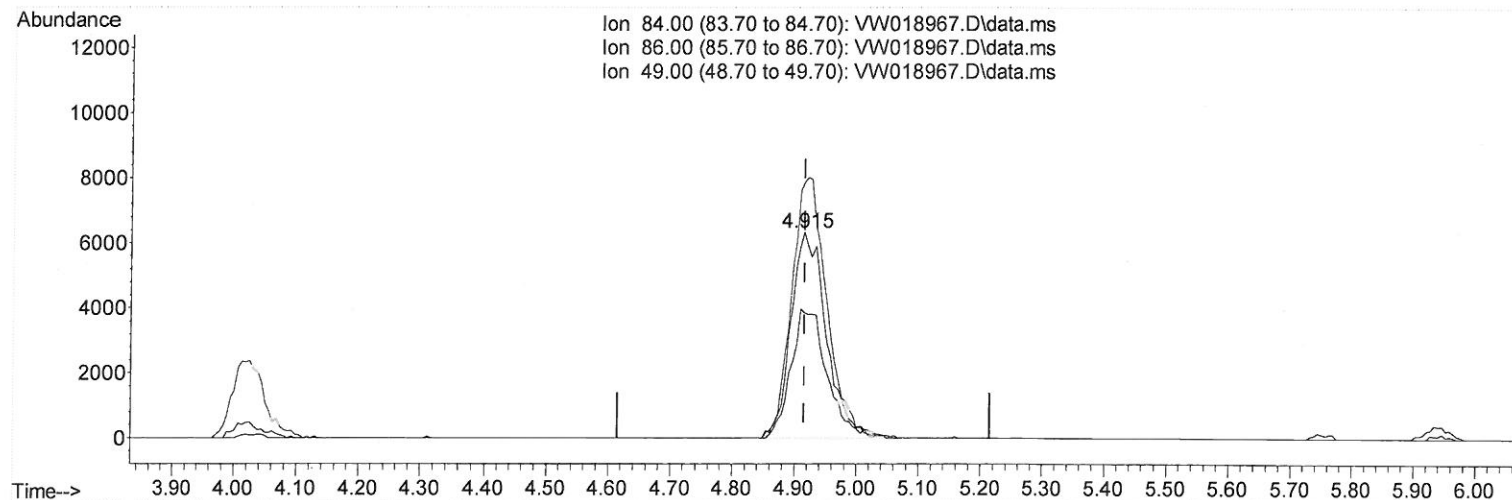

TIC: VW018967.D\data.ms

(16) Methylene chloride (T)

4.915min (0.000) 2.40 ug/L m

response 25010

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	60.96
49.00	123.70	124.28
0.00	0.00	0.00

05/11/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051021\
 Data File : VW018967.D
 Acq On : 10 May 2021 10:42
 Operator : SY/VA
 Sample : M2272-09
 Misc : 5.03G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual Integrations
 APPROVED

MMDadoda
 5/11/2021 1:05:11 PM

Quant Time: May 11 01:27:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 11 01:26:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	629484	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	584104	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	279073	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	161298	19.97	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 79.88%			
7) Chloroethane-d5	2.891	69	133916	21.40	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 85.60%			
11) 1,1-Dichloroethene-d2	4.019	63	282551	17.62	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 70.48%			
21) 2-Butanone-d5	7.074	46	119752	56.94	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 113.88%			
24) Chloroform-d	7.647	84	433593	26.24	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 104.96%			
26) 1,2-Dichloroethane-d4	8.305	65	256794	27.83	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 111.32%			
32) Benzene-d6	8.275	84	817397	24.77	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 99.08%			
36) 1,2-Dichloropropane-d6	9.274	67	251148	25.65	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 102.60%			
41) Toluene-d8	10.323	98	751909	24.43	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 97.72%			
43) trans-1,3-Dichloroprop...	10.579	79	108139	24.30	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 97.20%			
47) 2-Hexanone-d5	10.927	63	92377	52.70	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 105.40%			
56) 1,1,2,2-Tetrachloroeth...	12.694	84	208102	25.08	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 100.32%			
66) 1,2-Dichlorobenzene-d4	13.853	152	244474	25.57	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 102.28%			
Target Compounds						
16) Methylene chloride	4.915	84	25010m	2.40	ug/L	Qvalue
42) Toluene	10.390	91	12921	0.34	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051021\
Data File : VW018967.D
Acq On : 10 May 2021 10:42
Operator : SY/VA
Sample : M2272-09
Misc : 5.03G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual Integrations
APPROVED

MMDadoda
5/11/2021 1:05:11 PM

Quant Time: May 11 01:27:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042921SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 11 01:26:53 2021
Response via : Initial Calibration

