




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
 Data File : VW022946.D
 Acq On : 10 May 2022 11:05
 Operator : SY/VA
 Sample : N2714-08RE
 Misc : 6.51g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 11 01:20:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 11 01:19:10 2022
 Response via : Initial Calibration

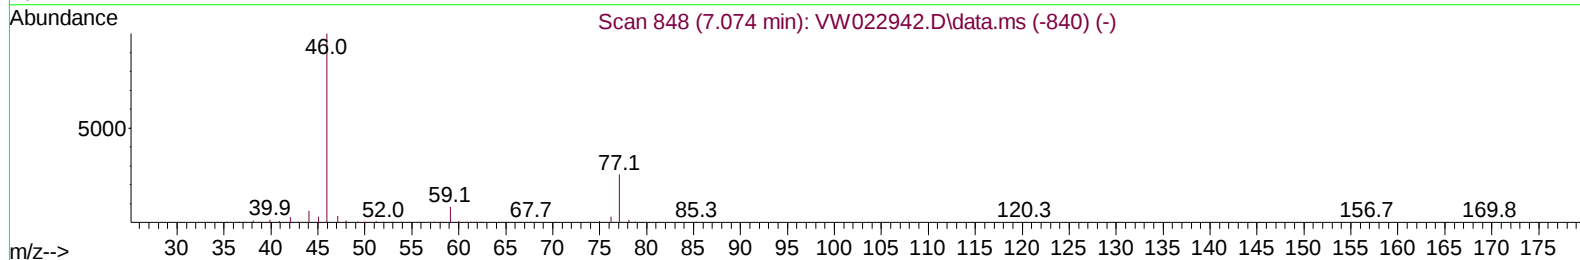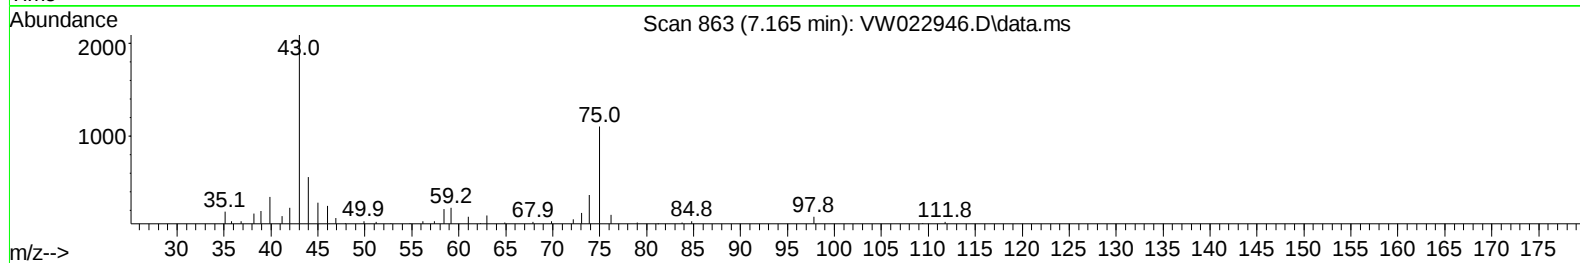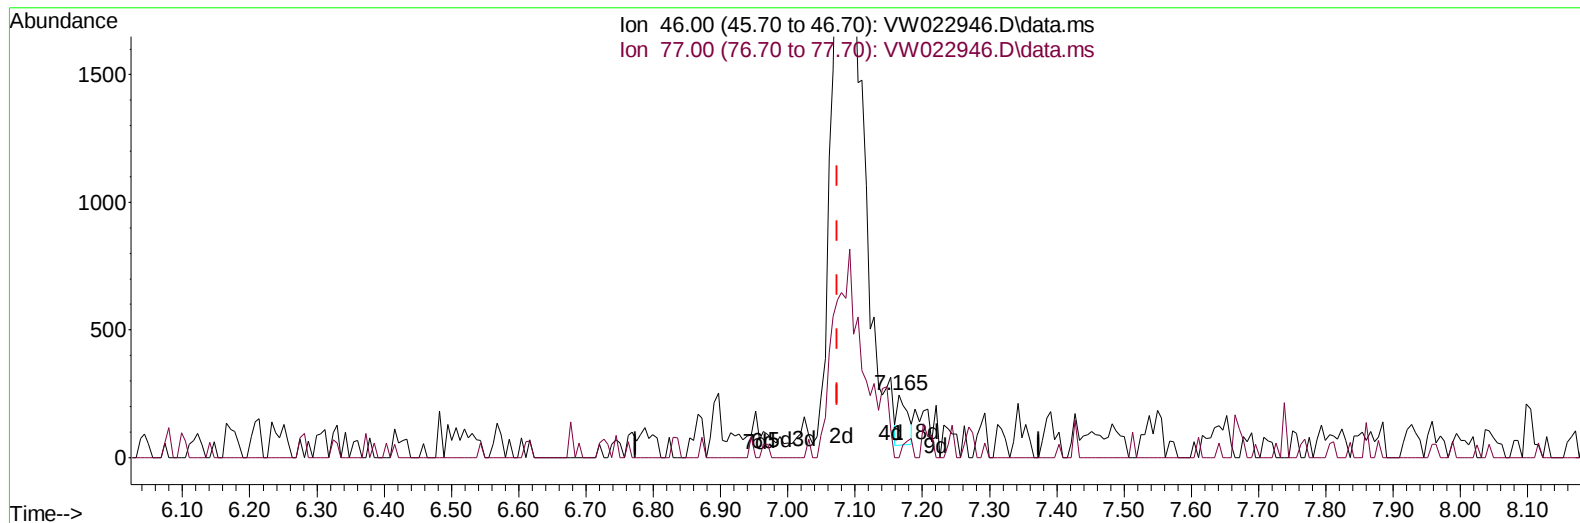

TIC: VW022946.D\data.ms

(21) 2-Butanone-d5 (S)

7.165min (+ 0.092) 0.15 ug/L

response 205

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	33.66
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
 Data File : VW022946.D
 Acq On : 10 May 2022 11:05
 Operator : SY/VA
 Sample : N2714-08RE
 Misc : 6.51g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X9RE

Manual IntegrationsAPPROVED

Quant Time: May 11 01:20:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 11 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/11/2022
 Supervised By :Mahesh Dadoda 05/16/2022

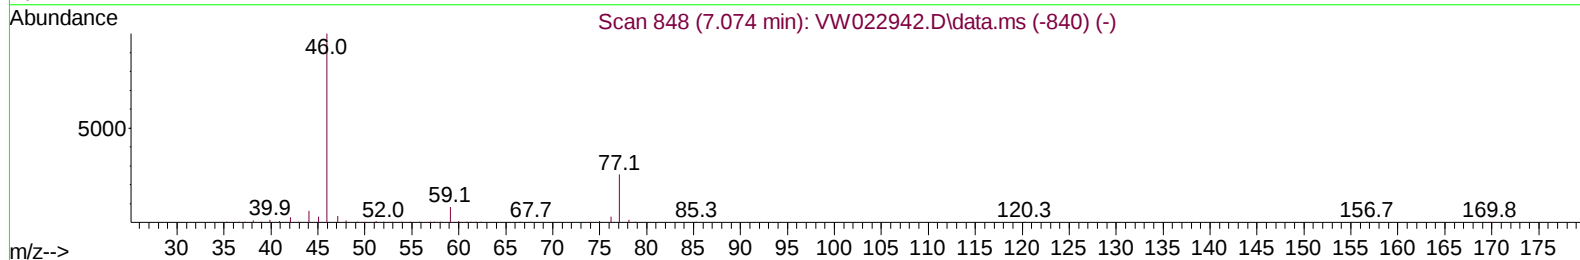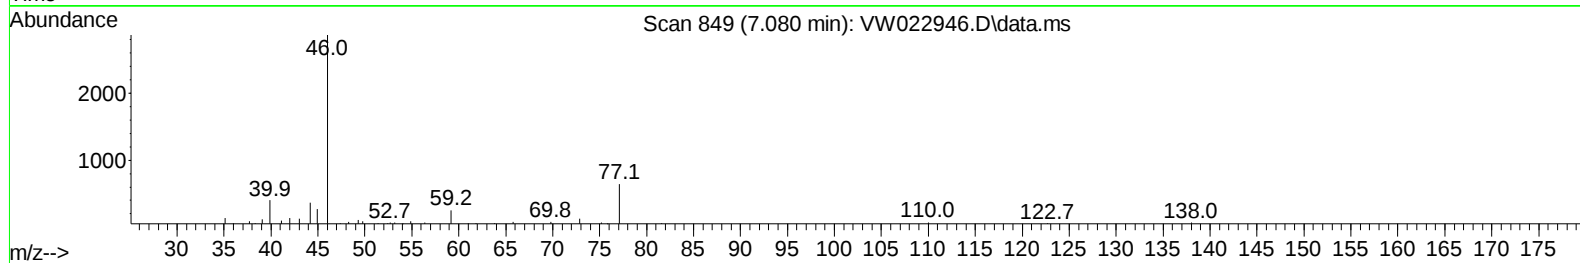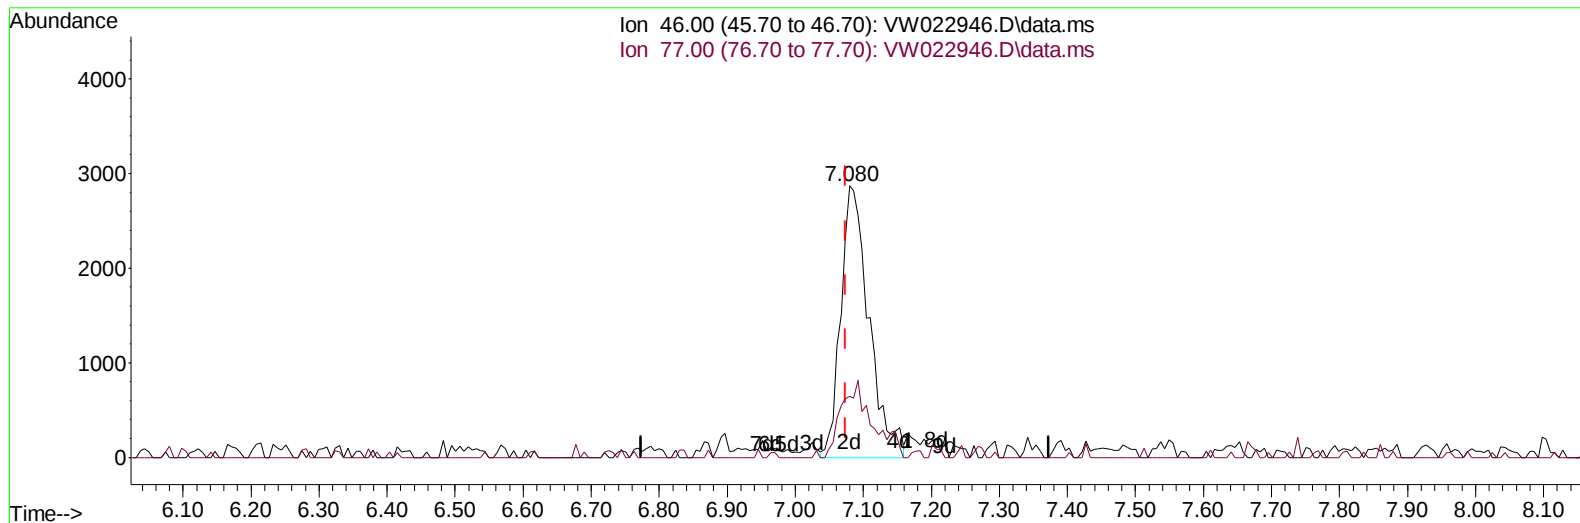

TIC: VW022946.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 5.98 ug/L m

response 8216

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.84#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
 Data File : VW022946.D
 Acq On : 10 May 2022 11:05
 Operator : SY/VA
 Sample : N2714-08RE
 Misc : 6.51g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 11 01:20:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 11 01:19:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	352229	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	305436	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	109948	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	90955	12.586	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	50.360%	
7) Chloroethane-d5	2.885	69	86258	18.347	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	73.400%	
11) 1,1-Dichloroethene-d2	4.013	63	104654	11.208	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	44.840%#	
21) 2-Butanone-d5	7.080	46	8216m	5.980	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	11.960%#	
24) Chloroform-d	7.647	84	187279	18.148	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	72.600%	
26) 1,2-Dichloroethane-d4	8.305	65	107478	18.990	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	75.960%	
32) Benzene-d6	8.275	84	332813	18.904	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	75.600%	
36) 1,2-Dichloropropane-d6	9.275	67	108596	21.959	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	87.840%	
41) Toluene-d8	10.323	98	274019	16.112	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	64.440%	
43) trans-1,3-Dichloroprop...	10.579	79	13508	5.932	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	23.720%#	
47) 2-Hexanone-d5	10.927	63	6184	6.550	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	13.100%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	81601	17.703	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	70.800%	
66) 1,2-Dichlorobenzene-d4	13.853	152	71066	18.490	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	73.960%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
Data File : VW022946.D
Acq On : 10 May 2022 11:05
Operator : SY/VA
Sample : N2714-08RE
Misc : 6.51g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW2X9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 11 01:20:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 11 01:19:10 2022
Response via : Initial Calibration

